

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048217.D
 Acq On : 22 Apr 2022 12:06
 Operator : SY/MD
 Sample : VIBLK065
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	104	rBV	163543	194196	16.38%	2.046%
2	1.916	171	179	201	rVB	119449	167429	14.13%	1.764%
3	2.568	369	382	398	rBV	261795	432043	36.45%	4.551%
4	2.752	436	439	444	rBV4	309	368	0.03%	0.004%
5	2.957	500	503	506	rVV4	468	423	0.04%	0.004%
6	3.051	522	532	542	rBV3	5021	9133	0.77%	0.096%
7	3.192	563	576	595	rVB2	3307	8006	0.68%	0.084%
8	3.263	595	598	601	rBV	275	191	0.02%	0.002%
9	3.302	606	610	613	rBV2	251	199	0.02%	0.002%
10	3.443	651	654	657	rVV2	330	247	0.02%	0.003%
11	3.488	663	668	670	rBV	243	190	0.02%	0.002%
12	3.562	687	691	696	rBV	230	222	0.02%	0.002%
13	3.652	716	719	724	rVB2	410	327	0.03%	0.003%
14	3.697	728	733	736	rBV2	271	235	0.02%	0.002%
15	3.967	812	817	824	rVV3	269	313	0.03%	0.003%
16	4.038	835	839	844	rBV	158	190	0.02%	0.002%
17	4.060	844	846	849	rBV2	355	240	0.02%	0.003%
18	4.179	877	883	887	rBV3	261	265	0.02%	0.003%
19	4.546	994	997	1000	rBV2	256	209	0.02%	0.002%
20	4.626	1009	1022	1053	rBV	123213	315941	26.65%	3.328%
21	4.842	1087	1089	1096	rVB5	481	338	0.03%	0.004%
22	4.903	1106	1108	1113	rVB2	277	196	0.02%	0.002%
23	5.067	1138	1159	1180	rBV	207989	459477	38.76%	4.840%
24	5.240	1209	1213	1215	rVB2	291	200	0.02%	0.002%
25	5.272	1220	1223	1226	rVV3	355	303	0.03%	0.003%
26	5.289	1226	1228	1235	rVB3	551	665	0.06%	0.007%
27	5.334	1235	1242	1244	rBV2	153	179	0.02%	0.002%
28	5.385	1256	1258	1264	rVB2	306	179	0.02%	0.002%
29	5.729	1342	1365	1398	rBV2	434041	1185298	100.00%	12.487%
30	6.250	1511	1527	1547	rBV	374486	717148	60.50%	7.555%
31	6.475	1592	1597	1600	rBV3	289	329	0.03%	0.003%
32	6.533	1607	1615	1624	rVB6	1773	2812	0.24%	0.030%
33	6.571	1624	1627	1630	rBV	443	318	0.03%	0.003%
34	6.594	1631	1634	1641	rVB3	431	420	0.04%	0.004%
35	6.694	1649	1665	1692	rBV	267552	527336	44.49%	5.555%
36	6.809	1695	1701	1710	rVV3	938	1313	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048217.D
 Acq On : 22 Apr 2022 12:06
 Operator : SY/MD
 Sample : VIBLK065
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.851	1710	1714	1718	rVB4	478	396	0.03%	0.004%
38	6.899	1725	1729	1732	rBV	321	208	0.02%	0.002%
39	6.967	1746	1750	1753	rBV2	254	220	0.02%	0.002%
40	7.044	1770	1774	1778	rBV2	328	284	0.02%	0.003%
41	7.186	1812	1818	1828	rVV5	1503	2536	0.21%	0.027%
42	7.301	1852	1854	1859	rVB2	323	251	0.02%	0.003%
43	7.333	1859	1864	1865	rBV	353	251	0.02%	0.003%
44	7.565	1923	1936	1958	rBV	137168	245180	20.69%	2.583%
45	7.687	1967	1974	1977	rBV5	1269	1301	0.11%	0.014%
46	7.739	1988	1990	1993	rVB3	386	190	0.02%	0.002%
47	7.793	2001	2007	2009	rBV3	540	485	0.04%	0.005%
48	7.803	2009	2010	2014	rVB	557	270	0.02%	0.003%
49	7.835	2016	2020	2023	rBV2	374	322	0.03%	0.003%
50	7.899	2023	2040	2056	rBV	500091	876885	73.98%	9.238%
51	8.179	2115	2127	2147	rBV	93650	164086	13.84%	1.729%
52	8.475	2216	2219	2225	rVB3	372	310	0.03%	0.003%
53	8.526	2232	2235	2239	rBV3	279	276	0.02%	0.003%
54	8.555	2242	2244	2248	rVB2	361	225	0.02%	0.002%
55	8.636	2256	2269	2304	rBV	328067	638852	53.90%	6.730%
56	8.906	2347	2353	2354	rBV	716	482	0.04%	0.005%
57	9.192	2436	2442	2445	rBV3	319	352	0.03%	0.004%
58	9.259	2461	2463	2468	rVB2	508	374	0.03%	0.004%
59	9.292	2468	2473	2477	rBV	333	407	0.03%	0.004%
60	9.356	2489	2493	2496	rVV2	326	301	0.03%	0.003%
61	9.417	2499	2512	2556	rVV	533553	1001822	84.52%	10.554%
62	9.571	2556	2560	2566	rVB2	383	422	0.04%	0.004%
63	9.616	2571	2574	2578	rBV	313	283	0.02%	0.003%
64	9.642	2578	2582	2585	rBV2	426	236	0.02%	0.002%
65	9.700	2591	2600	2606	rBV4	986	1239	0.10%	0.013%
66	9.790	2623	2628	2633	rBV2	252	355	0.03%	0.004%
67	10.263	2771	2775	2779	rBV2	371	290	0.02%	0.003%
68	10.311	2786	2790	2795	rVV2	280	350	0.03%	0.004%
69	10.349	2799	2802	2804	rVV	431	268	0.02%	0.003%
70	10.378	2808	2811	2814	rVB2	329	202	0.02%	0.002%
71	10.526	2854	2857	2859	rBV	323	246	0.02%	0.003%
72	10.597	2876	2879	2885	rBV2	235	212	0.02%	0.002%
73	10.674	2892	2903	2912	rBV3	2262	3330	0.28%	0.035%
74	10.755	2916	2928	2948	rVV	389020	623284	52.58%	6.566%
75	10.867	2956	2963	2966	rBV2	519	576	0.05%	0.006%
76	10.899	2969	2973	2977	rVB4	488	496	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048217.D
 Acq On : 22 Apr 2022 12:06
 Operator : SY/MD
 Sample : VIBLK065
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.021	3008	3011	3018	rVB	214	223	0.02%	0.002%
78	11.089	3024	3032	3037	rBV3	469	787	0.07%	0.008%
79	11.202	3062	3067	3068	rBV2	322	224	0.02%	0.002%
80	11.459	3136	3147	3157	rVB7	1443	2703	0.23%	0.028%
81	11.574	3179	3183	3185	rBV2	293	241	0.02%	0.003%
82	11.697	3213	3221	3226	rBV4	851	1141	0.10%	0.012%
83	11.751	3230	3238	3245	rBV6	2153	3174	0.27%	0.033%
84	11.812	3245	3257	3284	rBV	571341	975182	82.27%	10.273%
85	11.973	3302	3307	3311	rVB6	1361	1458	0.12%	0.015%
86	12.057	3328	3333	3337	rVV3	331	376	0.03%	0.004%
87	12.192	3360	3375	3397	rBV	508147	894166	75.44%	9.420%
88	12.365	3424	3429	3430	rBV2	266	189	0.02%	0.002%
89	12.513	3473	3475	3479	rVB2	444	249	0.02%	0.003%
90	12.616	3503	3507	3509	rBV3	322	250	0.02%	0.003%
91	12.639	3510	3514	3521	rVB3	437	504	0.04%	0.005%
92	12.674	3522	3525	3530	rVB3	311	241	0.02%	0.003%
93	12.896	3592	3594	3597	rBV2	346	182	0.02%	0.002%
94	13.221	3693	3695	3701	rBV3	454	389	0.03%	0.004%
95	13.848	3882	3890	3901	rVB2	6495	9855	0.83%	0.104%
96	14.092	3962	3966	3968	rBV	845	711	0.06%	0.007%
97	14.333	4035	4041	4051	rVB5	2659	3857	0.33%	0.041%
98	14.481	4084	4087	4089	rBV	358	246	0.02%	0.003%
99	14.536	4101	4104	4107	rBV2	400	331	0.03%	0.003%
100	15.889	4522	4525	4529	rBV3	854	922	0.08%	0.010%




Sum of corrected areas: 9492534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048217.D
Acq On : 22 Apr 2022 12:06
Operator : SY/MD
Sample : VIBLK065
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

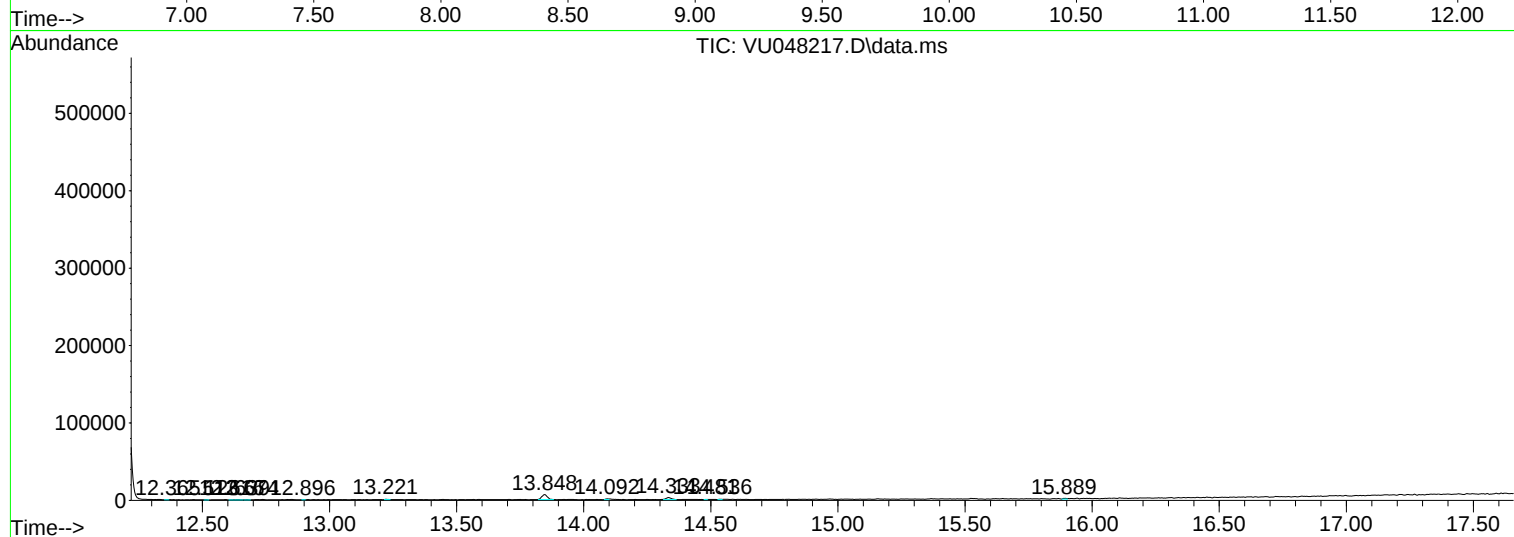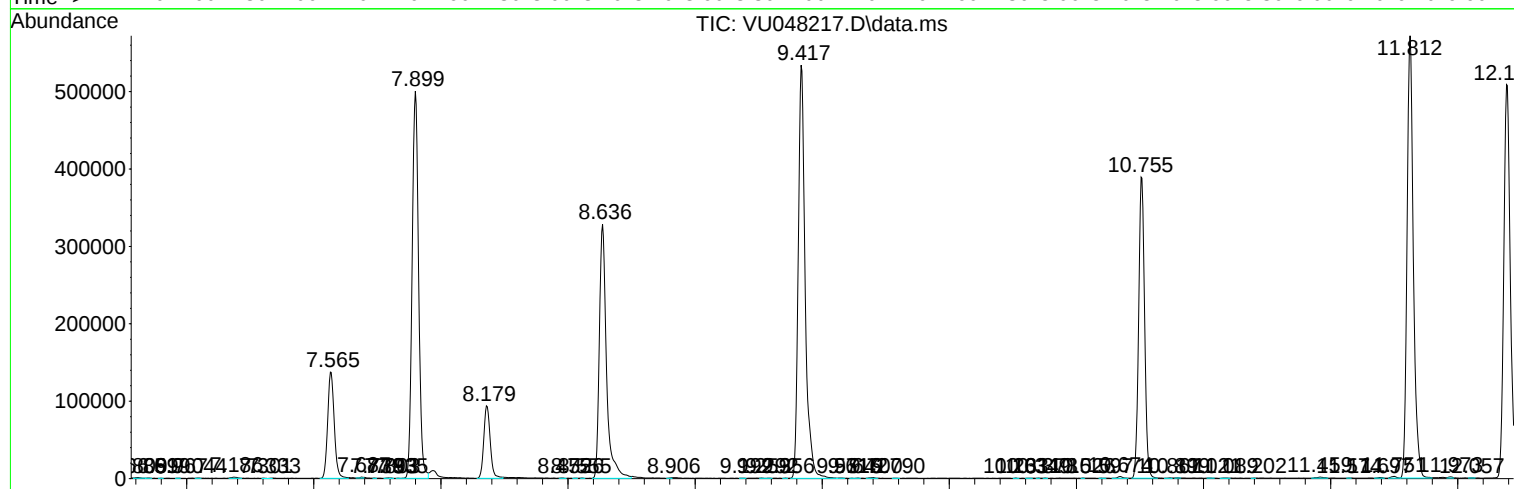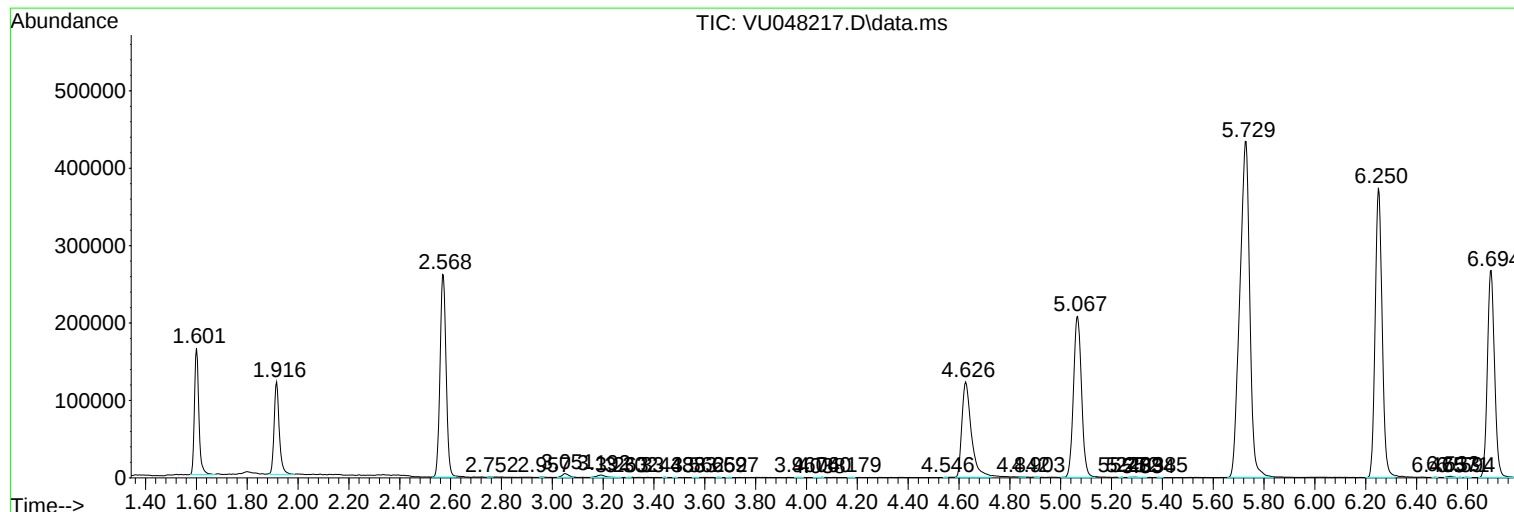

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048217.D
Acq On : 22 Apr 2022 12:06
Operator : SY/MD
Sample : VIBLK065
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048217.D
Acq On : 22 Apr 2022 12:06
Operator : SY/MD
Sample : VIBLK065
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------