

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048219.D
 Acq On : 22 Apr 2022 12:59
 Operator : SY/MD
 Sample : VIBLK066
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	148602	175100	15.39%	1.915%
2	1.916	171	179	197	rBV	109258	154051	13.54%	1.684%
3	2.523	362	368	370	rBV3	323	356	0.03%	0.004%
4	2.572	370	383	400	rBV	240944	396874	34.89%	4.340%
5	2.752	436	439	440	rBV	529	324	0.03%	0.004%
6	2.793	449	452	460	rVB4	636	687	0.06%	0.008%
7	2.855	468	471	474	rVB3	480	284	0.02%	0.003%
8	2.900	477	485	488	rBV2	212	362	0.03%	0.004%
9	2.957	500	503	508	rBV3	279	310	0.03%	0.003%
10	3.051	522	532	546	rVV2	4394	8832	0.78%	0.097%
11	3.189	559	575	593	rBV	16698	38437	3.38%	0.420%
12	3.347	617	624	630	rVV3	290	402	0.04%	0.004%
13	3.755	745	751	754	rBV2	221	249	0.02%	0.003%
14	3.871	782	787	790	rBV2	274	279	0.02%	0.003%
15	4.105	852	860	863	rBV2	329	427	0.04%	0.005%
16	4.173	876	881	886	rBV	277	367	0.03%	0.004%
17	4.208	886	892	895	rBV2	283	338	0.03%	0.004%
18	4.247	900	904	911	rVV	263	349	0.03%	0.004%
19	4.363	935	940	945	rBV2	281	364	0.03%	0.004%
20	4.568	998	1004	1006	rBV2	336	398	0.03%	0.004%
21	4.620	1007	1020	1063	rVV	121399	307302	27.02%	3.360%
22	5.067	1141	1159	1184	rBV	203034	443551	38.99%	4.850%
23	5.266	1217	1221	1224	rBV2	286	259	0.02%	0.003%
24	5.298	1224	1231	1237	rVV3	821	1216	0.11%	0.013%
25	5.424	1267	1270	1275	rVB	319	265	0.02%	0.003%
26	5.729	1343	1365	1397	rBV2	413856	1137495	100.00%	12.438%
27	5.948	1431	1433	1438	rVB3	380	245	0.02%	0.003%
28	5.973	1438	1441	1444	rBV2	274	203	0.02%	0.002%
29	6.115	1481	1485	1488	rBV3	422	431	0.04%	0.005%
30	6.250	1512	1527	1559	rBV	352927	680136	59.79%	7.437%
31	6.475	1593	1597	1599	rBV2	349	205	0.02%	0.002%
32	6.526	1606	1613	1623	rBV7	1233	2226	0.20%	0.024%
33	6.623	1640	1643	1648	rVB2	269	228	0.02%	0.002%
34	6.694	1650	1665	1693	rBV	258467	509013	44.75%	5.566%
35	6.809	1698	1701	1706	rVV3	1089	1058	0.09%	0.012%
36	7.044	1769	1774	1776	rBV	414	385	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048219.D
 Acq On : 22 Apr 2022 12:59
 Operator : SY/MD
 Sample : VIBLK066
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.057	1776	1778	1781	rVB	343	208	0.02%	0.002%
38	7.182	1812	1817	1825	rVV4	1251	1698	0.15%	0.019%
39	7.256	1835	1840	1842	rBV2	286	224	0.02%	0.002%
40	7.311	1851	1857	1865	rVB2	264	339	0.03%	0.004%
41	7.417	1887	1890	1896	rVB2	229	200	0.02%	0.002%
42	7.568	1924	1937	1954	rBV	133072	236387	20.78%	2.585%
43	7.690	1969	1975	1978	rBV3	763	987	0.09%	0.011%
44	7.748	1988	1993	1999	rBV2	273	270	0.02%	0.003%
45	7.796	2004	2008	2011	rBV2	612	536	0.05%	0.006%
46	7.899	2026	2040	2056	rBV	499820	863328	75.90%	9.440%
47	8.182	2115	2128	2142	rBV	94116	161289	14.18%	1.764%
48	8.452	2207	2212	2215	rBV3	278	314	0.03%	0.003%
49	8.542	2235	2240	2244	rBV2	332	278	0.02%	0.003%
50	8.571	2245	2249	2256	rVB2	380	474	0.04%	0.005%
51	8.636	2256	2269	2302	rBV	305862	628448	55.25%	6.872%
52	8.838	2330	2332	2336	rBV2	384	286	0.03%	0.003%
53	8.938	2361	2363	2366	rBV3	386	212	0.02%	0.002%
54	8.957	2366	2369	2373	rBV4	325	254	0.02%	0.003%
55	9.002	2381	2383	2391	rVB2	339	352	0.03%	0.004%
56	9.041	2391	2395	2399	rBV2	293	279	0.02%	0.003%
57	9.131	2417	2423	2426	rVV2	415	397	0.03%	0.004%
58	9.163	2430	2433	2438	rVV3	353	337	0.03%	0.004%
59	9.362	2492	2495	2499	rBV2	279	217	0.02%	0.002%
60	9.420	2499	2513	2548	rBV	548095	979701	86.13%	10.712%
61	9.571	2557	2560	2567	rBV2	434	463	0.04%	0.005%
62	9.649	2581	2584	2589	rVV3	424	343	0.03%	0.004%
63	9.697	2593	2599	2604	rVB3	898	1010	0.09%	0.011%
64	10.118	2728	2730	2733	rVB	484	246	0.02%	0.003%
65	10.137	2733	2736	2738	rBV	268	204	0.02%	0.002%
66	10.153	2738	2741	2749	rVB3	236	225	0.02%	0.002%
67	10.671	2896	2902	2912	rVB3	2289	3294	0.29%	0.036%
68	10.758	2916	2929	2946	rBV	386200	625624	55.00%	6.841%
69	10.861	2957	2961	2963	rBV4	459	325	0.03%	0.004%
70	11.153	3049	3052	3063	rVV4	472	577	0.05%	0.006%
71	11.201	3064	3067	3070	rVB2	421	233	0.02%	0.003%
72	11.298	3094	3097	3099	rBV2	376	239	0.02%	0.003%
73	11.324	3103	3105	3111	rVV2	414	348	0.03%	0.004%
74	11.349	3111	3113	3118	rVV2	302	369	0.03%	0.004%
75	11.385	3121	3124	3128	rVV2	446	337	0.03%	0.004%
76	11.414	3130	3133	3137	rVV2	409	367	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048219.D
 Acq On : 22 Apr 2022 12:59
 Operator : SY/MD
 Sample : VIBLK066
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3159	rVB6	1628	3071	0.27%	0.034%
78	11.581	3182	3185	3191	rVB2	246	234	0.02%	0.003%
79	11.684	3214	3217	3219	rBV2	363	221	0.02%	0.002%
80	11.697	3219	3221	3225	rVV	474	366	0.03%	0.004%
81	11.748	3230	3237	3245	rVB4	2309	3263	0.29%	0.036%
82	11.812	3245	3257	3285	rBV	540961	911710	80.15%	9.969%
83	11.973	3304	3307	3314	rVB4	1805	1748	0.15%	0.019%
84	12.054	3329	3332	3335	rBV2	282	202	0.02%	0.002%
85	12.099	3343	3346	3350	rVB	343	237	0.02%	0.003%
86	12.195	3362	3376	3398	rBV	492877	837328	73.61%	9.156%
87	12.497	3469	3470	3477	rVB2	245	244	0.02%	0.003%
88	12.545	3483	3485	3490	rVB2	424	243	0.02%	0.003%
89	12.584	3494	3497	3502	rVB2	342	290	0.03%	0.003%
90	12.632	3509	3512	3513	rBV	425	260	0.02%	0.003%
91	12.668	3519	3523	3527	rVB2	256	226	0.02%	0.002%
92	12.758	3549	3551	3558	rVB3	225	226	0.02%	0.002%
93	12.896	3590	3594	3596	rBV	336	310	0.03%	0.003%
94	13.002	3623	3627	3629	rBV2	288	262	0.02%	0.003%
95	13.066	3645	3647	3654	rBV3	235	294	0.03%	0.003%
96	13.240	3692	3701	3705	rBV3	634	946	0.08%	0.010%
97	13.459	3766	3769	3773	rBV2	328	201	0.02%	0.002%
98	13.844	3882	3889	3898	rBV2	4301	6835	0.60%	0.075%
99	14.147	3981	3983	3989	rBV2	541	414	0.04%	0.005%
100	14.340	4037	4043	4050	rVB4	1676	2094	0.18%	0.023%




Sum of corrected areas: 9145452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048219.D
Acq On : 22 Apr 2022 12:59
Operator : SY/MD
Sample : VIBLK066
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

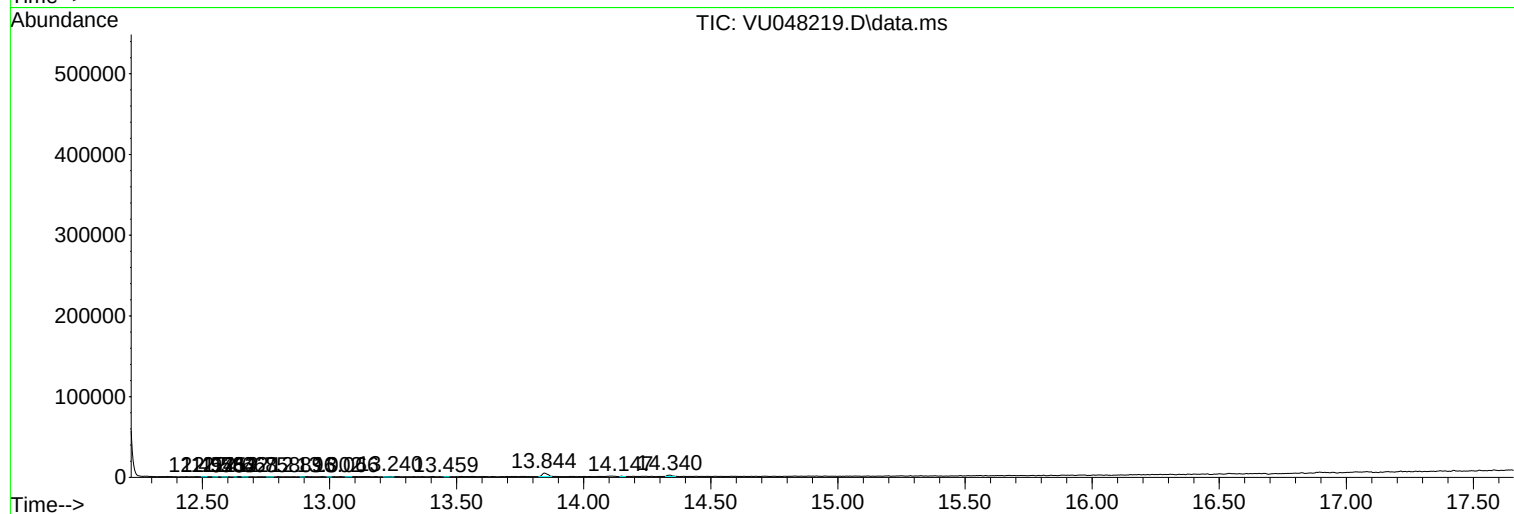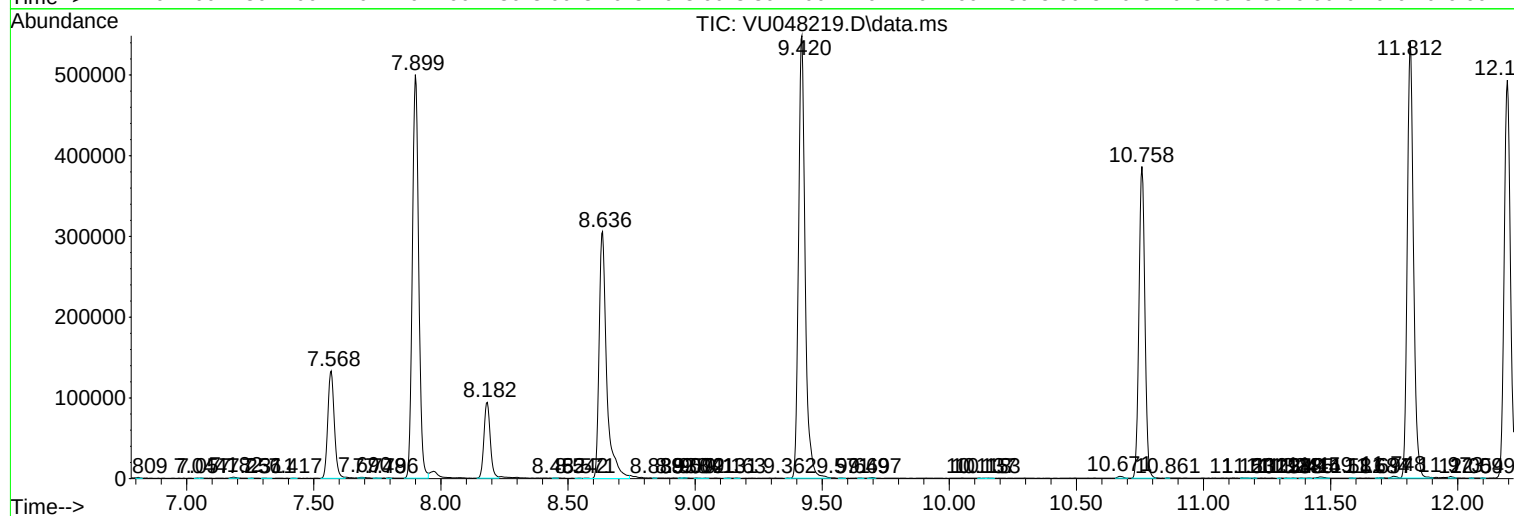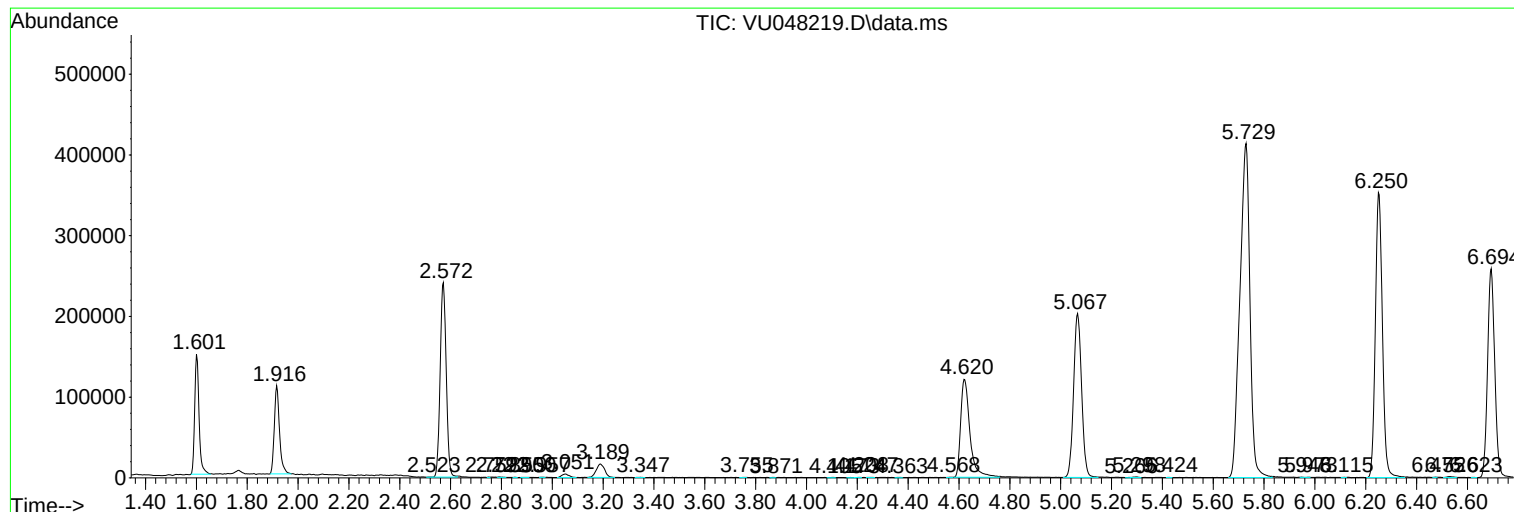

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048219.D
Acq On : 22 Apr 2022 12:59
Operator : SY/MD
Sample : VIBLK066
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048219.D
Acq On : 22 Apr 2022 12:59
Operator : SY/MD
Sample : VIBLK066
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------