

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048220.D
 Acq On : 22 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2485-12DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	151562	175997	13.60%	1.807%
2	1.916	170	179	199	rVB	110413	156449	12.09%	1.606%
3	2.572	370	383	397	rBV	241077	398139	30.77%	4.087%
4	2.655	407	409	412	rVB3	493	264	0.02%	0.003%
5	2.691	418	420	428	rVB3	282	323	0.02%	0.003%
6	2.729	428	432	434	rBV2	294	240	0.02%	0.002%
7	2.745	434	437	438	rBV	449	242	0.02%	0.002%
8	2.842	464	467	474	rVB4	379	468	0.04%	0.005%
9	2.890	479	482	487	rBV2	190	235	0.02%	0.002%
10	2.951	498	501	506	rBV3	262	318	0.02%	0.003%
11	3.051	522	532	547	rBV2	9720	18576	1.44%	0.191%
12	3.186	560	574	591	rBV2	16814	38513	2.98%	0.395%
13	3.363	626	629	632	rBV2	355	225	0.02%	0.002%
14	3.420	644	647	651	rBV2	213	160	0.01%	0.002%
15	3.575	691	695	697	rBV	218	176	0.01%	0.002%
16	3.761	747	753	757	rBV2	323	425	0.03%	0.004%
17	3.781	757	759	761	rBV	256	179	0.01%	0.002%
18	3.919	797	802	804	rBV2	328	278	0.02%	0.003%
19	3.961	812	815	819	rBV2	291	196	0.02%	0.002%
20	4.105	857	860	864	rVB2	239	211	0.02%	0.002%
21	4.128	864	867	871	rBV2	182	160	0.01%	0.002%
22	4.205	884	891	895	rBV2	152	218	0.02%	0.002%
23	4.369	938	942	946	rBV2	229	259	0.02%	0.003%
24	4.555	996	1000	1005	rBV3	319	377	0.03%	0.004%
25	4.620	1007	1020	1050	rBV	116760	287140	22.19%	2.948%
26	5.067	1139	1159	1186	rBV	196005	431344	33.34%	4.428%
27	5.247	1214	1215	1220	rVB2	250	173	0.01%	0.002%
28	5.391	1255	1260	1263	rVB2	394	254	0.02%	0.003%
29	5.729	1337	1365	1373	rBV2	404125	1102993	85.25%	11.322%
30	6.041	1459	1462	1466	rVB2	341	230	0.02%	0.002%
31	6.170	1500	1502	1506	rBV2	199	168	0.01%	0.002%
32	6.250	1512	1527	1553	rBV	364414	697255	53.89%	7.157%
33	6.369	1562	1564	1567	rVB	418	164	0.01%	0.002%
34	6.462	1589	1593	1595	rBV3	181	157	0.01%	0.002%
35	6.539	1608	1617	1620	rBV4	827	1186	0.09%	0.012%
36	6.600	1630	1636	1638	rBV	301	327	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048220.D
 Acq On : 22 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2485-12DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1648	1665	1690	rBV	251479	498528	38.53%	5.117%
38	6.864	1714	1718	1723	rVB2	385	489	0.04%	0.005%
39	6.890	1723	1726	1728	rBV2	345	289	0.02%	0.003%
40	7.057	1772	1778	1781	rBV3	436	545	0.04%	0.006%
41	7.166	1807	1812	1813	rBV	471	340	0.03%	0.003%
42	7.186	1813	1818	1827	rVB3	1300	2126	0.16%	0.022%
43	7.301	1850	1854	1856	rBV2	355	194	0.01%	0.002%
44	7.382	1872	1879	1880	rBV2	350	377	0.03%	0.004%
45	7.568	1922	1937	1957	rBV	126326	228877	17.69%	2.349%
46	7.678	1969	1971	1972	rBV	306	157	0.01%	0.002%
47	7.723	1983	1985	1987	rVB2	338	176	0.01%	0.002%
48	7.735	1987	1989	1992	rBV3	262	190	0.01%	0.002%
49	7.800	2007	2009	2013	rVB	622	363	0.03%	0.004%
50	7.899	2026	2040	2056	rBV	492267	841914	65.07%	8.642%
51	8.179	2111	2127	2142	rBV	90581	155972	12.06%	1.601%
52	8.356	2180	2182	2187	rVB3	386	277	0.02%	0.003%
53	8.533	2234	2237	2241	rBV2	223	218	0.02%	0.002%
54	8.555	2241	2244	2247	rVV2	722	356	0.03%	0.004%
55	8.633	2256	2268	2318	rBV	299601	618553	47.81%	6.350%
56	8.841	2331	2333	2338	rVB3	377	284	0.02%	0.003%
57	9.144	2423	2427	2428	rBV	296	159	0.01%	0.002%
58	9.166	2428	2434	2438	rVV3	617	634	0.05%	0.007%
59	9.272	2465	2467	2473	rVB2	248	178	0.01%	0.002%
60	9.420	2498	2513	2517	rBV	565492	955953	73.89%	9.813%
61	9.639	2578	2581	2583	rBV3	507	247	0.02%	0.003%
62	9.687	2591	2596	2597	rBV2	747	523	0.04%	0.005%
63	9.774	2621	2623	2628	rVB3	339	227	0.02%	0.002%
64	9.848	2640	2646	2649	rBV3	292	326	0.03%	0.003%
65	9.886	2656	2658	2662	rBV2	290	190	0.01%	0.002%
66	9.909	2663	2665	2669	rVB2	312	168	0.01%	0.002%
67	9.951	2673	2678	2680	rBV2	322	241	0.02%	0.002%
68	10.079	2714	2718	2723	rVB2	264	284	0.02%	0.003%
69	10.108	2723	2727	2730	rBV	378	198	0.02%	0.002%
70	10.124	2730	2732	2737	rBV2	387	359	0.03%	0.004%
71	10.198	2752	2755	2758	rVB	285	186	0.01%	0.002%
72	10.231	2761	2765	2770	rBV	316	356	0.03%	0.004%
73	10.327	2792	2795	2798	rBV	253	191	0.01%	0.002%
74	10.423	2822	2825	2827	rBV2	240	188	0.01%	0.002%
75	10.584	2869	2875	2878	rBV	381	486	0.04%	0.005%
76	10.668	2895	2901	2913	rVB5	1814	2920	0.23%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048220.D
 Acq On : 22 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2485-12DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2915	2929	2946	rBV	370872	605733	46.82%	6.218%
78	10.893	2967	2971	2978	rVB3	490	633	0.05%	0.006%
79	10.970	2992	2995	2998	rBV	284	196	0.02%	0.002%
80	10.993	2999	3002	3005	rBV2	239	221	0.02%	0.002%
81	11.134	3042	3046	3051	rVB3	353	324	0.03%	0.003%
82	11.459	3140	3147	3153	rVB4	1355	1726	0.13%	0.018%
83	11.568	3176	3181	3183	rBV2	457	377	0.03%	0.004%
84	11.693	3215	3220	3226	rBV3	728	780	0.06%	0.008%
85	11.748	3226	3237	3245	rBV2	18455	29043	2.24%	0.298%
86	11.812	3245	3257	3285	rVB3	573014	1293820	100.00%	13.281%
87	11.973	3302	3307	3318	rVB8	1420	2054	0.16%	0.021%
88	12.083	3338	3341	3346	rVB3	536	491	0.04%	0.005%
89	12.111	3346	3350	3352	rBV2	373	317	0.02%	0.003%
90	12.195	3357	3376	3402	rBV3	529943	1143457	88.38%	11.738%
91	12.333	3416	3419	3424	rBV2	337	266	0.02%	0.003%
92	12.446	3451	3454	3457	rBV3	306	227	0.02%	0.002%
93	12.613	3500	3506	3508	rBV3	413	459	0.04%	0.005%
94	12.648	3509	3517	3520	rBV3	731	1123	0.09%	0.012%
95	12.684	3525	3528	3533	rBV3	389	378	0.03%	0.004%
96	13.005	3624	3628	3631	rBV2	407	376	0.03%	0.004%
97	13.057	3642	3644	3646	rBV	326	182	0.01%	0.002%
98	13.388	3744	3747	3751	rBV2	406	320	0.02%	0.003%
99	13.845	3880	3889	3903	rBV2	16695	27555	2.13%	0.283%
100	14.336	4036	4042	4050	rVB7	2333	3321	0.26%	0.034%




Sum of corrected areas: 9741637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048220.D
Acq On : 22 Apr 2022 13:23
Operator : SY/MD
Sample : N2485-12DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

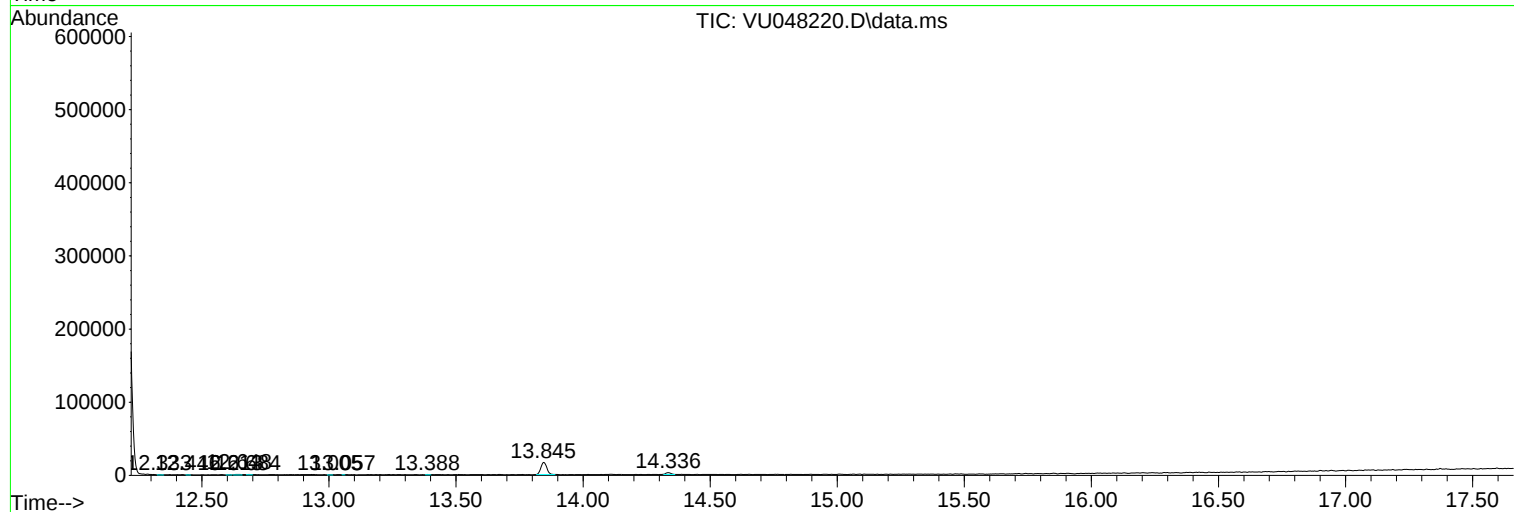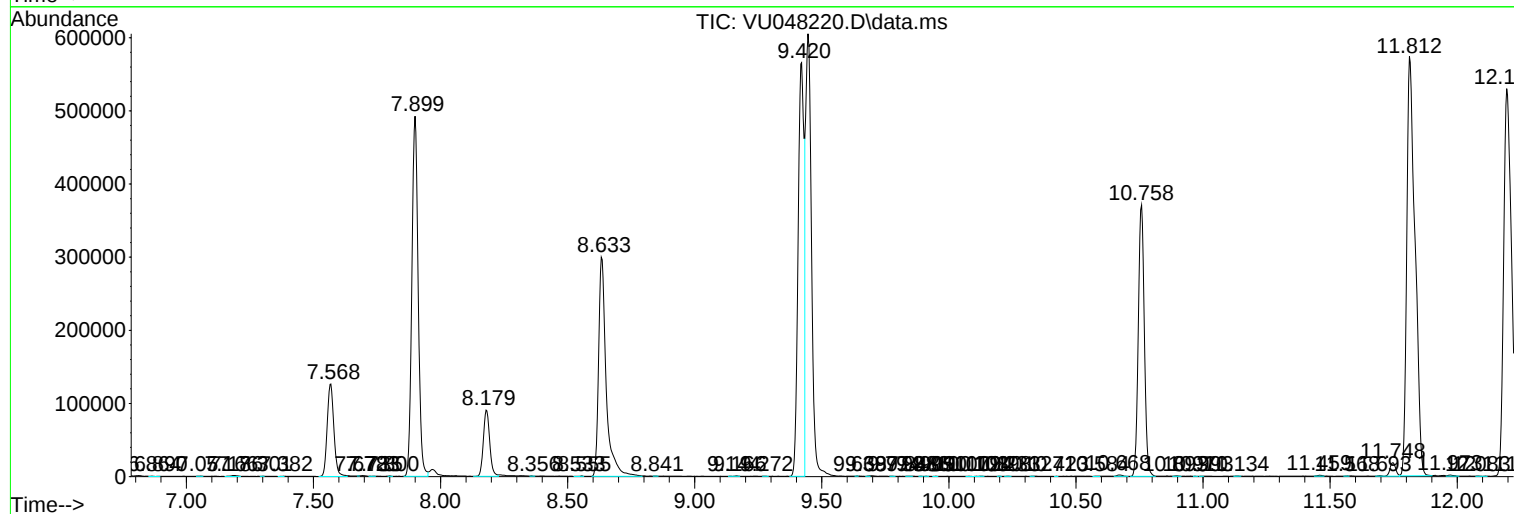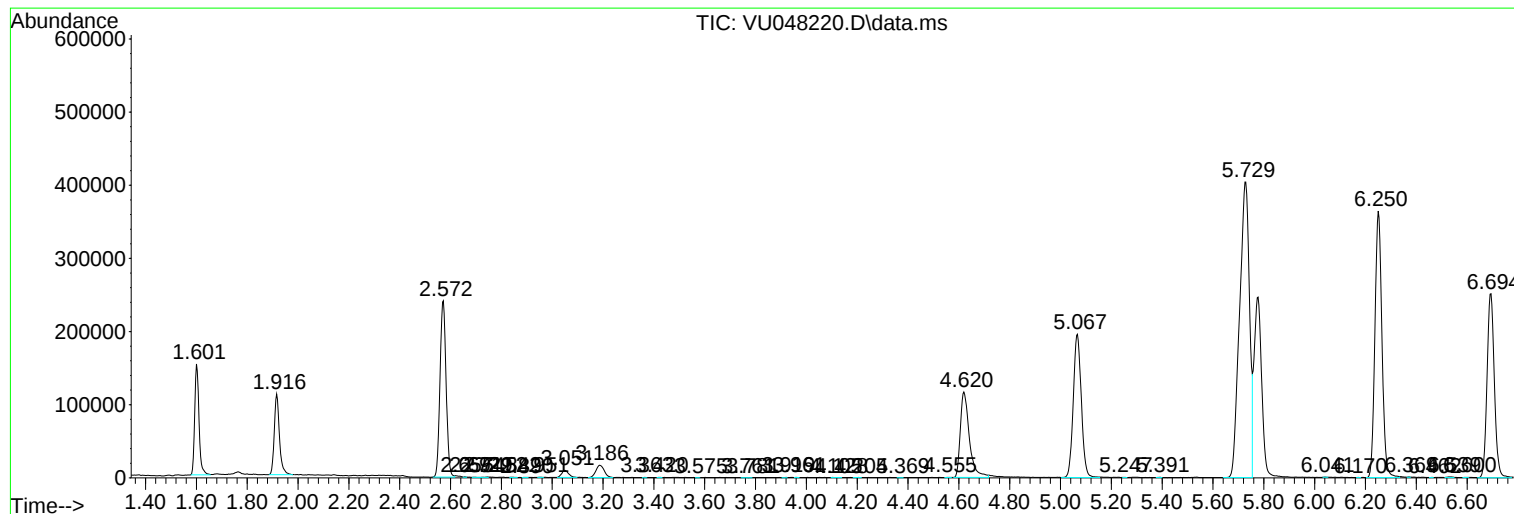

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048220.D
Acq On : 22 Apr 2022 13:23
Operator : SY/MD
Sample : N2485-12DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048220.D
Acq On : 22 Apr 2022 13:23
Operator : SY/MD
Sample : N2485-12DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------