

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048221.D
 Acq On : 22 Apr 2022 13:47
 Operator : SY/MD
 Sample : N2485-13DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	51	rBV3	2957	3691	0.28%	0.036%
2	1.601	73	81	100	rBV	138457	178035	13.32%	1.722%
3	1.880	163	168	193	rVB	91305	145435	10.88%	1.407%
4	2.504	358	362	367	rVB3	390	362	0.03%	0.004%
5	2.559	367	379	396	rBV	232431	386692	28.93%	3.741%
6	2.803	437	455	476	rVB	10015	28888	2.16%	0.279%
7	2.896	481	484	487	rBV3	329	244	0.02%	0.002%
8	2.938	494	497	501	rBV3	496	329	0.02%	0.003%
9	2.961	501	504	509	rVB	482	397	0.03%	0.004%
10	2.983	509	511	516	rBV3	317	232	0.02%	0.002%
11	3.047	522	531	545	rVB5	1906	3953	0.30%	0.038%
12	3.183	557	573	586	rBV	34945	82026	6.14%	0.793%
13	3.311	610	613	619	rVB2	412	363	0.03%	0.004%
14	3.533	678	682	686	rVB2	370	304	0.02%	0.003%
15	3.578	692	696	700	rVB2	304	226	0.02%	0.002%
16	3.787	758	761	767	rVB2	247	272	0.02%	0.003%
17	4.092	853	856	859	rBV2	286	253	0.02%	0.002%
18	4.166	871	879	882	rBV	223	271	0.02%	0.003%
19	4.456	966	969	975	rBV2	208	213	0.02%	0.002%
20	4.552	991	999	1003	rBV2	488	614	0.05%	0.006%
21	4.623	1008	1021	1041	rBV	107293	274648	20.55%	2.657%
22	4.954	1117	1124	1127	rBV3	295	342	0.03%	0.003%
23	5.063	1141	1158	1183	rVV	186575	410288	30.69%	3.969%
24	5.218	1204	1206	1210	rVV2	363	251	0.02%	0.002%
25	5.282	1222	1226	1227	rVV2	400	310	0.02%	0.003%
26	5.305	1231	1233	1235	rVV	725	431	0.03%	0.004%
27	5.330	1236	1241	1259	rVB4	1736	3959	0.30%	0.038%
28	5.446	1271	1277	1281	rVB2	258	351	0.03%	0.003%
29	5.514	1294	1298	1304	rBV4	381	438	0.03%	0.004%
30	5.723	1342	1363	1373	rBV2	395836	1077717	80.63%	10.425%
31	5.967	1430	1439	1455	rVB4	5477	11467	0.86%	0.111%
32	6.038	1456	1461	1464	rBV3	437	357	0.03%	0.003%
33	6.115	1480	1485	1489	rBV2	371	400	0.03%	0.004%
34	6.160	1494	1499	1505	rVV3	582	630	0.05%	0.006%
35	6.250	1512	1527	1551	rBV	355270	674437	50.46%	6.524%
36	6.510	1604	1608	1610	rBV3	1154	937	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048221.D
 Acq On : 22 Apr 2022 13:47
 Operator : SY/MD
 Sample : N2485-13DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.594	1625	1634	1642	rBV6	2466	4874	0.36%	0.047%
38	6.690	1650	1664	1685	rBV	244927	473300	35.41%	4.578%
39	6.809	1696	1701	1706	rBV5	696	701	0.05%	0.007%
40	6.890	1719	1726	1728	rBV3	203	237	0.02%	0.002%
41	6.922	1733	1736	1739	rVV2	247	220	0.02%	0.002%
42	6.938	1739	1741	1745	rVB3	322	209	0.02%	0.002%
43	7.179	1805	1816	1823	rBV2	3872	8282	0.62%	0.080%
44	7.321	1858	1860	1866	rVB3	357	233	0.02%	0.002%
45	7.565	1924	1936	1959	rVV	127609	220088	16.47%	2.129%
46	7.694	1967	1976	1984	rBV4	888	1651	0.12%	0.016%
47	7.755	1989	1995	2000	rVB2	271	307	0.02%	0.003%
48	7.803	2008	2010	2016	rVB2	338	282	0.02%	0.003%
49	7.899	2026	2040	2055	rBV	481687	830739	62.15%	8.036%
50	7.973	2057	2063	2079	rVV5	9026	20406	1.53%	0.197%
51	8.041	2082	2084	2087	rVB2	525	258	0.02%	0.002%
52	8.179	2116	2127	2145	rVV	90031	153615	11.49%	1.486%
53	8.346	2177	2179	2183	rVB2	594	305	0.02%	0.003%
54	8.423	2199	2203	2206	rBV3	304	278	0.02%	0.003%
55	8.468	2206	2217	2229	rVB3	4640	8612	0.64%	0.083%
56	8.530	2233	2236	2240	rVB3	397	288	0.02%	0.003%
57	8.555	2240	2244	2248	rVB2	324	308	0.02%	0.003%
58	8.639	2256	2270	2301	rBV	331656	643547	48.15%	6.225%
59	8.909	2352	2354	2361	rVB2	266	224	0.02%	0.002%
60	8.983	2372	2377	2383	rBV2	273	337	0.03%	0.003%
61	9.012	2383	2386	2391	rBV2	428	337	0.03%	0.003%
62	9.070	2399	2404	2408	rBV2	387	510	0.04%	0.005%
63	9.420	2499	2513	2517	rBV	578621	968371	72.45%	9.367%
64	9.674	2589	2592	2593	rBV	430	230	0.02%	0.002%
65	9.890	2655	2659	2664	rBV	166	235	0.02%	0.002%
66	10.009	2692	2696	2700	rBV2	304	279	0.02%	0.003%
67	10.054	2707	2710	2714	rVB2	384	250	0.02%	0.002%
68	10.153	2736	2741	2746	rBV2	184	293	0.02%	0.003%
69	10.571	2865	2871	2874	rBV	283	323	0.02%	0.003%
70	10.607	2879	2882	2890	rVV2	354	315	0.02%	0.003%
71	10.671	2896	2902	2912	rVB3	2194	2767	0.21%	0.027%
72	10.758	2917	2929	2949	rVV	415975	665641	49.80%	6.439%
73	10.893	2961	2971	2983	rVV	6941	11369	0.85%	0.110%
74	11.018	3004	3010	3013	rBV2	195	235	0.02%	0.002%
75	11.060	3019	3023	3030	rBV3	353	504	0.04%	0.005%
76	11.121	3040	3042	3046	rVB3	369	250	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048221.D
 Acq On : 22 Apr 2022 13:47
 Operator : SY/MD
 Sample : N2485-13DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.205	3063	3068	3070	rBV2	315	290	0.02%	0.003%
78	11.455	3138	3146	3148	rBV4	1743	1848	0.14%	0.018%
79	11.697	3219	3221	3226	rVV2	553	405	0.03%	0.004%
80	11.748	3226	3237	3246	rVV	39789	62892	4.71%	0.608%
81	11.812	3246	3257	3283	rVB2	615791	1336666	100.00%	12.930%
82	11.973	3303	3307	3318	rVB5	1783	2188	0.16%	0.021%
83	12.025	3320	3323	3326	rBV	349	287	0.02%	0.003%
84	12.198	3361	3377	3403	rVV3	592595	1315788	98.44%	12.728%
85	12.333	3415	3419	3425	rVB5	742	642	0.05%	0.006%
86	12.510	3470	3474	3478	rBV4	364	365	0.03%	0.004%
87	12.539	3481	3483	3488	rBV3	321	321	0.02%	0.003%
88	12.774	3545	3556	3563	rVB3	2784	4493	0.34%	0.043%
89	12.980	3614	3620	3623	rBV3	852	921	0.07%	0.009%
90	13.121	3661	3664	3667	rBV3	354	302	0.02%	0.003%
91	13.426	3755	3759	3764	rBV2	342	406	0.03%	0.004%
92	13.713	3842	3848	3850	rBV3	495	593	0.04%	0.006%
93	13.841	3876	3888	3905	rBV	144913	233805	17.49%	2.262%
94	14.025	3942	3945	3948	rBV2	269	213	0.02%	0.002%
95	14.095	3960	3967	3974	rVB2	706	1259	0.09%	0.012%
96	14.330	4030	4040	4054	rBV3	38811	61698	4.62%	0.597%
97	14.494	4087	4091	4097	rBV4	347	420	0.03%	0.004%
98	14.777	4176	4179	4182	rBV3	390	342	0.03%	0.003%
99	15.304	4341	4343	4345	rBV3	668	337	0.03%	0.003%
100	15.561	4421	4423	4426	rBV3	692	406	0.03%	0.004%


Sum of corrected areas: 10337860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048221.D
Acq On : 22 Apr 2022 13:47
Operator : SY/MD
Sample : N2485-13DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

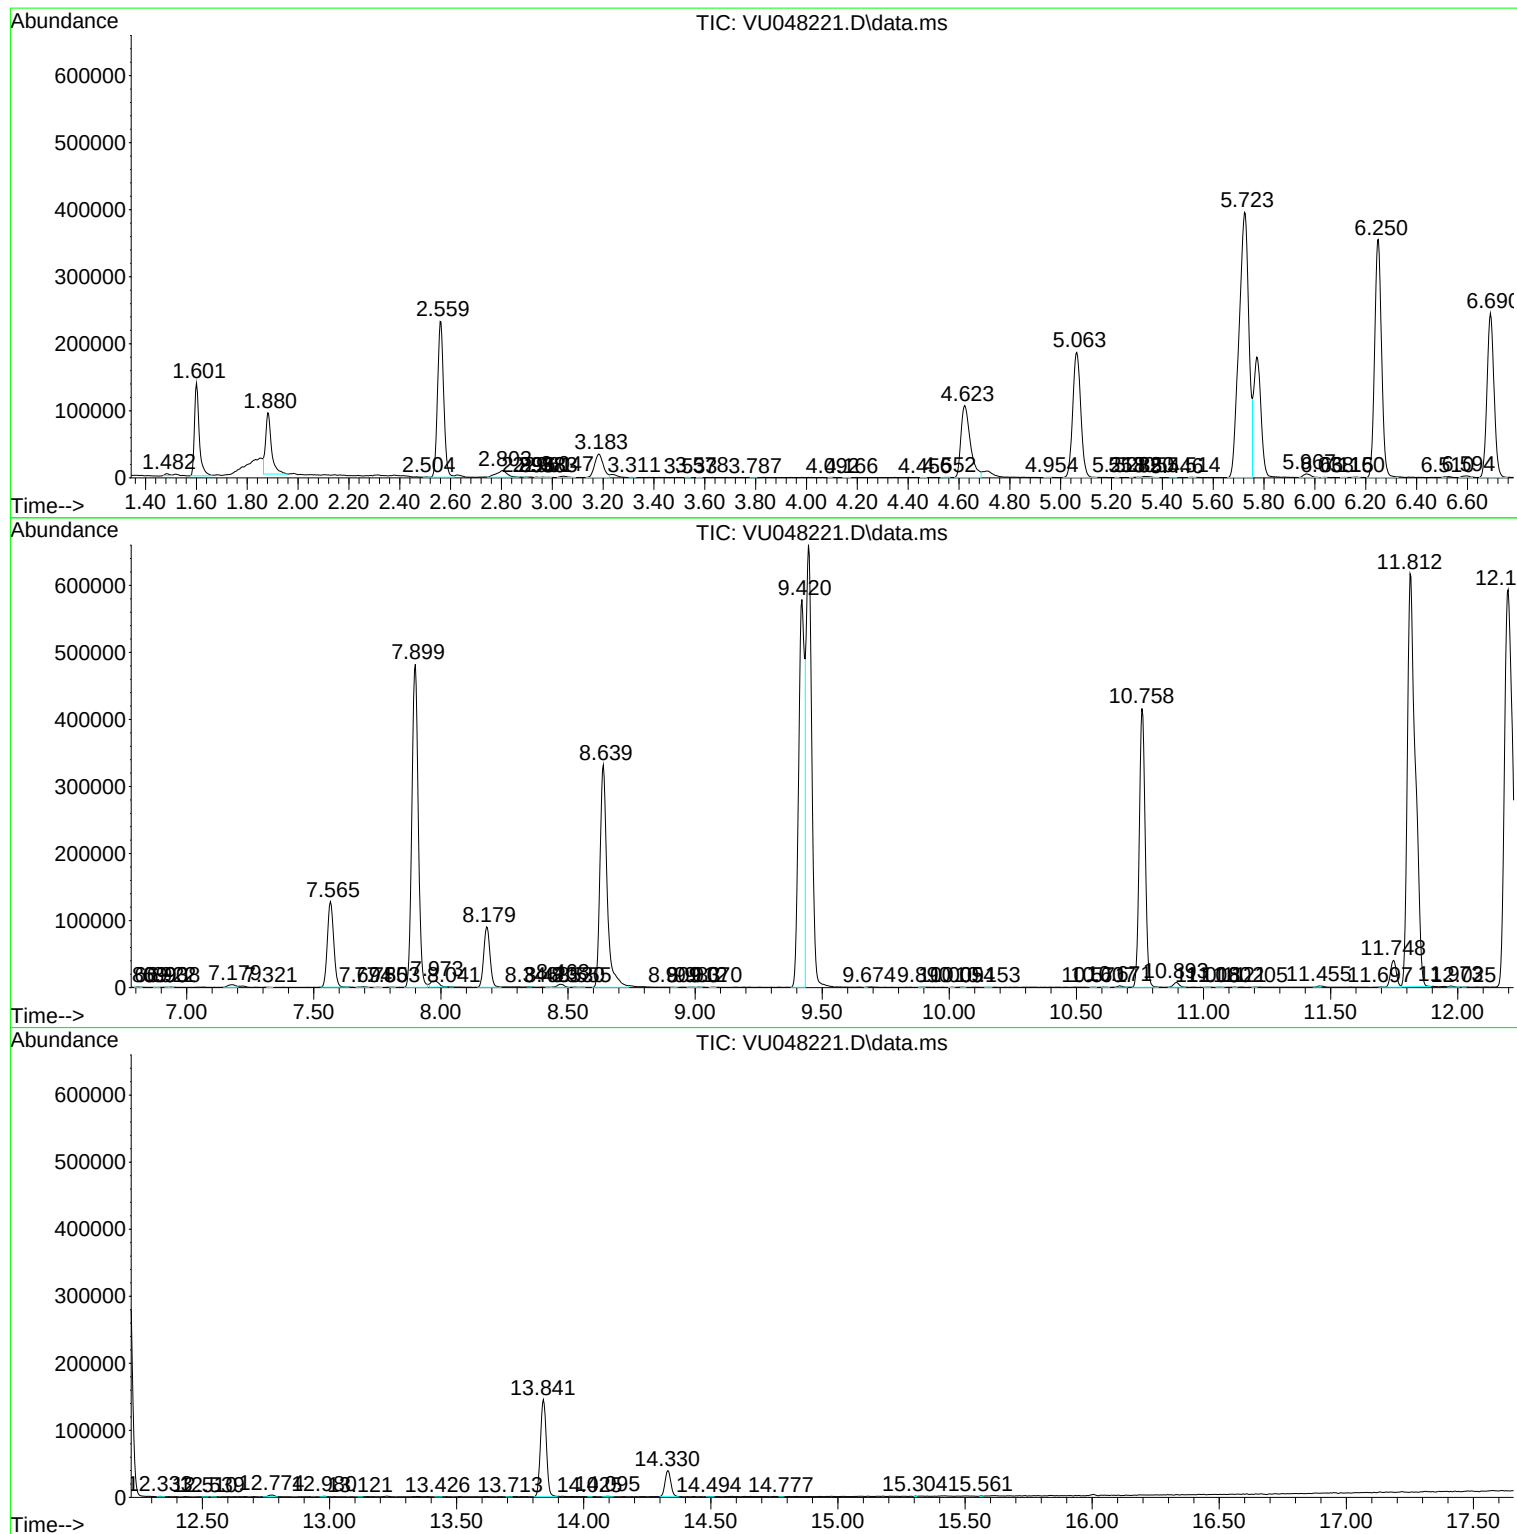

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048221.D
Acq On : 22 Apr 2022 13:47
Operator : SY/MD
Sample : N2485-13DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048221.D
Acq On : 22 Apr 2022 13:47
Operator : SY/MD
Sample : N2485-13DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------