

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048222.D
 Acq On : 22 Apr 2022 14:10
 Operator : SY/MD
 Sample : N2485-14DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	50	rBV2	5094	6192	0.24%	0.048%
2	1.600	73	81	100	rBV	145052	182150	7.08%	1.425%
3	1.887	163	170	189	rVB	92905	140321	5.45%	1.098%
4	2.562	368	380	398	rVV	237128	391638	15.22%	3.063%
5	2.716	425	428	430	rBV4	388	290	0.01%	0.002%
6	2.745	434	437	440	rVB	332	245	0.01%	0.002%
7	2.790	447	451	459	rVB5	1133	1507	0.06%	0.012%
8	2.829	459	463	464	rBV2	372	233	0.01%	0.002%
9	2.861	471	473	479	rBV4	260	261	0.01%	0.002%
10	2.925	489	493	496	rVB2	421	323	0.01%	0.003%
11	2.999	513	516	519	rBV2	478	389	0.02%	0.003%
12	3.044	522	530	540	rVV3	2252	4507	0.18%	0.035%
13	3.083	540	542	544	rVV2	519	220	0.01%	0.002%
14	3.115	548	552	558	rVV3	474	506	0.02%	0.004%
15	3.186	558	574	607	rVB	35834	96256	3.74%	0.753%
16	3.308	607	612	620	rVB4	494	672	0.03%	0.005%
17	3.485	661	667	668	rBV	279	220	0.01%	0.002%
18	3.587	694	699	702	rBV2	314	296	0.01%	0.002%
19	3.632	708	713	717	rBV3	249	241	0.01%	0.002%
20	3.887	786	792	799	rBV2	355	591	0.02%	0.005%
21	3.960	811	815	821	rVB2	271	322	0.01%	0.003%
22	4.067	846	848	854	rVB2	516	390	0.02%	0.003%
23	4.160	869	877	879	rBV2	265	336	0.01%	0.003%
24	4.420	955	958	961	rVB	307	223	0.01%	0.002%
25	4.517	985	988	995	rVB	283	258	0.01%	0.002%
26	4.552	995	999	1001	rBV3	349	312	0.01%	0.002%
27	4.623	1007	1021	1067	rBV	114739	296923	11.54%	2.323%
28	4.819	1080	1082	1090	rVB3	504	575	0.02%	0.004%
29	4.925	1106	1115	1119	rBV2	301	595	0.02%	0.005%
30	5.063	1142	1158	1179	rBV	192133	422459	16.41%	3.304%
31	5.282	1222	1226	1227	rBV	316	213	0.01%	0.002%
32	5.292	1227	1229	1231	rVV3	576	420	0.02%	0.003%
33	5.340	1235	1244	1258	rVB3	1766	4224	0.16%	0.033%
34	5.523	1293	1301	1305	rBV2	1030	1381	0.05%	0.011%
35	5.726	1341	1364	1374	rBV2	401240	1093299	42.47%	8.552%
36	5.967	1433	1439	1441	rBV5	771	843	0.03%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048222.D
 Acq On : 22 Apr 2022 14:10
 Operator : SY/MD
 Sample : N2485-14DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.015	1450	1454	1458	rBV2	520	420	0.02%	0.003%
38	6.054	1458	1466	1469	rVV4	413	532	0.02%	0.004%
39	6.108	1480	1483	1486	rVV2	334	267	0.01%	0.002%
40	6.250	1511	1527	1553	rBV	360755	680447	26.44%	5.322%
41	6.523	1606	1612	1614	rBV3	784	824	0.03%	0.006%
42	6.597	1627	1635	1637	rBV3	813	844	0.03%	0.007%
43	6.690	1649	1664	1686	rBV	247463	483066	18.77%	3.779%
44	7.179	1805	1816	1824	rVV5	2944	6640	0.26%	0.052%
45	7.224	1828	1830	1834	rVB2	717	319	0.01%	0.002%
46	7.263	1840	1842	1847	rBV	242	235	0.01%	0.002%
47	7.565	1924	1936	1952	rVV	126587	221823	8.62%	1.735%
48	7.687	1971	1974	1983	rVB4	928	1193	0.05%	0.009%
49	7.787	1998	2005	2006	rBV2	1206	1263	0.05%	0.010%
50	7.899	2025	2040	2055	rBV	488878	835624	32.46%	6.536%
51	8.092	2098	2100	2106	rVB2	600	485	0.02%	0.004%
52	8.127	2106	2111	2115	rBV3	427	561	0.02%	0.004%
53	8.179	2115	2127	2143	rBV	90932	151875	5.90%	1.188%
54	8.468	2209	2217	2219	rBV4	828	1037	0.04%	0.008%
55	8.636	2256	2269	2300	rBV	352633	679868	26.41%	5.318%
56	8.886	2345	2347	2353	rVB3	283	237	0.01%	0.002%
57	9.127	2415	2422	2425	rVB2	269	279	0.01%	0.002%
58	9.147	2425	2428	2431	rBV	366	238	0.01%	0.002%
59	9.166	2431	2434	2437	rBV	293	243	0.01%	0.002%
60	9.420	2499	2513	2516	rBV	572561	874390	33.97%	6.839%
61	9.645	2579	2583	2588	rVB3	387	338	0.01%	0.003%
62	9.680	2591	2594	2595	rVV	457	238	0.01%	0.002%
63	9.690	2595	2597	2605	rVB3	751	889	0.03%	0.007%
64	9.902	2660	2663	2668	rVV	249	245	0.01%	0.002%
65	10.102	2722	2725	2731	rBV2	369	412	0.02%	0.003%
66	10.201	2754	2756	2765	rVB2	332	297	0.01%	0.002%
67	10.407	2817	2820	2823	rBV	285	229	0.01%	0.002%
68	10.484	2840	2844	2847	rBV	273	218	0.01%	0.002%
69	10.510	2848	2852	2856	rVV2	278	245	0.01%	0.002%
70	10.671	2895	2902	2912	rVB3	2594	3325	0.13%	0.026%
71	10.758	2916	2929	2951	rVV	416976	674605	26.21%	5.277%
72	10.857	2957	2960	2965	rBV2	433	410	0.02%	0.003%
73	10.893	2967	2971	2978	rVV4	1401	1379	0.05%	0.011%
74	11.118	3036	3041	3042	rBV2	363	273	0.01%	0.002%
75	11.314	3099	3102	3106	rBV2	308	243	0.01%	0.002%
76	11.414	3131	3133	3140	rVB	308	233	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048222.D
 Acq On : 22 Apr 2022 14:10
 Operator : SY/MD
 Sample : N2485-14DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3158	rVB4	1482	2522	0.10%	0.020%
78	11.574	3180	3183	3188	rVV2	272	246	0.01%	0.002%
79	11.635	3197	3202	3206	rVB2	211	221	0.01%	0.002%
80	11.693	3217	3220	3225	rVB	520	421	0.02%	0.003%
81	11.748	3225	3237	3247	rBV	200705	314873	12.23%	2.463%
82	11.835	3247	3264	3284	rVB2	857783	2189246	85.05%	17.124%
83	11.967	3302	3305	3315	rVB5	2294	2701	0.10%	0.021%
84	12.211	3360	3381	3399	rBV2	1203418	2574012	100.00%	20.134%
85	12.397	3436	3439	3442	rBV2	408	222	0.01%	0.002%
86	12.475	3460	3463	3470	rBV3	448	555	0.02%	0.004%
87	12.545	3482	3485	3489	rVB3	404	318	0.01%	0.002%
88	12.574	3489	3494	3495	rBV2	311	239	0.01%	0.002%
89	12.671	3520	3524	3525	rBV2	328	264	0.01%	0.002%
90	12.777	3548	3557	3563	rVB4	1288	2347	0.09%	0.018%
91	12.970	3613	3617	3618	rBV2	835	498	0.02%	0.004%
92	13.037	3635	3638	3642	rBV3	394	350	0.01%	0.003%
93	13.323	3725	3727	3729	rBV	474	289	0.01%	0.002%
94	13.336	3729	3731	3735	rVB2	825	512	0.02%	0.004%
95	13.404	3748	3752	3756	rBV2	380	446	0.02%	0.003%
96	13.613	3813	3817	3819	rBV2	396	337	0.01%	0.003%
97	13.841	3876	3888	3909	rBV	183990	293231	11.39%	2.294%
98	14.095	3959	3967	3976	rVB2	883	1627	0.06%	0.013%
99	14.330	4030	4040	4056	rBV	76507	120727	4.69%	0.944%
100	16.002	4555	4560	4565	rBV5	1630	2181	0.08%	0.017%




Sum of corrected areas: 12784505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048222.D
Acq On : 22 Apr 2022 14:10
Operator : SY/MD
Sample : N2485-14DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

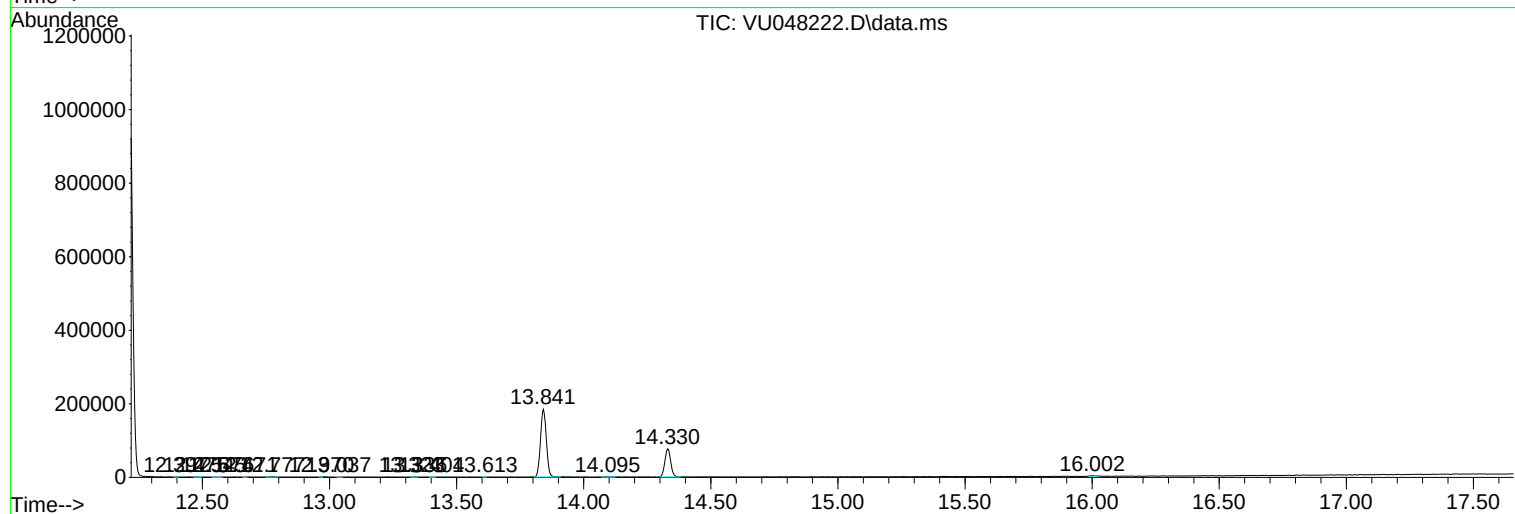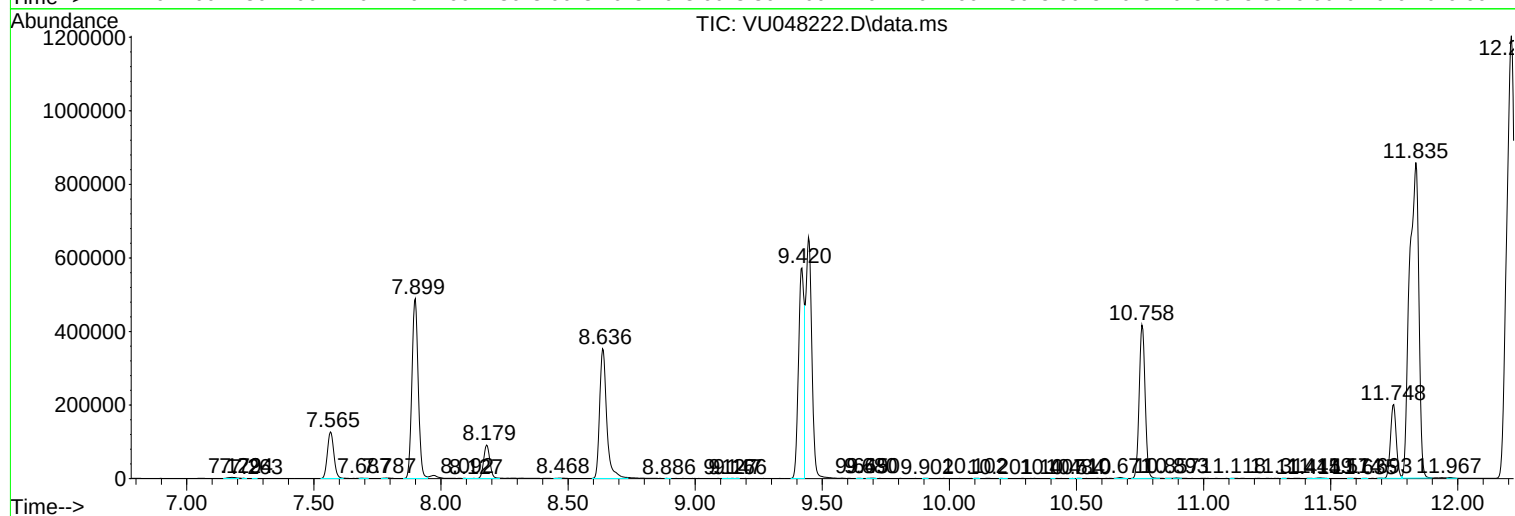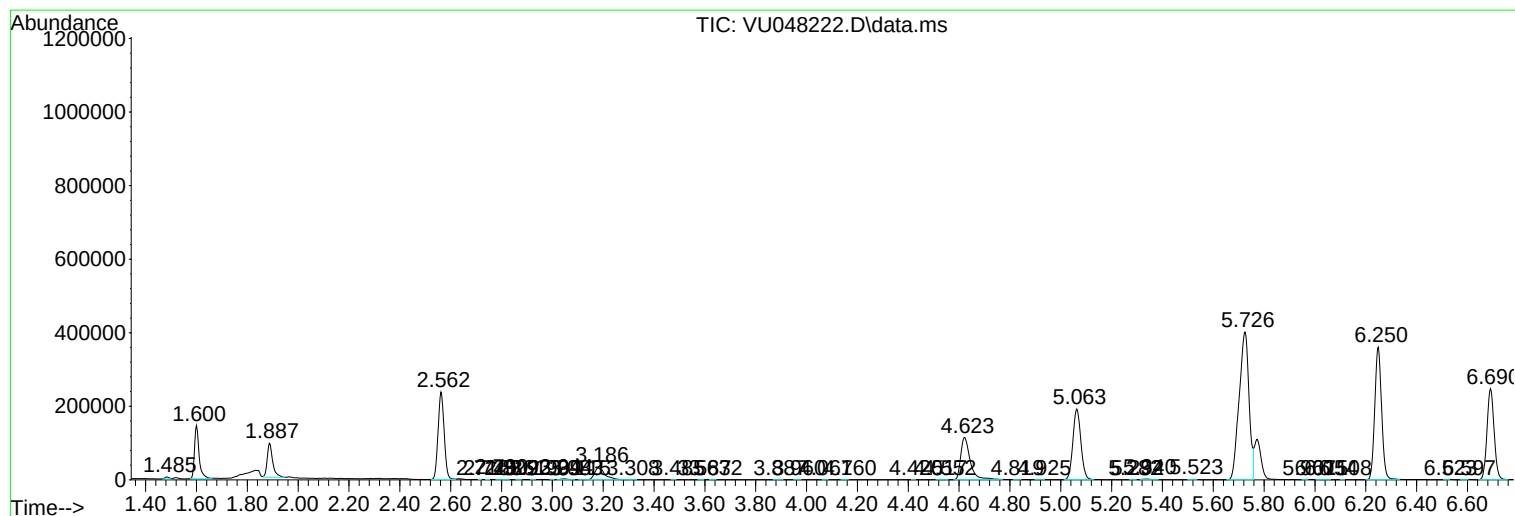

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048222.D
Acq On : 22 Apr 2022 14:10
Operator : SY/MD
Sample : N2485-14DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048222.D
Acq On : 22 Apr 2022 14:10
Operator : SY/MD
Sample : N2485-14DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------