

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048224.D
 Acq On : 22 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2485-15DL2 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	52	rBV3	4218	5845	0.51%	0.062%
2	1.600	73	81	99	rBV	130012	174767	15.16%	1.839%
3	1.877	162	167	182	rVB	87684	128343	11.13%	1.351%
4	2.559	366	379	396	rBV	236224	387596	33.62%	4.079%
5	2.674	413	415	420	rVB2	425	291	0.03%	0.003%
6	2.764	439	443	445	rBV3	584	450	0.04%	0.005%
7	2.874	474	477	481	rVB3	621	583	0.05%	0.006%
8	2.903	484	486	490	rVV2	231	221	0.02%	0.002%
9	3.044	520	530	544	rBV2	8194	17068	1.48%	0.180%
10	3.182	557	573	587	rBV2	15418	34936	3.03%	0.368%
11	3.295	605	608	613	rBV2	232	237	0.02%	0.002%
12	3.327	613	618	621	rBV3	248	275	0.02%	0.003%
13	3.362	626	629	632	rBV2	390	330	0.03%	0.003%
14	3.385	634	636	638	rVV	346	186	0.02%	0.002%
15	3.398	638	640	646	rVB3	339	241	0.02%	0.003%
16	3.462	657	660	665	rVB3	293	227	0.02%	0.002%
17	3.491	665	669	670	rBV	204	159	0.01%	0.002%
18	3.501	670	672	677	rVB	284	173	0.02%	0.002%
19	3.588	696	699	702	rVB3	299	239	0.02%	0.003%
20	3.710	735	737	739	rBV	313	202	0.02%	0.002%
21	3.858	776	783	787	rBV2	237	335	0.03%	0.004%
22	3.909	793	799	803	rBV	308	357	0.03%	0.004%
23	4.366	935	941	944	rBV2	158	195	0.02%	0.002%
24	4.452	963	968	970	rBV2	224	215	0.02%	0.002%
25	4.549	996	998	1003	rVB2	228	168	0.01%	0.002%
26	4.623	1008	1021	1048	rBV	109485	286463	24.85%	3.015%
27	4.957	1121	1125	1128	rBV2	275	187	0.02%	0.002%
28	5.063	1141	1158	1175	rBV	190545	415753	36.06%	4.375%
29	5.285	1221	1227	1231	rBV3	574	772	0.07%	0.008%
30	5.340	1231	1244	1259	rVV2	2481	6381	0.55%	0.067%
31	5.723	1343	1363	1372	rBV2	402999	1089265	94.48%	11.463%
32	5.967	1432	1439	1441	rBV4	1777	1981	0.17%	0.021%
33	6.034	1455	1460	1465	rVV2	371	395	0.03%	0.004%
34	6.150	1492	1496	1498	rBV	397	311	0.03%	0.003%
35	6.247	1512	1526	1553	rBV	358257	685455	59.45%	7.214%
36	6.526	1606	1613	1623	rBV5	1104	1714	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048224.D
 Acq On : 22 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2485-15DL2 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.594	1627	1634	1636	rBV4	1067	1192	0.10%	0.013%
38	6.690	1650	1664	1685	rBV	249060	485774	42.13%	5.112%
39	6.796	1694	1697	1698	rBV2	373	204	0.02%	0.002%
40	7.031	1765	1770	1774	rBV4	350	388	0.03%	0.004%
41	7.057	1774	1778	1781	rBV3	244	205	0.02%	0.002%
42	7.112	1792	1795	1800	rBV2	264	261	0.02%	0.003%
43	7.176	1804	1815	1824	rBV3	3877	8170	0.71%	0.086%
44	7.285	1841	1849	1855	rBV2	307	365	0.03%	0.004%
45	7.388	1877	1881	1886	rVB	243	186	0.02%	0.002%
46	7.462	1901	1904	1909	rVV2	172	183	0.02%	0.002%
47	7.488	1909	1912	1915	rVV2	191	169	0.01%	0.002%
48	7.565	1923	1936	1960	rBV	127023	221401	19.20%	2.330%
49	7.687	1966	1974	1979	rBV4	1001	1319	0.11%	0.014%
50	7.742	1986	1991	1994	rBV3	317	277	0.02%	0.003%
51	7.780	1998	2003	2004	rBV2	737	504	0.04%	0.005%
52	7.899	2026	2040	2055	rBV	469858	816436	70.82%	8.592%
53	8.089	2097	2099	2104	rVB3	433	357	0.03%	0.004%
54	8.179	2116	2127	2141	rBV	88970	148570	12.89%	1.564%
55	8.398	2192	2195	2199	rVB3	447	305	0.03%	0.003%
56	8.468	2206	2217	2227	rBV3	4999	9369	0.81%	0.099%
57	8.639	2257	2270	2308	rBV	353567	680191	59.00%	7.158%
58	8.829	2327	2329	2337	rVB4	303	337	0.03%	0.004%
59	8.944	2354	2365	2368	rBV2	389	638	0.06%	0.007%
60	8.970	2371	2373	2378	rVV2	289	187	0.02%	0.002%
61	9.018	2382	2388	2390	rVV3	290	312	0.03%	0.003%
62	9.031	2390	2392	2398	rVB3	355	285	0.02%	0.003%
63	9.118	2415	2419	2423	rBV3	327	279	0.02%	0.003%
64	9.240	2453	2457	2460	rBV	314	241	0.02%	0.003%
65	9.337	2485	2487	2489	rBV	291	155	0.01%	0.002%
66	9.420	2498	2513	2516	rBV	581594	881157	76.43%	9.273%
67	9.607	2566	2571	2576	rBV3	340	387	0.03%	0.004%
68	9.693	2592	2598	2605	rBV3	852	1057	0.09%	0.011%
69	9.873	2652	2654	2658	rVB	253	157	0.01%	0.002%
70	9.986	2685	2689	2691	rBV	247	155	0.01%	0.002%
71	10.102	2722	2725	2730	rVV2	345	301	0.03%	0.003%
72	10.465	2835	2838	2840	rBV	202	168	0.01%	0.002%
73	10.671	2895	2902	2911	rVB4	2063	3236	0.28%	0.034%
74	10.758	2915	2929	2958	rVB	424396	680048	58.99%	7.157%
75	10.893	2958	2971	2982	rBV	8093	14297	1.24%	0.150%
76	10.967	2990	2994	2997	rVB	374	245	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048224.D
 Acq On : 22 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2485-15DL2 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.012	3004	3008	3011	rBV3	452	358	0.03%	0.004%
78	11.050	3018	3020	3024	rVB	376	203	0.02%	0.002%
79	11.111	3035	3039	3041	rBV2	331	292	0.03%	0.003%
80	11.179	3056	3060	3065	rVB2	364	313	0.03%	0.003%
81	11.398	3125	3128	3129	rBV	242	166	0.01%	0.002%
82	11.449	3137	3144	3145	rBV	1012	739	0.06%	0.008%
83	11.693	3216	3220	3226	rVB3	988	1084	0.09%	0.011%
84	11.748	3227	3237	3245	rBV2	9209	13980	1.21%	0.147%
85	11.816	3245	3258	3283	rVV2	557578	1152908	100.00%	12.133%
86	11.970	3303	3306	3317	rVB5	1744	2586	0.22%	0.027%
87	12.028	3321	3324	3326	rBV	243	162	0.01%	0.002%
88	12.105	3345	3348	3351	rBV2	353	318	0.03%	0.003%
89	12.195	3358	3376	3406	rBV2	530484	1103727	95.73%	11.616%
90	12.324	3412	3416	3419	rBV4	521	402	0.03%	0.004%
91	12.359	3425	3427	3431	rBV3	250	189	0.02%	0.002%
92	12.426	3446	3448	3455	rVB3	373	424	0.04%	0.004%
93	12.603	3499	3503	3507	rVB3	462	475	0.04%	0.005%
94	12.639	3508	3514	3517	rVV4	516	551	0.05%	0.006%
95	12.684	3526	3528	3531	rBV2	230	173	0.02%	0.002%
96	12.770	3548	3555	3565	rVB2	2931	4652	0.40%	0.049%
97	13.224	3695	3696	3699	rBV	365	166	0.01%	0.002%
98	13.848	3881	3890	3901	rBV2	8016	12253	1.06%	0.129%
99	14.333	4035	4041	4052	rVB6	2274	3898	0.34%	0.041%
100	14.835	4195	4197	4199	rBV	423	254	0.02%	0.003%




Sum of corrected areas: 9502057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048224.D
Acq On : 22 Apr 2022 14:58
Operator : SY/MD
Sample : N2485-15DL2 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

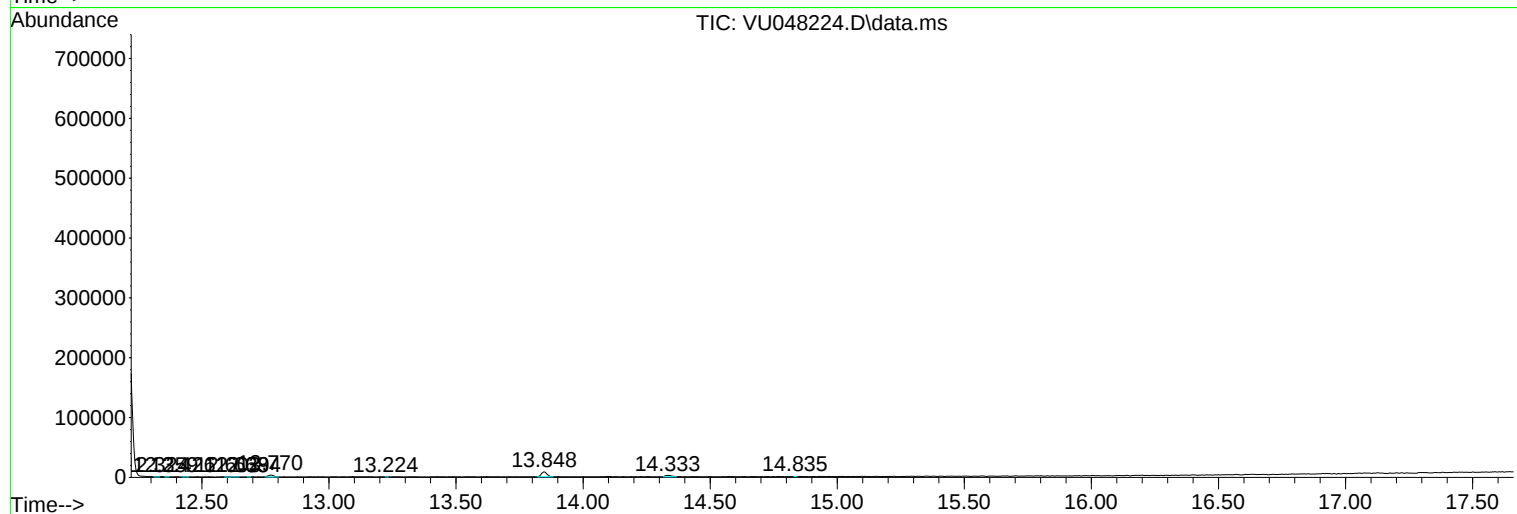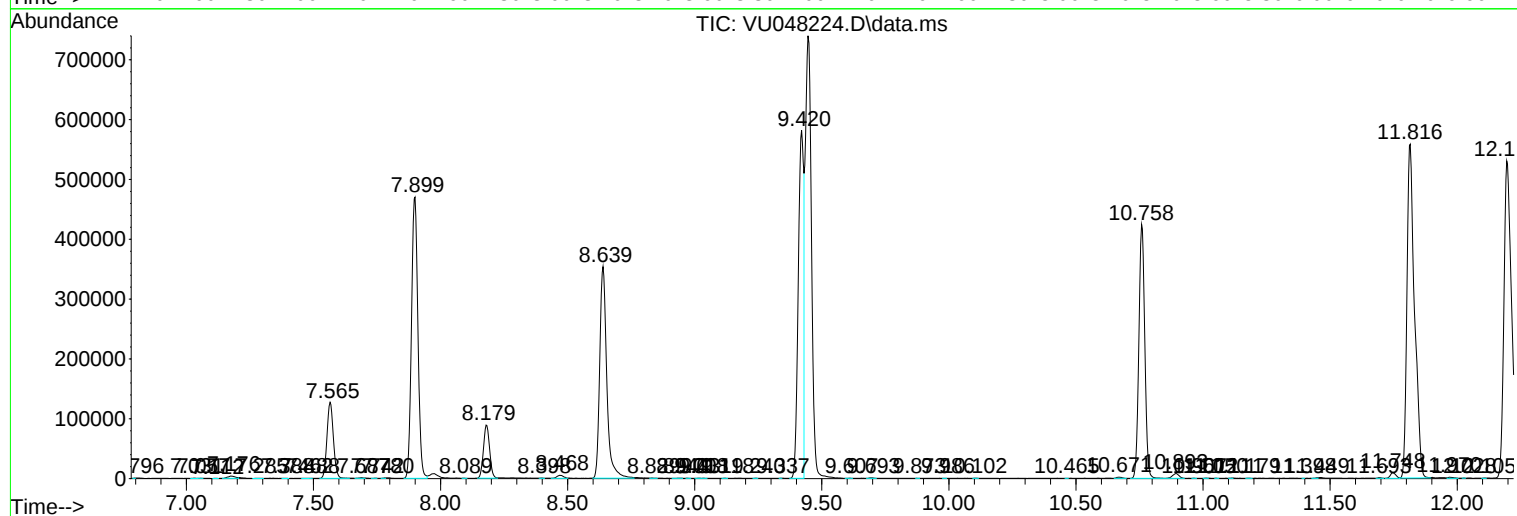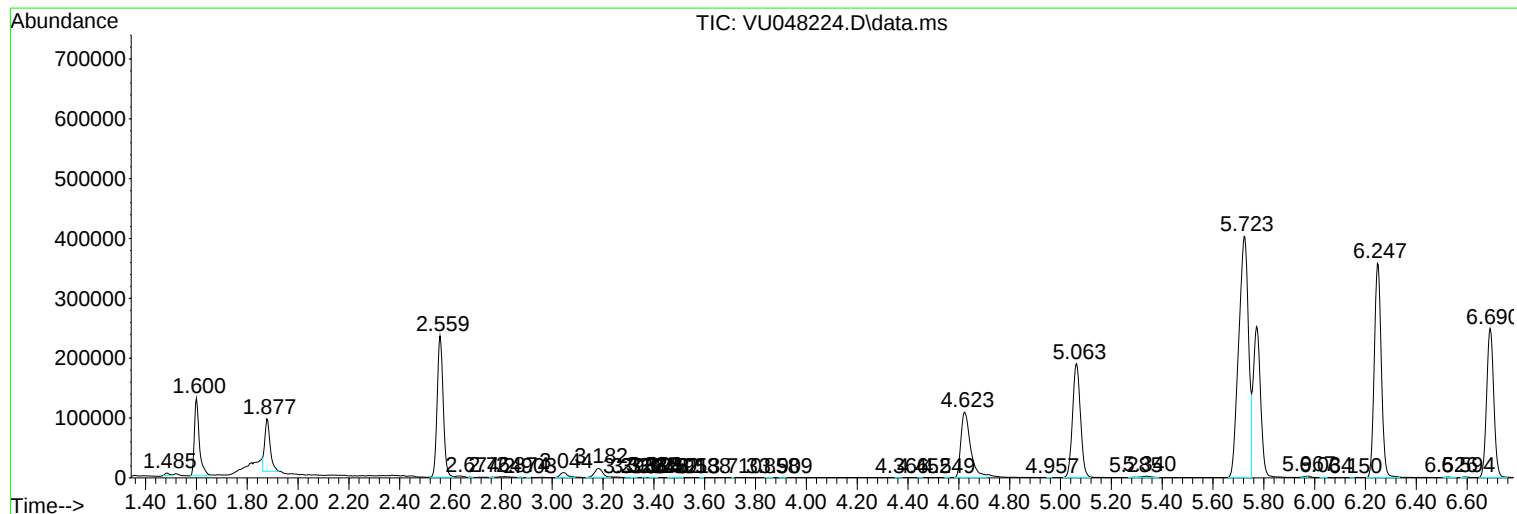

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048224.D
Acq On : 22 Apr 2022 14:58
Operator : SY/MD
Sample : N2485-15DL2 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048224.D
Acq On : 22 Apr 2022 14:58
Operator : SY/MD
Sample : N2485-15DL2 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------