

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048226.D
 Acq On : 22 Apr 2022 15:45
 Operator : SY/MD
 Sample : N2486-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	52	rBV3	4063	5538	0.51%	0.062%
2	1.601	73	81	98	rBV	127019	175160	16.07%	1.972%
3	1.877	161	167	197	rVB	98073	155470	14.27%	1.750%
4	2.556	364	378	398	rBV	229900	385428	35.37%	4.339%
5	2.723	427	430	432	rBV3	536	336	0.03%	0.004%
6	2.777	442	447	448	rBV3	740	678	0.06%	0.008%
7	2.816	454	459	469	rVB5	2199	3508	0.32%	0.039%
8	2.880	477	479	485	rVB3	439	358	0.03%	0.004%
9	2.909	485	488	494	rVB	586	393	0.04%	0.004%
10	2.957	495	503	508	rBV3	586	815	0.07%	0.009%
11	3.047	520	531	541	rVB6	1788	3443	0.32%	0.039%
12	3.089	542	544	548	rVB2	423	302	0.03%	0.003%
13	3.118	548	553	557	rBV3	484	567	0.05%	0.006%
14	3.182	557	573	587	rBV2	7659	17582	1.61%	0.198%
15	3.330	615	619	626	rVV	266	242	0.02%	0.003%
16	3.408	638	643	646	rBV	1365	936	0.09%	0.011%
17	3.453	653	657	660	rBV	1068	711	0.07%	0.008%
18	3.523	673	679	683	rBV	1174	964	0.09%	0.011%
19	3.549	684	687	690	rBV	841	538	0.05%	0.006%
20	3.568	690	693	696	rBV2	748	546	0.05%	0.006%
21	3.613	704	707	708	rBV	810	534	0.05%	0.006%
22	3.674	722	726	730	rBV	692	590	0.05%	0.007%
23	3.697	730	733	736	rBV	936	478	0.04%	0.005%
24	3.752	744	750	756	rBV	995	1052	0.10%	0.012%
25	3.777	756	758	762	rVB	363	237	0.02%	0.003%
26	3.800	762	765	769	rVB	559	369	0.03%	0.004%
27	3.826	769	773	777	rBV2	440	399	0.04%	0.004%
28	3.848	777	780	783	rVV	370	276	0.03%	0.003%
29	3.887	787	792	799	rVB2	900	1010	0.09%	0.011%
30	3.967	813	817	822	rBV2	702	625	0.06%	0.007%
31	4.118	858	864	866	rBV	239	227	0.02%	0.003%
32	4.221	893	896	902	rVB2	245	221	0.02%	0.002%
33	4.507	976	985	989	rBV2	248	357	0.03%	0.004%
34	4.623	1008	1021	1073	rBV	109751	302004	27.71%	3.400%
35	4.838	1086	1088	1091	rBV2	352	226	0.02%	0.003%
36	4.973	1127	1130	1133	rVB3	326	223	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048226.D
 Acq On : 22 Apr 2022 15:45
 Operator : SY/MD
 Sample : N2486-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.063	1136	1158	1182	rBV	191068	419942	38.53%	4.728%
38	5.192	1193	1198	1204	rBV2	225	232	0.02%	0.003%
39	5.289	1221	1228	1231	rBV3	696	1023	0.09%	0.012%
40	5.330	1235	1241	1242	rBV2	1239	1128	0.10%	0.013%
41	5.723	1341	1363	1392	rBV2	410543	1089779	100.00%	12.268%
42	5.967	1431	1439	1442	rBV3	2367	3118	0.29%	0.035%
43	6.038	1458	1461	1465	rVB2	270	210	0.02%	0.002%
44	6.067	1465	1470	1472	rBV2	229	212	0.02%	0.002%
45	6.179	1502	1505	1508	rBV	377	209	0.02%	0.002%
46	6.247	1508	1526	1546	rBV	349828	665751	61.09%	7.495%
47	6.523	1605	1612	1620	rVB5	1291	1735	0.16%	0.020%
48	6.597	1628	1635	1643	rBV3	1192	1874	0.17%	0.021%
49	6.690	1649	1664	1688	rBV	243525	473108	43.41%	5.326%
50	6.803	1695	1699	1706	rVB2	479	582	0.05%	0.007%
51	6.899	1725	1729	1733	rBV	218	267	0.02%	0.003%
52	7.051	1773	1776	1777	rVV2	322	232	0.02%	0.003%
53	7.060	1777	1779	1784	rVB3	581	381	0.03%	0.004%
54	7.176	1805	1815	1835	rBV3	4392	10781	0.99%	0.121%
55	7.317	1856	1859	1863	rBV2	357	235	0.02%	0.003%
56	7.340	1863	1866	1870	rVB2	320	208	0.02%	0.002%
57	7.414	1885	1889	1893	rVB2	277	233	0.02%	0.003%
58	7.565	1923	1936	1954	rBV	127798	222361	20.40%	2.503%
59	7.677	1966	1971	1972	rBV2	458	406	0.04%	0.005%
60	7.690	1972	1975	1981	rVB3	763	858	0.08%	0.010%
61	7.800	2006	2009	2012	rVV2	375	293	0.03%	0.003%
62	7.899	2025	2040	2055	rBV	477901	832601	76.40%	9.373%
63	8.034	2079	2082	2090	rVB3	496	568	0.05%	0.006%
64	8.086	2096	2098	2105	rVB2	468	394	0.04%	0.004%
65	8.179	2112	2127	2145	rBV	87038	150142	13.78%	1.690%
66	8.346	2177	2179	2182	rVB2	492	287	0.03%	0.003%
67	8.366	2182	2185	2190	rBV3	408	398	0.04%	0.004%
68	8.423	2201	2203	2206	rVB	383	228	0.02%	0.003%
69	8.475	2214	2219	2222	rVV3	478	457	0.04%	0.005%
70	8.517	2229	2232	2237	rVB2	309	280	0.03%	0.003%
71	8.639	2256	2270	2302	rBV	355138	689834	63.30%	7.766%
72	8.793	2317	2318	2323	rVB4	328	236	0.02%	0.003%
73	8.928	2357	2360	2363	rBV	397	292	0.03%	0.003%
74	8.973	2370	2374	2378	rVB2	363	365	0.03%	0.004%
75	9.224	2446	2452	2461	rVB2	321	462	0.04%	0.005%
76	9.417	2498	2512	2538	rBV	526016	914046	83.87%	10.290%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048226.D
 Acq On : 22 Apr 2022 15:45
 Operator : SY/MD
 Sample : N2486-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.571	2555	2560	2564	rBV2	469	552	0.05%	0.006%
78	9.697	2592	2599	2607	rBV4	608	1041	0.10%	0.012%
79	9.877	2649	2655	2660	rBV2	280	349	0.03%	0.004%
80	10.407	2816	2820	2826	rVB2	232	231	0.02%	0.003%
81	10.674	2895	2903	2911	rVB4	2039	2809	0.26%	0.032%
82	10.758	2916	2929	2946	rBV	426157	686572	63.00%	7.729%
83	10.864	2958	2962	2963	rBV2	383	283	0.03%	0.003%
84	10.890	2967	2970	2971	rBV2	546	345	0.03%	0.004%
85	10.925	2979	2981	2985	rVB2	377	206	0.02%	0.002%
86	10.951	2985	2989	2994	rBV2	344	257	0.02%	0.003%
87	11.420	3131	3135	3140	rVB3	390	346	0.03%	0.004%
88	11.462	3140	3148	3158	rBV6	1420	2566	0.24%	0.029%
89	11.697	3219	3221	3230	rVB6	698	631	0.06%	0.007%
90	11.748	3230	3237	3245	rBV3	1825	2492	0.23%	0.028%
91	11.812	3245	3257	3282	rBV	515464	853334	78.30%	9.607%
92	11.941	3294	3297	3301	rVB4	619	455	0.04%	0.005%
93	11.963	3301	3304	3307	rBV5	650	569	0.05%	0.006%
94	12.195	3362	3376	3397	rBV	464560	775806	71.19%	8.734%
95	12.494	3466	3469	3472	rBV2	404	271	0.02%	0.003%
96	12.639	3510	3514	3518	rBV2	533	484	0.04%	0.005%
97	12.771	3546	3555	3564	rBV3	1180	2005	0.18%	0.023%
98	12.870	3583	3586	3588	rBV2	316	266	0.02%	0.003%
99	13.179	3679	3682	3686	rBV3	325	281	0.03%	0.003%
100	13.851	3885	3891	3899	rVB4	1884	2512	0.23%	0.028%




Sum of corrected areas: 8882754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048226.D
Acq On : 22 Apr 2022 15:45
Operator : SY/MD
Sample : N2486-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

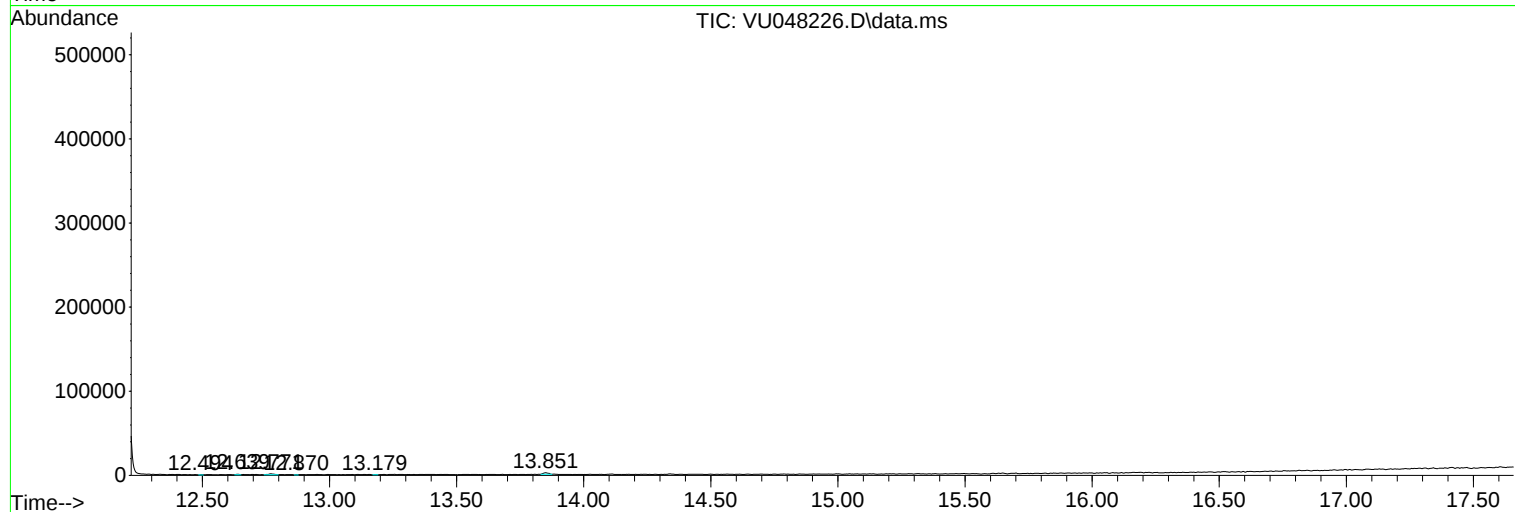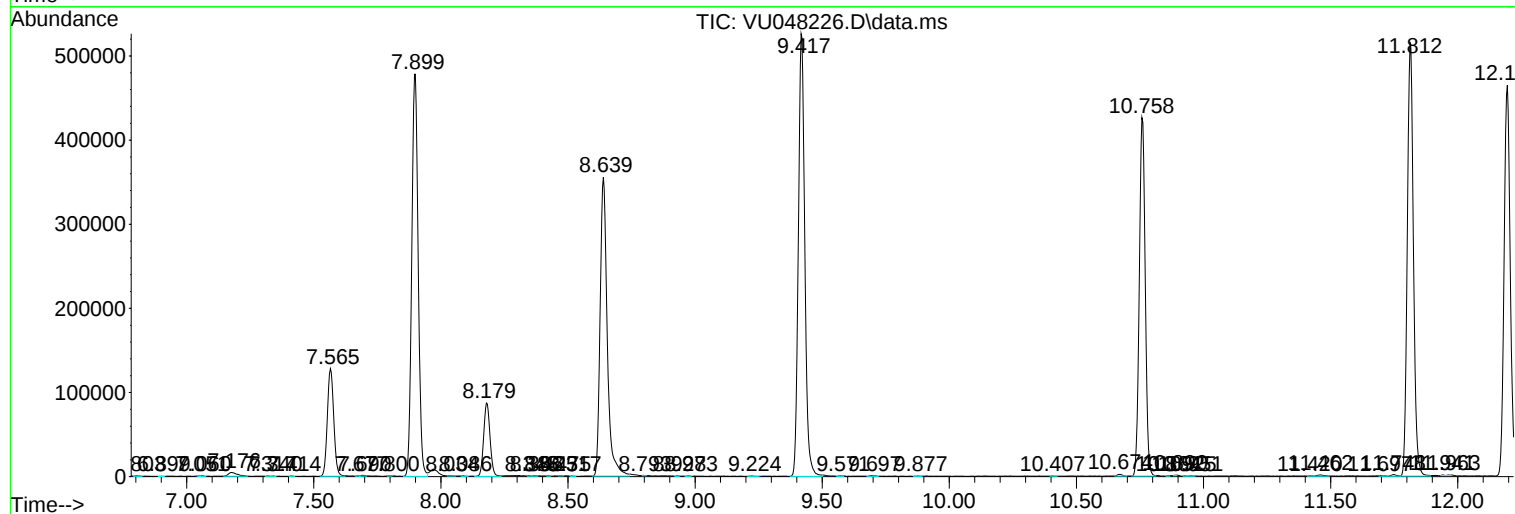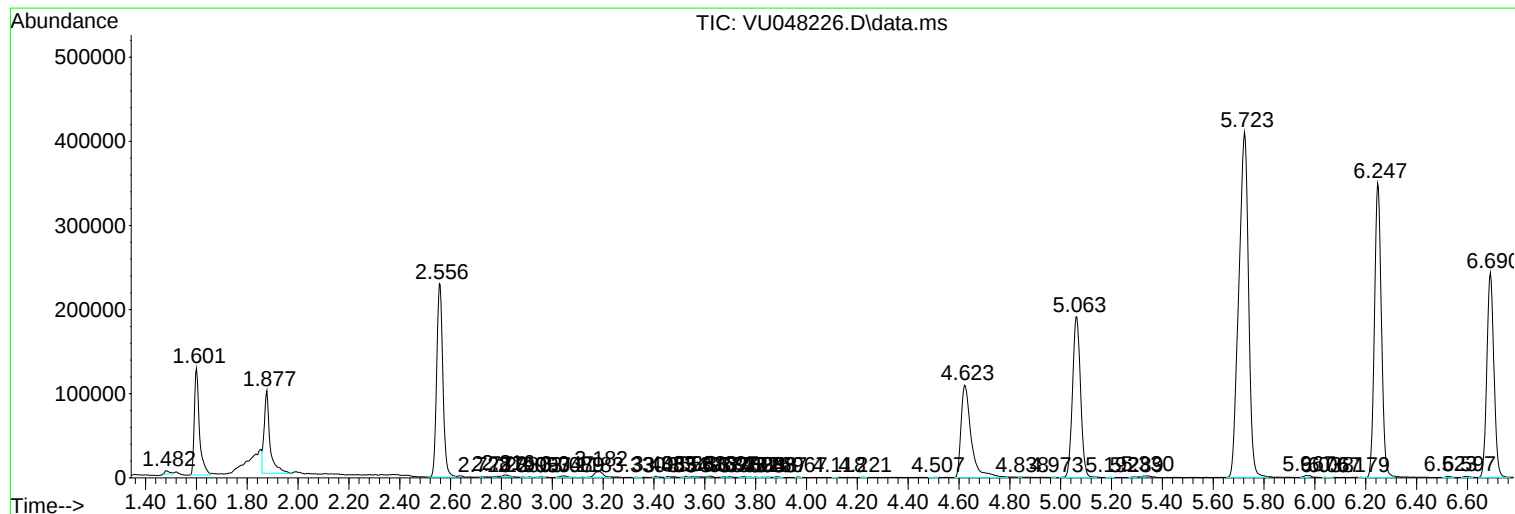

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048226.D
Acq On : 22 Apr 2022 15:45
Operator : SY/MD
Sample : N2486-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048226.D
Acq On : 22 Apr 2022 15:45
Operator : SY/MD
Sample : N2486-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
