

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048230.D
 Acq On : 22 Apr 2022 17:20
 Operator : SY/MD
 Sample : N2486-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rVB4	4245	4397	0.25%	0.039%
2	1.601	73	81	98	rBV	124730	159366	9.22%	1.428%
3	1.893	165	172	186	rVB	89098	126516	7.32%	1.133%
4	2.562	368	380	394	rBV	218109	364846	21.10%	3.269%
5	2.681	411	417	428	rVB2	7186	11869	0.69%	0.106%
6	2.771	428	445	477	rBV	712942	1728741	100.00%	15.487%
7	3.269	597	600	605	rVB4	643	454	0.03%	0.004%
8	3.726	739	742	747	rVB2	272	192	0.01%	0.002%
9	3.771	753	756	760	rVB2	361	284	0.02%	0.003%
10	3.848	776	780	781	rBV	336	209	0.01%	0.002%
11	3.858	781	783	788	rVV3	334	296	0.02%	0.003%
12	3.887	788	792	797	rVB3	416	411	0.02%	0.004%
13	4.157	870	876	879	rBV2	211	246	0.01%	0.002%
14	4.472	967	974	975	rBV2	356	429	0.02%	0.004%
15	4.504	978	984	992	rVB2	330	381	0.02%	0.003%
16	4.620	1007	1020	1046	rBV	123125	302170	17.48%	2.707%
17	4.909	1107	1110	1114	rBV2	450	262	0.02%	0.002%
18	4.993	1127	1136	1137	rBV2	337	383	0.02%	0.003%
19	5.002	1137	1139	1141	rVV2	334	228	0.01%	0.002%
20	5.063	1141	1158	1185	rVV	199739	433695	25.09%	3.885%
21	5.205	1193	1202	1214	rBV2	2837	5939	0.34%	0.053%
22	5.289	1224	1228	1229	rBV2	292	233	0.01%	0.002%
23	5.334	1237	1242	1256	rVB4	1873	4000	0.23%	0.036%
24	5.424	1268	1270	1278	rVB	233	197	0.01%	0.002%
25	5.491	1288	1291	1297	rBV	226	231	0.01%	0.002%
26	5.552	1305	1310	1313	rBV2	281	245	0.01%	0.002%
27	5.726	1339	1364	1375	rBV2	402802	1112921	64.38%	9.970%
28	5.964	1434	1438	1439	rBV	439	337	0.02%	0.003%
29	6.057	1465	1467	1471	rVB	335	215	0.01%	0.002%
30	6.102	1476	1481	1484	rBV2	349	346	0.02%	0.003%
31	6.189	1504	1508	1512	rBV2	211	223	0.01%	0.002%
32	6.250	1512	1527	1547	rBV	375142	707299	40.91%	6.337%
33	6.401	1566	1574	1582	rVB8	2149	3614	0.21%	0.032%
34	6.456	1588	1591	1594	rVB2	340	257	0.01%	0.002%
35	6.494	1594	1603	1606	rBV3	385	395	0.02%	0.004%
36	6.536	1606	1616	1617	rBV4	1335	1878	0.11%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048230.D
 Acq On : 22 Apr 2022 17:20
 Operator : SY/MD
 Sample : N2486-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1685	rBV2	253967	490346	28.36%	4.393%
38	6.771	1685	1689	1690	rBV4	947	629	0.04%	0.006%
39	6.829	1705	1707	1710	rVB2	416	213	0.01%	0.002%
40	6.851	1710	1714	1718	rBV2	340	240	0.01%	0.002%
41	6.896	1725	1728	1731	rVV2	530	256	0.01%	0.002%
42	7.063	1774	1780	1782	rBV3	330	344	0.02%	0.003%
43	7.079	1782	1785	1789	rVV	221	200	0.01%	0.002%
44	7.186	1805	1818	1833	rVV5	9602	19200	1.11%	0.172%
45	7.411	1885	1888	1892	rBV	310	259	0.01%	0.002%
46	7.465	1902	1905	1909	rBV2	255	210	0.01%	0.002%
47	7.565	1924	1936	1957	rVV	110673	190982	11.05%	1.711%
48	7.684	1966	1973	1974	rBV2	1273	1275	0.07%	0.011%
49	7.742	1988	1991	1994	rVB3	350	196	0.01%	0.002%
50	7.790	2002	2006	2008	rBV2	457	420	0.02%	0.004%
51	7.899	2026	2040	2056	rVV	481703	816343	47.22%	7.313%
52	7.970	2057	2062	2074	rVB	9178	14654	0.85%	0.131%
53	8.137	2112	2114	2116	rBV	302	203	0.01%	0.002%
54	8.179	2116	2127	2147	rVV	79879	132917	7.69%	1.191%
55	8.346	2177	2179	2187	rVB3	408	508	0.03%	0.005%
56	8.382	2187	2190	2194	rVB	302	217	0.01%	0.002%
57	8.472	2205	2218	2227	rBV3	3134	5548	0.32%	0.050%
58	8.636	2255	2269	2303	rBV	372814	696447	40.29%	6.239%
59	8.983	2371	2377	2384	rBV3	1468	2040	0.12%	0.018%
60	9.169	2429	2435	2440	rVB2	346	296	0.02%	0.003%
61	9.208	2441	2447	2450	rBV2	320	289	0.02%	0.003%
62	9.282	2468	2470	2477	rVB2	320	274	0.02%	0.002%
63	9.420	2498	2513	2515	rBV	601294	846010	48.94%	7.579%
64	9.597	2566	2568	2571	rBV2	331	254	0.01%	0.002%
65	9.642	2581	2582	2586	rBV	278	208	0.01%	0.002%
66	9.697	2591	2599	2607	rBV4	1201	2265	0.13%	0.020%
67	9.816	2633	2636	2638	rVB2	401	205	0.01%	0.002%
68	9.922	2665	2669	2672	rBV2	285	202	0.01%	0.002%
69	10.147	2734	2739	2741	rBV3	278	279	0.02%	0.002%
70	10.298	2782	2786	2789	rVB2	350	244	0.01%	0.002%
71	10.372	2806	2809	2814	rVB2	298	248	0.01%	0.002%
72	10.414	2818	2822	2826	rBV	227	226	0.01%	0.002%
73	10.472	2836	2840	2846	rBV2	260	271	0.02%	0.002%
74	10.665	2897	2900	2905	rVV3	615	504	0.03%	0.005%
75	10.758	2915	2929	2956	rVB	427773	687152	39.75%	6.156%
76	10.896	2961	2972	2981	rBV2	3969	6642	0.38%	0.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048230.D
 Acq On : 22 Apr 2022 17:20
 Operator : SY/MD
 Sample : N2486-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.992	2994	3002	3006	rBV2	1507	1843	0.11%	0.017%
78	11.452	3143	3145	3148	rBV2	382	297	0.02%	0.003%
79	11.745	3224	3236	3246	rBV	153222	242155	14.01%	2.169%
80	11.816	3246	3258	3260	rBV	590383	826168	47.79%	7.401%
81	11.976	3304	3308	3312	rVB2	828	625	0.04%	0.006%
82	12.066	3327	3336	3349	rBV5	5085	9731	0.56%	0.087%
83	12.195	3363	3376	3395	rBV2	531128	1067362	61.74%	9.562%
84	12.526	3476	3479	3482	rBV2	309	218	0.01%	0.002%
85	12.555	3482	3488	3490	rBV3	491	453	0.03%	0.004%
86	12.639	3509	3514	3520	rVB3	349	387	0.02%	0.003%
87	12.677	3521	3526	3529	rBV3	459	309	0.02%	0.003%
88	12.709	3533	3536	3537	rBV	318	192	0.01%	0.002%
89	12.774	3547	3556	3563	rBV3	1961	3163	0.18%	0.028%
90	12.854	3577	3581	3583	rBV3	273	238	0.01%	0.002%
91	12.976	3613	3619	3627	rVB5	843	1257	0.07%	0.011%
92	13.160	3665	3676	3687	rVB5	1980	3975	0.23%	0.036%
93	13.227	3687	3697	3704	rBV4	1821	2801	0.16%	0.025%
94	13.443	3761	3764	3767	rVB2	459	317	0.02%	0.003%
95	13.465	3767	3771	3774	rBV2	339	286	0.02%	0.003%
96	13.841	3877	3888	3908	rVB2	61880	99804	5.77%	0.894%
97	14.050	3950	3953	3956	rBV2	301	215	0.01%	0.002%
98	14.333	4034	4041	4051	rVB3	4896	7075	0.41%	0.063%
99	14.629	4130	4133	4135	rBV2	370	241	0.01%	0.002%
100	14.925	4223	4225	4227	rBV	543	241	0.01%	0.002%




Sum of corrected areas: 11162274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048230.D
Acq On : 22 Apr 2022 17:20
Operator : SY/MD
Sample : N2486-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

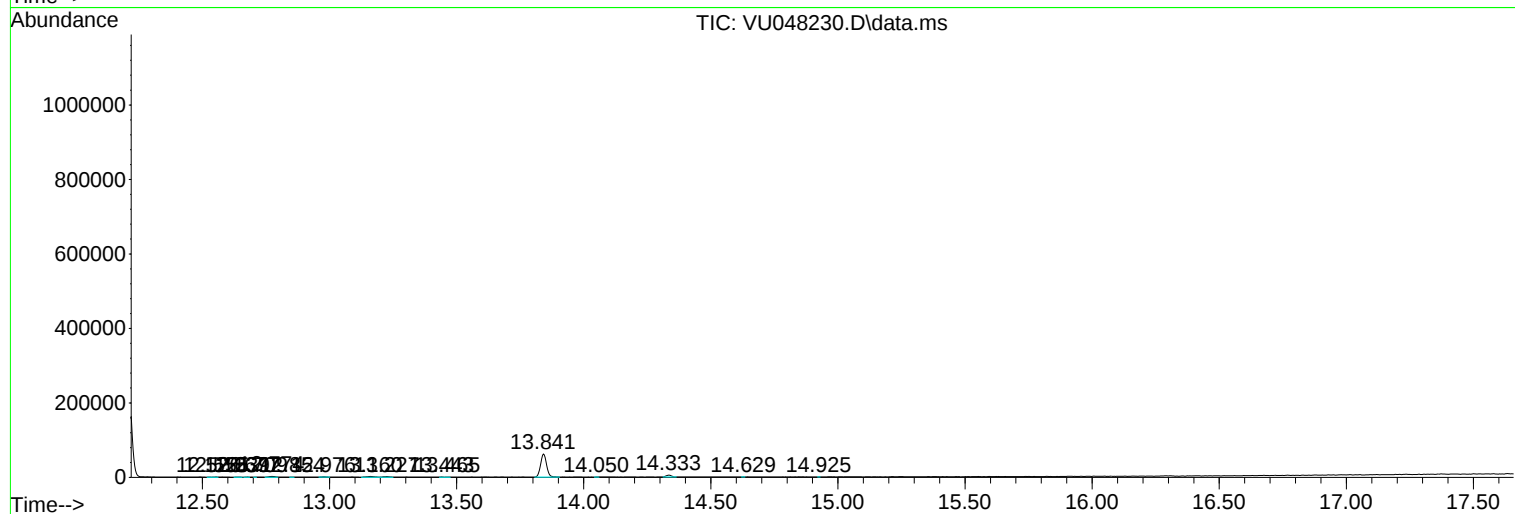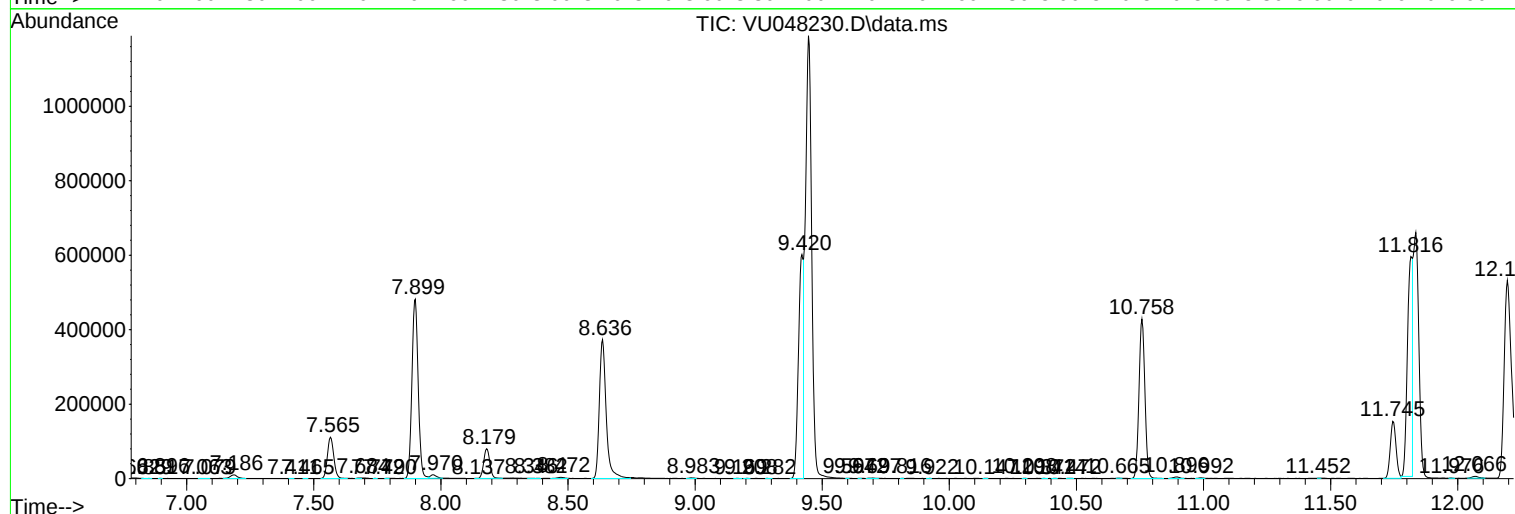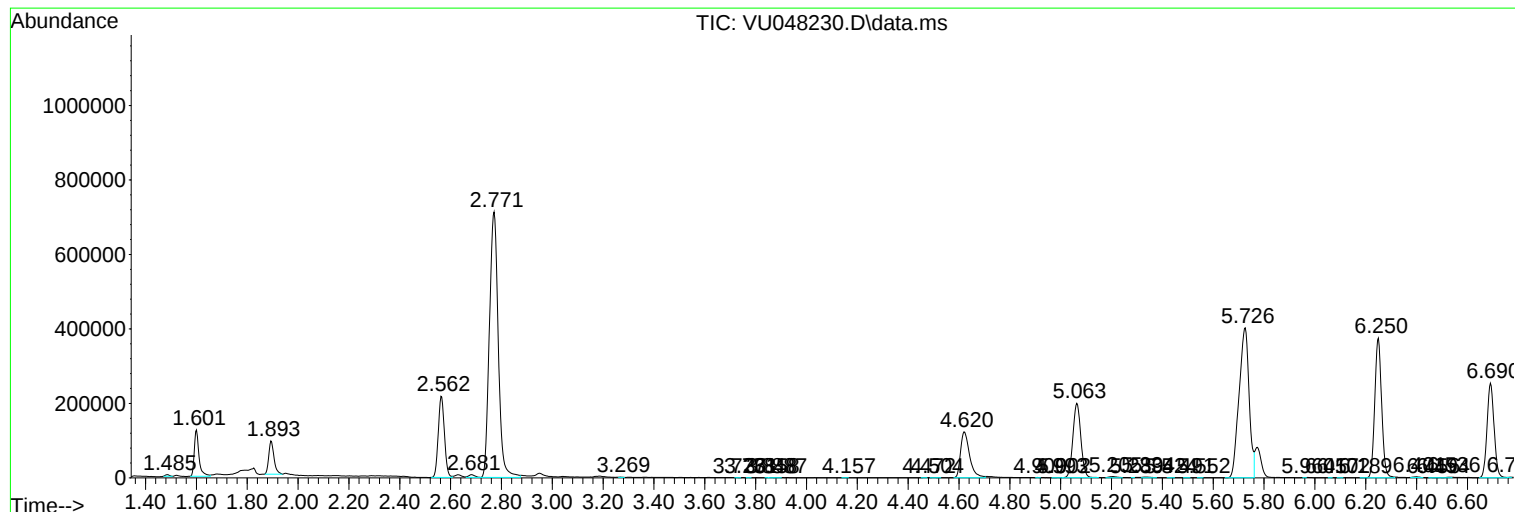

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048230.D
Acq On : 22 Apr 2022 17:20
Operator : SY/MD
Sample : N2486-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048230.D
Acq On : 22 Apr 2022 17:20
Operator : SY/MD
Sample : N2486-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------