

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048233.D
 Acq On : 22 Apr 2022 18:32
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	39	46	53	rBV2	6271	10495	0.30%	0.071%
2	1.600	73	81	96	rBV	137825	175305	4.98%	1.180%
3	1.893	164	172	187	rVB	94273	140371	3.99%	0.945%
4	2.456	345	347	351	rVB2	672	348	0.01%	0.002%
5	2.562	368	380	396	rBV	225352	374596	10.64%	2.521%
6	2.697	420	422	426	rBV	275	212	0.01%	0.001%
7	2.790	446	451	454	rVV3	966	1047	0.03%	0.007%
8	2.948	496	500	502	rBV2	502	387	0.01%	0.003%
9	2.996	512	515	519	rVB2	331	216	0.01%	0.001%
10	3.047	521	531	541	rBV5	2881	5790	0.16%	0.039%
11	3.115	550	552	555	rVB2	379	239	0.01%	0.002%
12	3.137	555	559	561	rBV	253	213	0.01%	0.001%
13	3.186	561	574	596	rVB2	7802	18851	0.54%	0.127%
14	3.478	660	665	673	rBV	359	420	0.01%	0.003%
15	3.536	679	683	685	rBV	241	192	0.01%	0.001%
16	3.616	704	708	711	rBV3	437	242	0.01%	0.002%
17	3.645	715	717	725	rVB2	287	247	0.01%	0.002%
18	4.063	843	847	850	rBV	306	241	0.01%	0.002%
19	4.089	850	855	857	rBV2	275	294	0.01%	0.002%
20	4.118	862	864	869	rVB	327	214	0.01%	0.001%
21	4.234	896	900	908	rBV2	285	397	0.01%	0.003%
22	4.269	908	911	920	rVV2	291	268	0.01%	0.002%
23	4.620	1007	1020	1045	rBV	113915	280359	7.97%	1.886%
24	4.893	1101	1105	1108	rBV2	226	207	0.01%	0.001%
25	4.973	1124	1130	1134	rVB3	432	546	0.02%	0.004%
26	5.005	1134	1140	1141	rBV	244	240	0.01%	0.002%
27	5.063	1141	1158	1180	rVV	189344	416752	11.84%	2.804%
28	5.288	1223	1228	1233	rBV3	584	883	0.03%	0.006%
29	5.330	1236	1241	1244	rBV3	838	928	0.03%	0.006%
30	5.523	1292	1301	1302	rBV2	1009	1172	0.03%	0.008%
31	5.726	1338	1364	1372	rBV2	399158	1067092	30.32%	7.180%
32	5.970	1435	1440	1444	rBV5	819	763	0.02%	0.005%
33	6.041	1459	1462	1467	rVB3	383	354	0.01%	0.002%
34	6.157	1493	1498	1501	rBV2	209	181	0.01%	0.001%
35	6.250	1509	1527	1548	rBV	353099	663798	18.86%	4.467%
36	6.452	1587	1590	1595	rBV2	457	352	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048233.D
 Acq On : 22 Apr 2022 18:32
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.510	1604	1608	1609	rBV2	260	202	0.01%	0.001%
38	6.526	1609	1613	1617	rBV2	396	532	0.02%	0.004%
39	6.571	1624	1627	1628	rBV	325	187	0.01%	0.001%
40	6.642	1645	1649	1650	rBV2	364	254	0.01%	0.002%
41	6.690	1650	1664	1686	rVV	250064	485471	13.79%	3.267%
42	6.803	1695	1699	1700	rBV2	498	324	0.01%	0.002%
43	7.012	1758	1764	1766	rBV	378	346	0.01%	0.002%
44	7.038	1766	1772	1777	rBV3	297	354	0.01%	0.002%
45	7.176	1805	1815	1830	rBV5	2436	5696	0.16%	0.038%
46	7.279	1844	1847	1850	rBV	221	199	0.01%	0.001%
47	7.417	1885	1890	1892	rBV2	249	200	0.01%	0.001%
48	7.481	1905	1910	1913	rVB	291	248	0.01%	0.002%
49	7.520	1918	1922	1923	rBV	382	237	0.01%	0.002%
50	7.565	1924	1936	1959	rVB	125302	213952	6.08%	1.440%
51	7.645	1959	1961	1967	rVB2	557	477	0.01%	0.003%
52	7.677	1967	1971	1972	rBV	871	565	0.02%	0.004%
53	7.793	2003	2007	2013	rVB2	655	518	0.01%	0.003%
54	7.832	2013	2019	2020	rBV2	363	324	0.01%	0.002%
55	7.899	2026	2040	2056	rBV	464560	808886	22.98%	5.443%
56	7.970	2057	2062	2074	rVB2	7983	13063	0.37%	0.088%
57	8.179	2116	2127	2141	rBV	86399	144904	4.12%	0.975%
58	8.275	2154	2157	2160	rBV2	345	305	0.01%	0.002%
59	8.308	2165	2167	2172	rVB3	507	376	0.01%	0.003%
60	8.472	2213	2218	2230	rVB3	989	1378	0.04%	0.009%
61	8.636	2257	2269	2301	rBV	355930	649976	18.47%	4.374%
62	8.935	2356	2362	2364	rBV	318	317	0.01%	0.002%
63	9.054	2395	2399	2402	rBV2	256	206	0.01%	0.001%
64	9.253	2458	2461	2464	rBV2	322	257	0.01%	0.002%
65	9.327	2481	2484	2486	rBV	262	177	0.01%	0.001%
66	9.446	2499	2521	2557	rVV2	1618130	3519635	100.00%	23.683%
67	9.687	2591	2596	2598	rBV3	763	620	0.02%	0.004%
68	9.816	2632	2636	2641	rBV2	200	207	0.01%	0.001%
69	10.208	2754	2758	2761	rBV	269	217	0.01%	0.001%
70	10.269	2771	2777	2781	rBV3	354	416	0.01%	0.003%
71	10.529	2856	2858	2863	rBV2	210	211	0.01%	0.001%
72	10.574	2868	2872	2875	rVV	247	208	0.01%	0.001%
73	10.671	2895	2902	2912	rVB4	1980	2318	0.07%	0.016%
74	10.758	2916	2929	2947	rBV	417945	662832	18.83%	4.460%
75	10.896	2966	2972	2980	rVB2	1362	1889	0.05%	0.013%
76	11.031	3009	3014	3017	rBV2	209	221	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048233.D
 Acq On : 22 Apr 2022 18:32
 Operator : SY/MD
 Sample : N2486-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.205	3066	3068	3073	rBV	308	235	0.01%	0.002%
78	11.279	3089	3091	3097	rVB	281	234	0.01%	0.002%
79	11.407	3128	3131	3135	rBV	343	280	0.01%	0.002%
80	11.455	3140	3146	3159	rVB7	1175	2032	0.06%	0.014%
81	11.597	3186	3190	3193	rBV3	367	180	0.01%	0.001%
82	11.690	3215	3219	3222	rBV3	995	696	0.02%	0.005%
83	11.748	3226	3237	3246	rBV	75353	117411	3.34%	0.790%
84	11.835	3246	3264	3286	rVB2	837256	2098852	59.63%	14.123%
85	12.092	3341	3344	3352	rVB4	404	487	0.01%	0.003%
86	12.211	3362	3381	3405	rBV2	977992	2159423	61.35%	14.530%
87	12.481	3462	3465	3468	rVB2	400	268	0.01%	0.002%
88	12.526	3475	3479	3482	rBV3	348	335	0.01%	0.002%
89	12.770	3549	3555	3564	rVB5	1385	2417	0.07%	0.016%
90	12.812	3564	3568	3571	rBV3	508	479	0.01%	0.003%
91	12.973	3611	3618	3632	rBV4	3805	5479	0.16%	0.037%
92	13.024	3632	3634	3639	rBV2	331	240	0.01%	0.002%
93	13.153	3666	3674	3675	rBV2	1468	1545	0.04%	0.010%
94	13.217	3690	3694	3697	rBV4	420	365	0.01%	0.002%
95	13.327	3723	3728	3738	rVB5	1702	2864	0.08%	0.019%
96	13.372	3739	3742	3746	rVV	365	267	0.01%	0.002%
97	13.391	3746	3748	3752	rVB2	321	189	0.01%	0.001%
98	13.841	3876	3888	3906	rBV	397853	630399	17.91%	4.242%
99	14.156	3983	3986	3989	rBV	446	296	0.01%	0.002%
100	14.330	4029	4040	4054	rBV3	95790	153648	4.37%	1.034%




Sum of corrected areas: 14861538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048233.D
Acq On : 22 Apr 2022 18:32
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

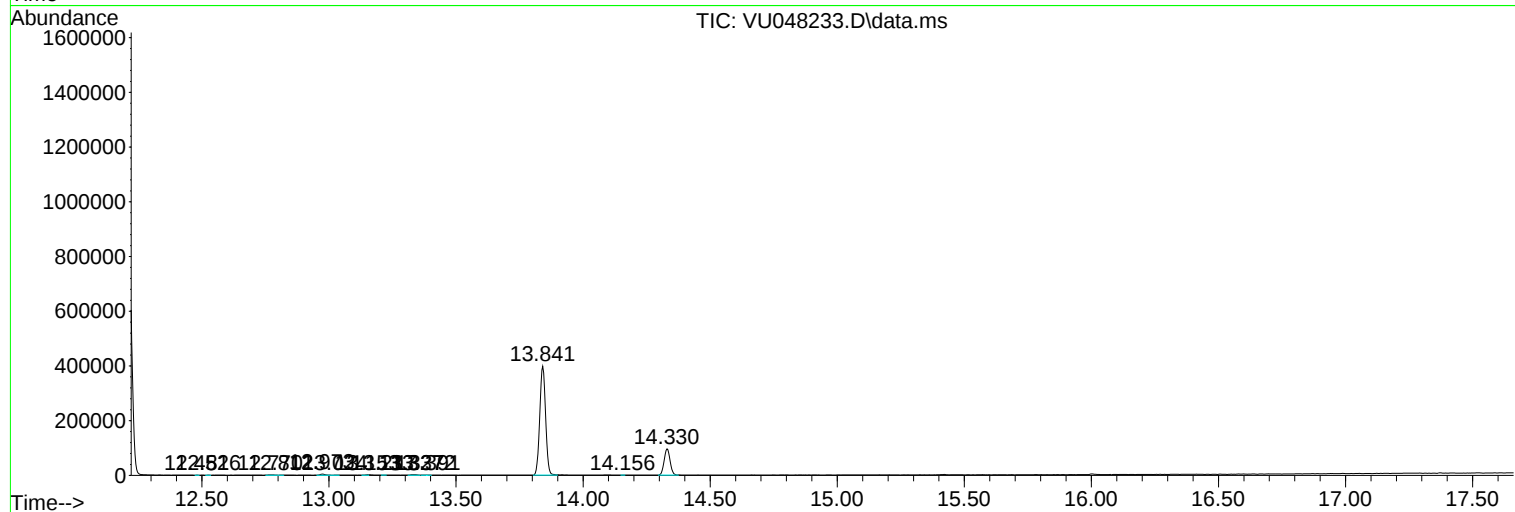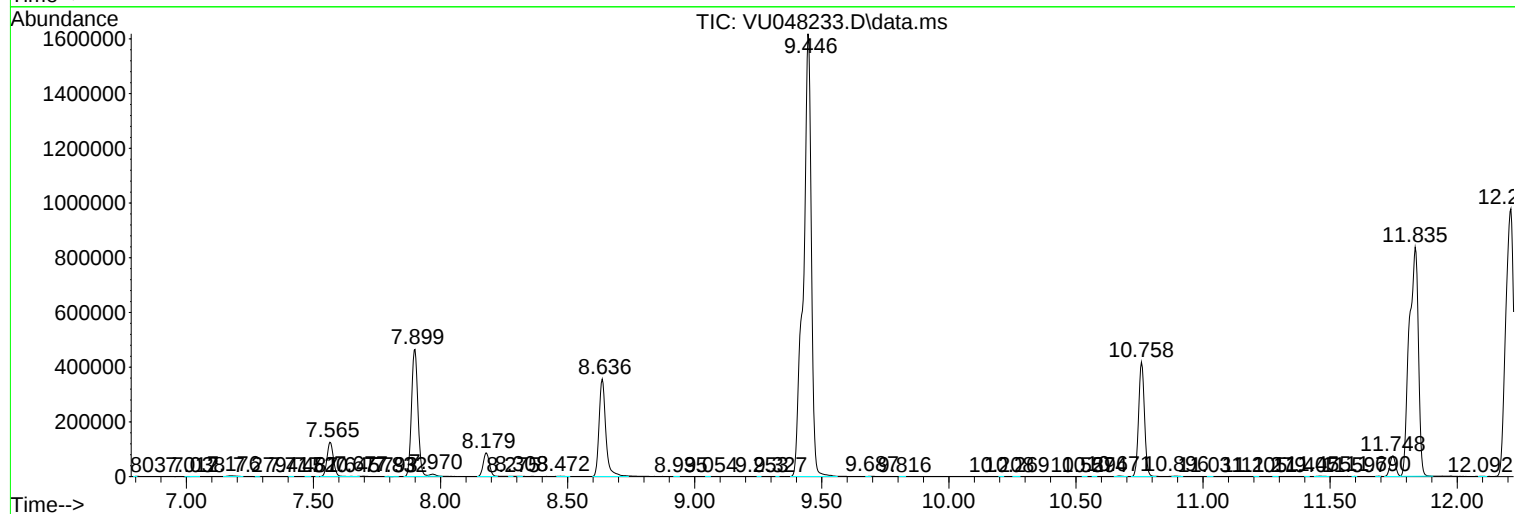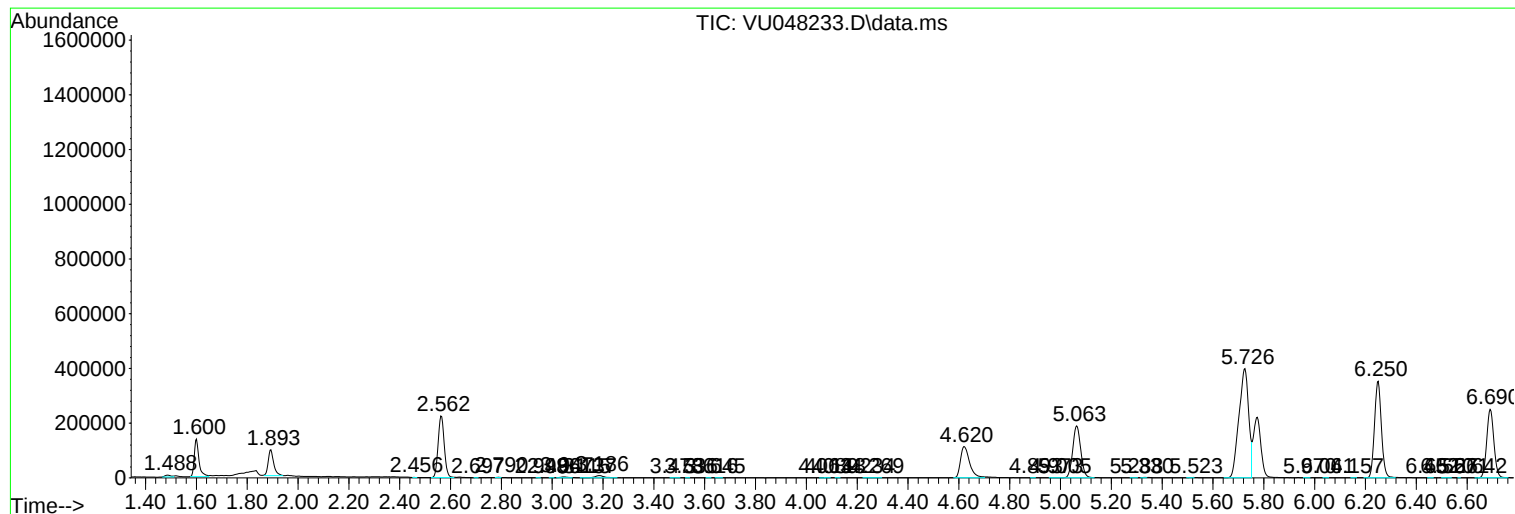

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048233.D
Acq On : 22 Apr 2022 18:32
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048233.D
Acq On : 22 Apr 2022 18:32
Operator : SY/MD
Sample : N2486-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------