

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048234.D
 Acq On : 22 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2486-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV3	5538	8476	0.49%	0.085%
2	1.600	73	81	100	rBV	120635	167057	9.66%	1.669%
3	1.877	162	167	187	rVB	92775	136310	7.88%	1.362%
4	2.559	366	379	397	rBV	220593	366499	21.20%	3.662%
5	2.732	425	433	438	rBV5	855	1376	0.08%	0.014%
6	2.816	455	459	462	rBV2	480	321	0.02%	0.003%
7	3.044	519	530	541	rBV7	3744	7252	0.42%	0.072%
8	3.179	559	572	588	rBV2	11181	25620	1.48%	0.256%
9	3.343	621	623	626	rBV	307	191	0.01%	0.002%
10	3.401	638	641	644	rVB2	357	211	0.01%	0.002%
11	3.472	660	663	666	rVV	312	243	0.01%	0.002%
12	3.629	708	712	716	rBV2	235	217	0.01%	0.002%
13	3.690	728	731	735	rBV3	362	314	0.02%	0.003%
14	3.710	735	737	738	rVV	324	174	0.01%	0.002%
15	3.735	742	745	747	rVV2	309	204	0.01%	0.002%
16	3.764	751	754	759	rVV	295	322	0.02%	0.003%
17	3.980	819	821	825	rVB	221	168	0.01%	0.002%
18	4.018	831	833	844	rBV2	169	297	0.02%	0.003%
19	4.176	879	882	886	rVB2	272	242	0.01%	0.002%
20	4.205	886	891	895	rBV2	332	419	0.02%	0.004%
21	4.295	914	919	921	rBV	255	272	0.02%	0.003%
22	4.350	933	936	938	rBV	249	171	0.01%	0.002%
23	4.459	965	970	974	rBV2	170	235	0.01%	0.002%
24	4.510	983	986	988	rBV2	222	178	0.01%	0.002%
25	4.552	994	999	1002	rBV3	201	208	0.01%	0.002%
26	4.623	1007	1021	1066	rVV	106652	286533	16.57%	2.863%
27	4.796	1072	1075	1077	rVB2	384	193	0.01%	0.002%
28	4.851	1087	1092	1095	rBV2	320	403	0.02%	0.004%
29	5.063	1140	1158	1179	rBV	183079	403989	23.37%	4.036%
30	5.292	1222	1229	1230	rBV2	496	536	0.03%	0.005%
31	5.333	1235	1242	1244	rBV4	824	1065	0.06%	0.011%
32	5.398	1257	1262	1265	rBV2	187	189	0.01%	0.002%
33	5.520	1294	1300	1303	rBV3	465	577	0.03%	0.006%
34	5.562	1310	1313	1316	rBV	257	185	0.01%	0.002%
35	5.723	1341	1363	1374	rBV2	392724	1053077	60.91%	10.521%
36	5.919	1420	1424	1426	rBV3	214	179	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048234.D
 Acq On : 22 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2486-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.970	1432	1440	1441	rBV3	1148	1331	0.08%	0.013%
38	6.108	1480	1483	1487	rBV3	404	304	0.02%	0.003%
39	6.247	1512	1526	1550	rBV	359177	682382	39.47%	6.818%
40	6.526	1607	1613	1614	rBV2	830	561	0.03%	0.006%
41	6.597	1627	1635	1640	rBV5	965	1348	0.08%	0.013%
42	6.690	1648	1664	1687	rBV	242357	472446	27.33%	4.720%
43	6.771	1687	1689	1692	rVB	466	233	0.01%	0.002%
44	6.796	1695	1697	1701	rBV3	478	306	0.02%	0.003%
45	6.848	1707	1713	1715	rBV	237	195	0.01%	0.002%
46	6.864	1715	1718	1723	rVB3	335	267	0.02%	0.003%
47	6.906	1728	1731	1735	rBV2	235	210	0.01%	0.002%
48	7.041	1770	1773	1778	rBV3	361	385	0.02%	0.004%
49	7.176	1803	1815	1832	rBV2	4407	9981	0.58%	0.100%
50	7.507	1912	1918	1923	rBV2	188	255	0.01%	0.003%
51	7.565	1923	1936	1955	rBV	121639	210483	12.17%	2.103%
52	7.684	1966	1973	1975	rBV4	890	892	0.05%	0.009%
53	7.796	1994	2008	2010	rBV4	662	1121	0.06%	0.011%
54	7.809	2010	2012	2014	rVB	425	202	0.01%	0.002%
55	7.899	2025	2040	2056	rBV	459469	791133	45.76%	7.904%
56	8.111	2104	2106	2113	rVB2	421	402	0.02%	0.004%
57	8.179	2116	2127	2141	rBV	84159	141791	8.20%	1.417%
58	8.417	2198	2201	2205	rBV	358	242	0.01%	0.002%
59	8.639	2256	2270	2297	rBV	331279	634181	36.68%	6.336%
60	8.922	2355	2358	2361	rVV3	269	186	0.01%	0.002%
61	8.944	2363	2365	2370	rVB2	293	229	0.01%	0.002%
62	9.005	2381	2384	2387	rBV3	314	257	0.01%	0.003%
63	9.234	2451	2455	2461	rVB	264	324	0.02%	0.003%
64	9.417	2500	2512	2518	rBV	535926	932574	53.94%	9.317%
65	9.642	2579	2582	2588	rVB2	273	253	0.01%	0.003%
66	9.742	2607	2613	2614	rBV	194	178	0.01%	0.002%
67	10.031	2699	2703	2706	rBV2	259	216	0.01%	0.002%
68	10.086	2717	2720	2723	rBV	279	202	0.01%	0.002%
69	10.426	2822	2826	2832	rVB2	320	297	0.02%	0.003%
70	10.671	2894	2902	2909	rBV3	1883	2412	0.14%	0.024%
71	10.758	2917	2929	2952	rBV	399268	648126	37.49%	6.475%
72	10.889	2965	2970	2976	rBV3	808	993	0.06%	0.010%
73	10.957	2983	2991	2993	rBV	356	350	0.02%	0.003%
74	11.018	3007	3010	3017	rVB2	328	369	0.02%	0.004%
75	11.060	3017	3023	3025	rBV	356	363	0.02%	0.004%
76	11.111	3037	3039	3045	rVB2	484	271	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048234.D
 Acq On : 22 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2486-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.282	3087	3092	3093	rBV2	175	171	0.01%	0.002%
78	11.349	3110	3113	3117	rBV	208	183	0.01%	0.002%
79	11.410	3128	3132	3134	rBV2	334	232	0.01%	0.002%
80	11.462	3141	3148	3157	rVB6	1068	1557	0.09%	0.016%
81	11.584	3181	3186	3188	rBV	227	188	0.01%	0.002%
82	11.668	3206	3212	3215	rBV2	394	398	0.02%	0.004%
83	11.697	3215	3221	3226	rBV4	608	529	0.03%	0.005%
84	11.748	3226	3237	3246	rBV	85485	134015	7.75%	1.339%
85	11.816	3246	3258	3262	rBV	561038	947276	54.79%	9.464%
86	11.973	3302	3307	3315	rVB7	1607	2048	0.12%	0.020%
87	12.127	3353	3355	3359	rVB2	576	344	0.02%	0.003%
88	12.208	3363	3380	3400	rVV2	726833	1728966	100.00%	17.274%
89	12.336	3417	3420	3422	rBV2	478	309	0.02%	0.003%
90	12.471	3460	3462	3465	rBV2	298	230	0.01%	0.002%
91	12.539	3480	3483	3485	rBV2	262	213	0.01%	0.002%
92	12.725	3539	3541	3544	rBV2	258	179	0.01%	0.002%
93	12.979	3616	3620	3623	rBV2	467	289	0.02%	0.003%
94	13.163	3673	3677	3682	rBV2	378	391	0.02%	0.004%
95	13.224	3693	3696	3697	rBV2	328	185	0.01%	0.002%
96	13.368	3738	3741	3744	rBV	404	360	0.02%	0.004%
97	13.841	3877	3888	3909	rBV	86523	140601	8.13%	1.405%
98	14.333	4031	4041	4055	rVB2	29169	47299	2.74%	0.473%
99	14.497	4089	4092	4099	rBV3	478	436	0.03%	0.004%
100	15.545	4415	4418	4424	rBV2	746	666	0.04%	0.007%




Sum of corrected areas: 10009219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048234.D
Acq On : 22 Apr 2022 18:56
Operator : SY/MD
Sample : N2486-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

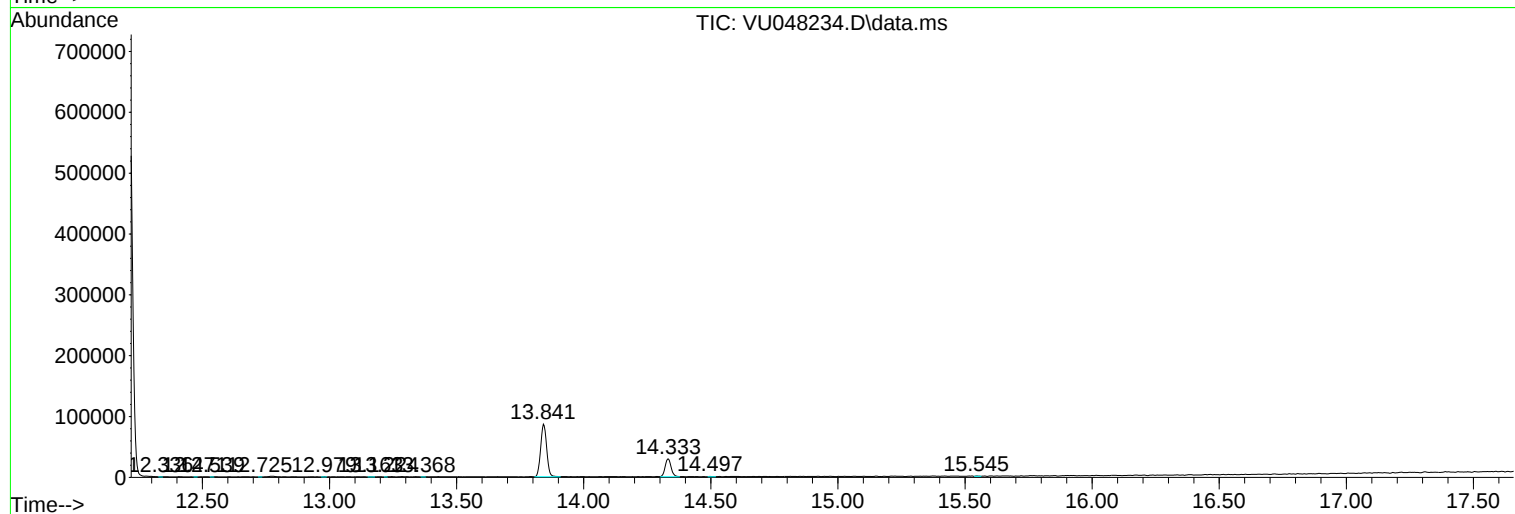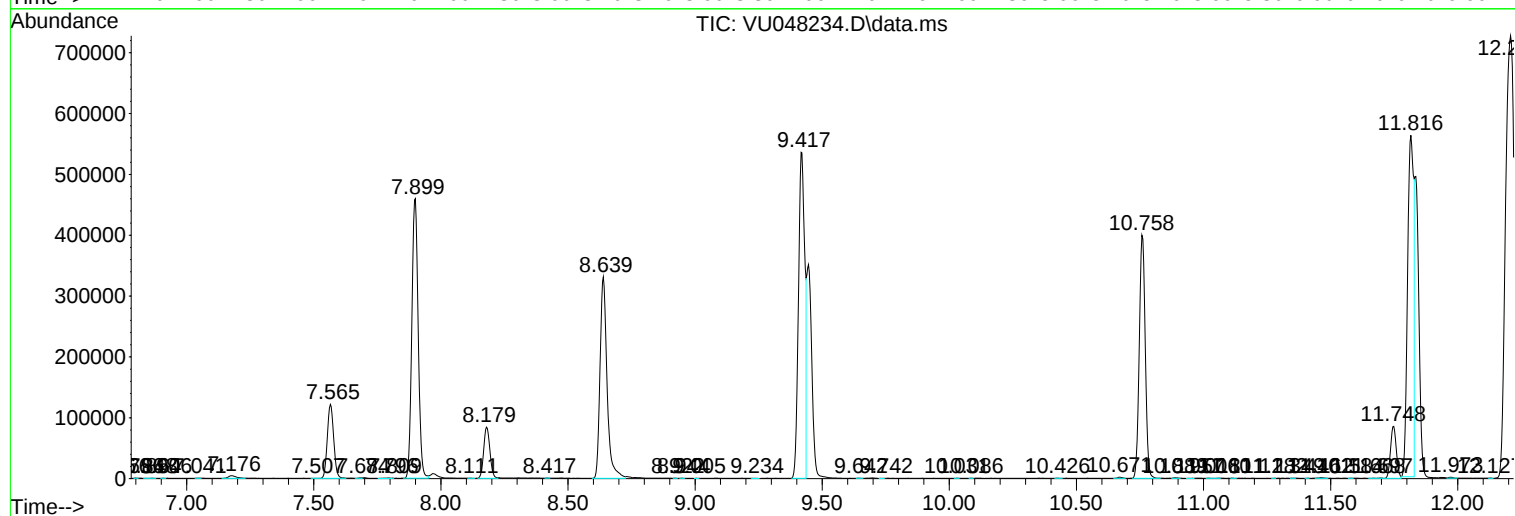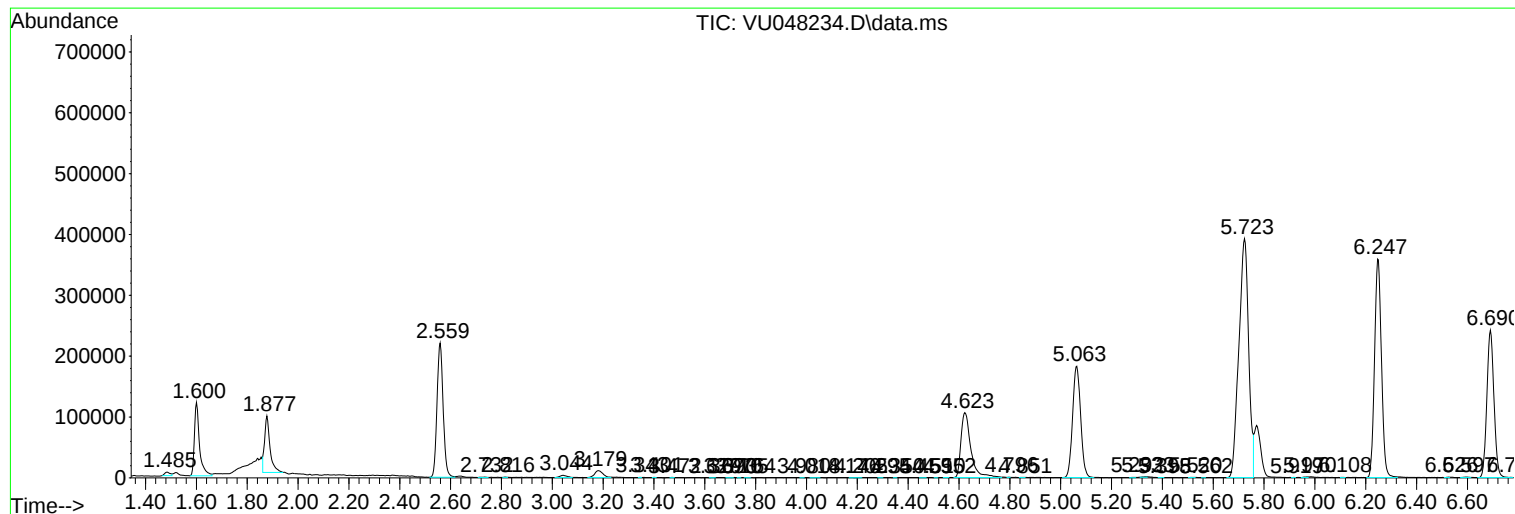

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048234.D
Acq On : 22 Apr 2022 18:56
Operator : SY/MD
Sample : N2486-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048234.D
Acq On : 22 Apr 2022 18:56
Operator : SY/MD
Sample : N2486-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc