

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048235.D
 Acq On : 22 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2486-11DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	39	44	50	rBV3	5937	7759	0.74%	0.087%
2	1.600	73	81	98	rBV	118874	164741	15.68%	1.850%
3	1.877	162	167	198	rVB	89498	142981	13.61%	1.606%
4	2.555	366	378	396	rBV	220994	368463	35.06%	4.138%
5	2.703	421	424	426	rBV	282	197	0.02%	0.002%
6	2.774	441	446	448	rBV4	470	453	0.04%	0.005%
7	2.890	474	482	486	rBV2	344	560	0.05%	0.006%
8	2.909	486	488	492	rVB	283	191	0.02%	0.002%
9	2.944	496	499	502	rVV3	417	306	0.03%	0.003%
10	3.041	521	529	542	rBV2	3640	7233	0.69%	0.081%
11	3.179	557	572	587	rBV	5129	11365	1.08%	0.128%
12	3.250	593	594	602	rVB3	574	613	0.06%	0.007%
13	3.616	707	708	712	rVB2	357	189	0.02%	0.002%
14	3.719	736	740	743	rBV2	170	186	0.02%	0.002%
15	3.813	763	769	775	rVB2	182	220	0.02%	0.002%
16	4.288	908	917	920	rBV	277	515	0.05%	0.006%
17	4.343	931	934	939	rBV2	222	205	0.02%	0.002%
18	4.394	946	950	952	rBV2	218	200	0.02%	0.002%
19	4.513	981	987	993	rBV2	248	398	0.04%	0.004%
20	4.626	1008	1022	1042	rBV	99146	262304	24.96%	2.945%
21	4.877	1098	1100	1106	rBV3	259	200	0.02%	0.002%
22	5.063	1140	1158	1177	rVV	186105	406594	38.69%	4.566%
23	5.134	1177	1180	1186	rVB4	876	718	0.07%	0.008%
24	5.189	1194	1197	1203	rBV2	270	267	0.03%	0.003%
25	5.333	1239	1242	1254	rVB4	1200	1936	0.18%	0.022%
26	5.414	1261	1267	1270	rBV3	349	371	0.04%	0.004%
27	5.722	1340	1363	1371	rBV2	397117	1050895	100.00%	11.801%
28	5.967	1431	1439	1453	rVB5	4308	8435	0.80%	0.095%
29	6.047	1460	1464	1471	rVB2	386	367	0.03%	0.004%
30	6.086	1471	1476	1479	rBV2	243	251	0.02%	0.003%
31	6.111	1481	1484	1487	rVV2	300	185	0.02%	0.002%
32	6.147	1491	1495	1499	rBV4	358	404	0.04%	0.005%
33	6.247	1512	1526	1551	rVV	352567	674981	64.23%	7.579%
34	6.517	1606	1610	1611	rBV2	1087	581	0.06%	0.007%
35	6.594	1626	1634	1650	rVB4	1444	2888	0.27%	0.032%
36	6.690	1650	1664	1688	rVV	246239	475881	45.28%	5.344%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048235.D
 Acq On : 22 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2486-11DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.774	1688	1690	1694	rVB2	447	292	0.03%	0.003%
38	6.812	1694	1702	1708	rBV5	606	964	0.09%	0.011%
39	6.925	1735	1737	1739	rBV3	316	193	0.02%	0.002%
40	7.050	1772	1776	1779	rBV3	240	271	0.03%	0.003%
41	7.105	1789	1793	1797	rBV	160	185	0.02%	0.002%
42	7.176	1804	1815	1823	rBV2	4422	8466	0.81%	0.095%
43	7.382	1875	1879	1882	rVV3	255	212	0.02%	0.002%
44	7.404	1882	1886	1891	rVB2	302	286	0.03%	0.003%
45	7.565	1924	1936	1952	rBV	119191	211391	20.12%	2.374%
46	7.681	1969	1972	1973	rBV	613	370	0.04%	0.004%
47	7.690	1973	1975	1979	rVV2	949	822	0.08%	0.009%
48	7.722	1982	1985	1989	rVB3	674	469	0.04%	0.005%
49	7.748	1989	1993	1997	rVB2	433	284	0.03%	0.003%
50	7.899	2026	2040	2055	rBV	454193	788366	75.02%	8.853%
51	8.066	2090	2092	2094	rBV2	391	199	0.02%	0.002%
52	8.134	2109	2113	2116	rVB2	375	283	0.03%	0.003%
53	8.179	2116	2127	2143	rBV	83341	144955	13.79%	1.628%
54	8.562	2241	2246	2249	rBV3	265	198	0.02%	0.002%
55	8.639	2258	2270	2315	rBV	341142	659179	62.73%	7.402%
56	8.812	2322	2324	2328	rVB4	458	284	0.03%	0.003%
57	8.838	2329	2332	2341	rVB3	442	292	0.03%	0.003%
58	8.912	2350	2355	2359	rVB2	274	274	0.03%	0.003%
59	9.176	2433	2437	2438	rBV2	313	219	0.02%	0.002%
60	9.250	2455	2460	2465	rVV3	264	287	0.03%	0.003%
61	9.327	2481	2484	2487	rBV2	302	202	0.02%	0.002%
62	9.420	2499	2513	2518	rBV	547437	950431	90.44%	10.673%
63	9.690	2594	2597	2599	rBV	365	267	0.03%	0.003%
64	9.703	2599	2601	2604	rVB2	550	297	0.03%	0.003%
65	10.105	2724	2726	2733	rVB3	296	246	0.02%	0.003%
66	10.671	2890	2902	2910	rBV3	1911	2930	0.28%	0.033%
67	10.706	2910	2913	2917	rVV	353	215	0.02%	0.002%
68	10.758	2917	2929	2951	rVV	407433	660761	62.88%	7.420%
69	10.864	2958	2962	2965	rBV3	278	271	0.03%	0.003%
70	11.037	3012	3016	3019	rBV2	269	221	0.02%	0.002%
71	11.108	3033	3038	3039	rBV	426	294	0.03%	0.003%
72	11.301	3095	3098	3101	rBV3	380	265	0.03%	0.003%
73	11.391	3121	3126	3129	rVB2	240	245	0.02%	0.003%
74	11.407	3129	3131	3134	rBV2	336	252	0.02%	0.003%
75	11.468	3138	3150	3160	rBV4	1319	2647	0.25%	0.030%
76	11.545	3170	3174	3176	rBV	441	276	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048235.D
 Acq On : 22 Apr 2022 19:19
 Operator : SY/MD
 Sample : N2486-11DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.696	3216	3221	3226	rBV3	870	965	0.09%	0.011%
78	11.748	3229	3237	3245	rBV2	5525	8217	0.78%	0.092%
79	11.815	3245	3258	3280	rVV2	506130	960266	91.38%	10.783%
80	11.973	3302	3307	3314	rVB5	1309	1597	0.15%	0.018%
81	12.005	3315	3317	3323	rVB4	453	436	0.04%	0.005%
82	12.034	3323	3326	3328	rBV	481	353	0.03%	0.004%
83	12.121	3349	3353	3358	rVB2	421	399	0.04%	0.004%
84	12.195	3361	3376	3395	rBV2	469484	870224	82.81%	9.772%
85	12.430	3443	3449	3451	rBV2	404	390	0.04%	0.004%
86	12.481	3462	3465	3470	rVV2	404	374	0.04%	0.004%
87	12.552	3483	3487	3490	rBV2	471	401	0.04%	0.005%
88	12.606	3500	3504	3506	rBV	250	218	0.02%	0.002%
89	12.767	3547	3554	3559	rBV4	1071	1452	0.14%	0.016%
90	12.809	3563	3567	3574	rVV4	447	624	0.06%	0.007%
91	12.854	3578	3581	3584	rBV3	372	302	0.03%	0.003%
92	12.880	3584	3589	3596	rVB3	316	439	0.04%	0.005%
93	13.008	3627	3629	3631	rBV2	335	218	0.02%	0.002%
94	13.076	3646	3650	3654	rBV2	347	377	0.04%	0.004%
95	13.134	3664	3668	3670	rBV	276	234	0.02%	0.003%
96	13.844	3880	3889	3900	rBV3	12379	20078	1.91%	0.225%
97	13.979	3928	3931	3933	rBV	278	192	0.02%	0.002%
98	14.333	4036	4041	4049	rVB4	3254	4140	0.39%	0.046%
99	14.745	4167	4169	4173	rVB2	414	208	0.02%	0.002%
100	15.597	4431	4434	4438	rBV2	824	698	0.07%	0.008%


Sum of corrected areas: 8905396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048235.D
Acq On : 22 Apr 2022 19:19
Operator : SY/MD
Sample : N2486-11DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

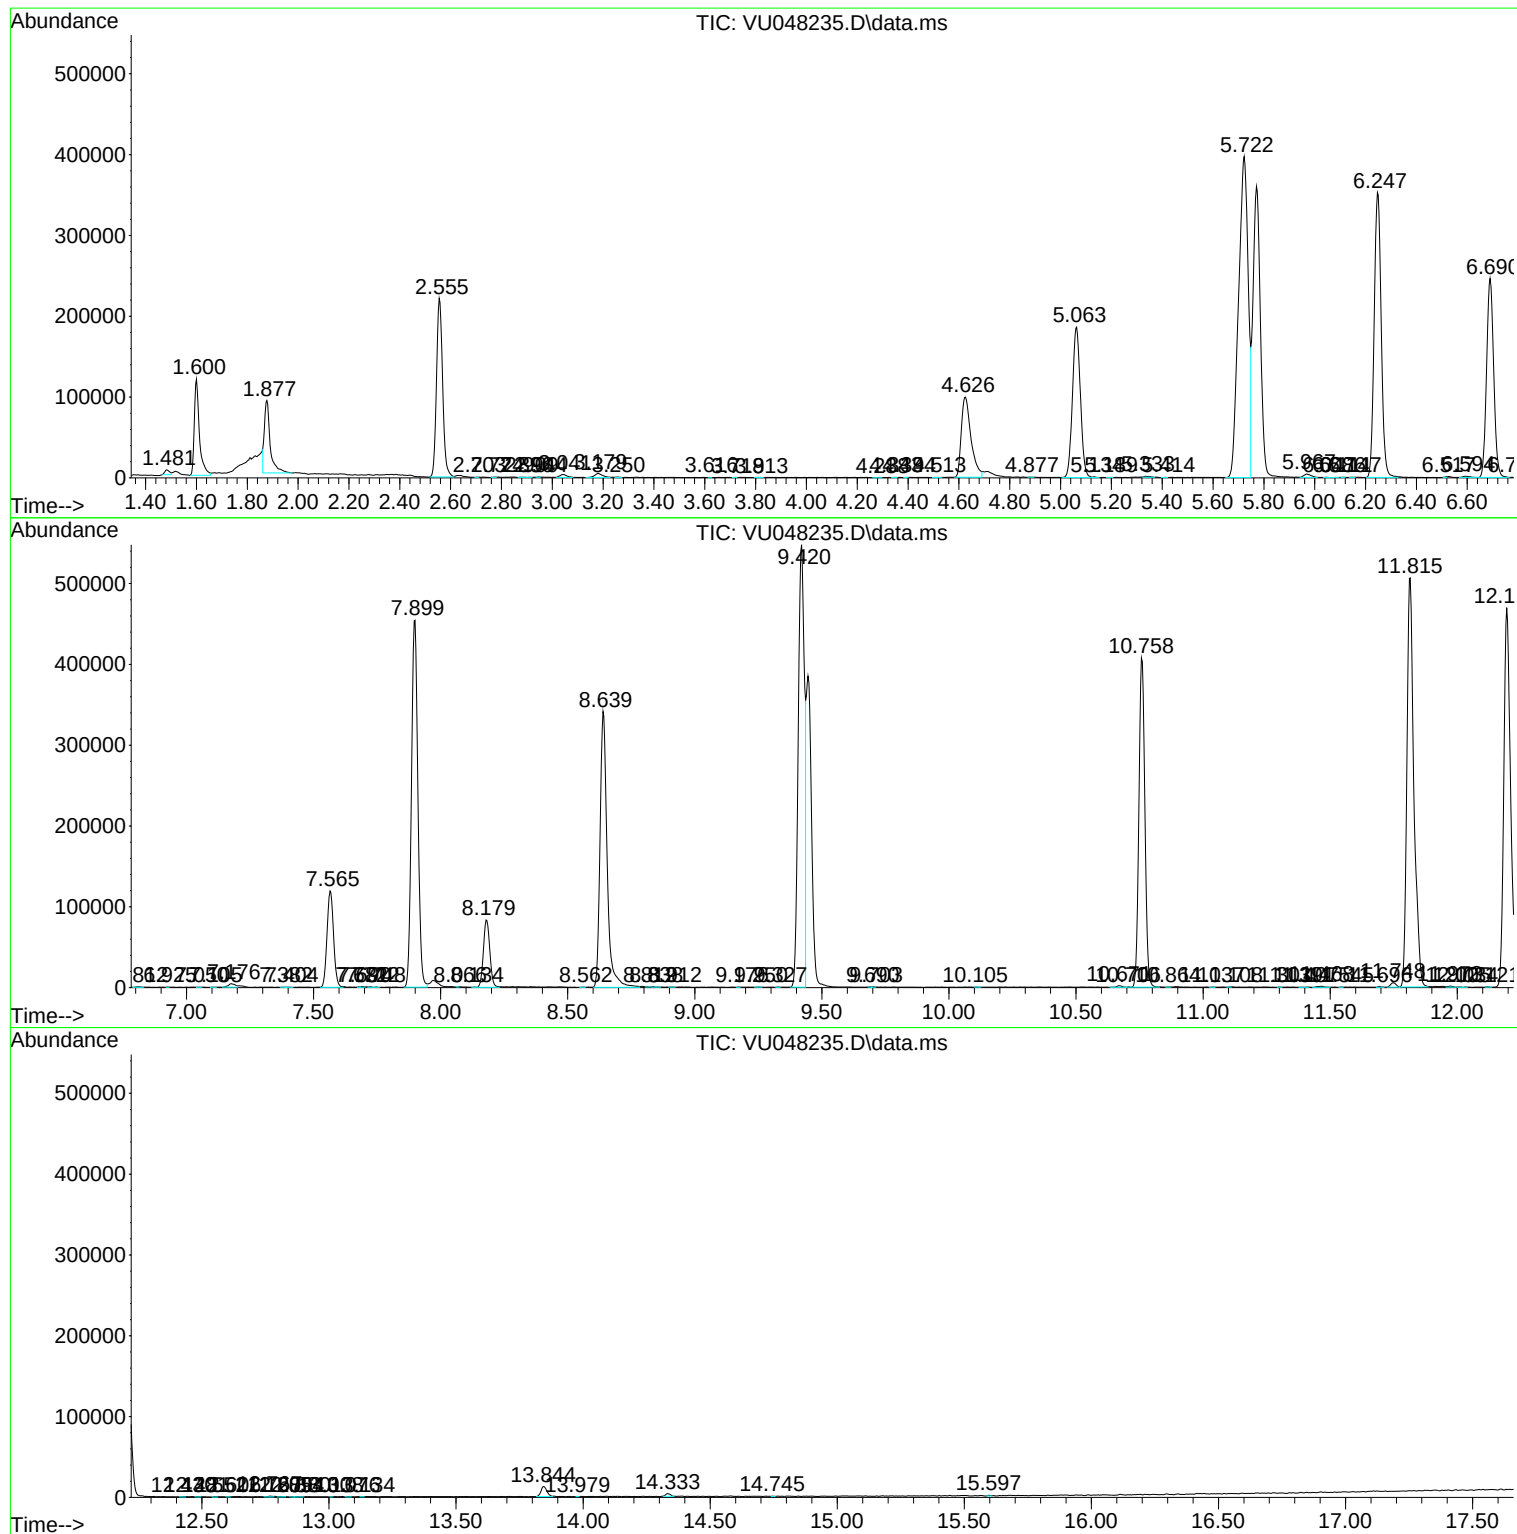

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048235.D
Acq On : 22 Apr 2022 19:19
Operator : SY/MD
Sample : N2486-11DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048235.D
Acq On : 22 Apr 2022 19:19
Operator : SY/MD
Sample : N2486-11DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------