

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048236.D
 Acq On : 22 Apr 2022 19:43
 Operator : SY/MD
 Sample : N2486-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	125628	172821	15.69%	1.904%
2	2.556	366	378	397	rBV	234321	389443	35.36%	4.291%
3	2.765	440	443	444	rBV	487	233	0.02%	0.003%
4	3.041	521	529	539	rBV4	3582	6533	0.59%	0.072%
5	3.183	559	573	589	rBV	13816	33284	3.02%	0.367%
6	3.350	623	625	627	rBV	177	81	0.01%	0.001%
7	3.533	679	682	684	rBV	130	78	0.01%	0.001%
8	3.591	697	700	704	rBV3	231	176	0.02%	0.002%
9	3.610	704	706	709	rVB2	187	87	0.01%	0.001%
10	3.675	723	726	731	rBV	137	133	0.01%	0.001%
11	3.745	745	748	753	rBV	138	107	0.01%	0.001%
12	3.797	762	764	766	rBV2	113	59	0.01%	0.001%
13	3.832	772	775	777	rBV	243	101	0.01%	0.001%
14	3.848	777	780	782	rBV2	113	79	0.01%	0.001%
15	3.912	797	800	802	rBV2	132	93	0.01%	0.001%
16	4.006	827	829	832	rBV2	83	57	0.01%	0.001%
17	4.051	840	843	845	rBV	150	100	0.01%	0.001%
18	4.134	864	869	872	rVB	176	82	0.01%	0.001%
19	4.154	872	875	880	rBV	234	205	0.02%	0.002%
20	4.179	880	883	885	rBV	111	69	0.01%	0.001%
21	4.292	915	918	921	rBV	208	157	0.01%	0.002%
22	4.340	931	933	936	rBV	191	122	0.01%	0.001%
23	4.379	941	945	948	rVB2	216	147	0.01%	0.002%
24	4.398	948	951	953	rBV2	127	73	0.01%	0.001%
25	4.414	953	956	958	rBV	140	103	0.01%	0.001%
26	4.517	985	988	992	rBV2	106	89	0.01%	0.001%
27	4.562	997	1002	1006	rBV3	419	519	0.05%	0.006%
28	4.623	1008	1021	1045	rBV	109192	293140	26.62%	3.230%
29	4.977	1128	1131	1136	rVB	220	206	0.02%	0.002%
30	5.064	1136	1158	1179	rBV	197942	431895	39.22%	4.759%
31	5.211	1198	1204	1206	rBV3	349	339	0.03%	0.004%
32	5.314	1234	1236	1237	rBV	231	88	0.01%	0.001%
33	5.388	1257	1259	1261	rVB2	190	61	0.01%	0.001%
34	5.404	1261	1264	1266	rVB2	166	91	0.01%	0.001%
35	5.475	1280	1286	1291	rBV2	161	166	0.02%	0.002%
36	5.501	1291	1294	1298	rVB2	240	153	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048236.D
 Acq On : 22 Apr 2022 19:43
 Operator : SY/MD
 Sample : N2486-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.520	1298	1300	1303	rBV	304	174	0.02%	0.002%
38	5.581	1315	1319	1323	rVB2	266	181	0.02%	0.002%
39	5.723	1342	1363	1371	rBV2	416760	1101317	100.00%	12.136%
40	5.973	1432	1441	1454	rVB7	3923	8355	0.76%	0.092%
41	6.031	1454	1459	1462	rBV2	417	425	0.04%	0.005%
42	6.080	1471	1474	1477	rVB2	242	153	0.01%	0.002%
43	6.112	1481	1484	1489	rBV2	212	200	0.02%	0.002%
44	6.134	1489	1491	1495	rBV2	248	195	0.02%	0.002%
45	6.247	1511	1526	1547	rBV	349887	669104	60.75%	7.373%
46	6.475	1593	1597	1598	rBV	214	141	0.01%	0.002%
47	6.523	1607	1612	1620	rBV7	1774	2301	0.21%	0.025%
48	6.597	1627	1635	1643	rBV5	1457	2422	0.22%	0.027%
49	6.690	1650	1664	1683	rBV	255057	499115	45.32%	5.500%
50	6.803	1696	1699	1709	rVB3	997	872	0.08%	0.010%
51	6.893	1723	1727	1733	rBV2	301	276	0.03%	0.003%
52	7.012	1760	1764	1767	rBV3	268	208	0.02%	0.002%
53	7.092	1787	1789	1790	rBV	246	89	0.01%	0.001%
54	7.182	1805	1817	1825	rBV2	4442	9566	0.87%	0.105%
55	7.260	1839	1841	1845	rVB2	203	79	0.01%	0.001%
56	7.282	1845	1848	1849	rBV2	187	100	0.01%	0.001%
57	7.301	1852	1854	1860	rVV2	244	194	0.02%	0.002%
58	7.330	1860	1863	1867	rVV	164	119	0.01%	0.001%
59	7.388	1879	1881	1886	rBV2	193	204	0.02%	0.002%
60	7.443	1895	1898	1900	rBV	153	104	0.01%	0.001%
61	7.478	1906	1909	1911	rBV	214	172	0.02%	0.002%
62	7.517	1919	1921	1923	rBV	156	84	0.01%	0.001%
63	7.565	1923	1936	1953	rVV	124864	223361	20.28%	2.461%
64	7.655	1963	1964	1967	rBV2	131	74	0.01%	0.001%
65	7.684	1969	1973	1974	rBV2	705	536	0.05%	0.006%
66	7.761	1994	1997	1998	rBV	136	79	0.01%	0.001%
67	7.793	2000	2007	2011	rBV4	595	912	0.08%	0.010%
68	7.832	2017	2019	2025	rVB2	310	224	0.02%	0.002%
69	7.896	2025	2039	2055	rBV	478905	828775	75.25%	9.132%
70	8.179	2116	2127	2142	rBV	86638	148744	13.51%	1.639%
71	8.462	2210	2215	2216	rBV	564	369	0.03%	0.004%
72	8.542	2238	2240	2241	rBV	173	60	0.01%	0.001%
73	8.588	2251	2254	2257	rBV2	213	185	0.02%	0.002%
74	8.639	2257	2270	2307	rBV	368177	716078	65.02%	7.891%
75	9.047	2392	2397	2399	rBV	275	213	0.02%	0.002%
76	9.256	2459	2462	2466	rVB	222	113	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048236.D
 Acq On : 22 Apr 2022 19:43
 Operator : SY/MD
 Sample : N2486-15DL 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.417	2498	2512	2518	rBV	535955	939936	85.35%	10.357%
78	9.626	2574	2577	2579	rBV	233	174	0.02%	0.002%
79	9.761	2616	2619	2623	rVB	246	193	0.02%	0.002%
80	9.784	2623	2626	2630	rBV3	270	293	0.03%	0.003%
81	9.954	2675	2679	2681	rBV2	247	223	0.02%	0.002%
82	10.083	2717	2719	2720	rBV2	179	58	0.01%	0.001%
83	10.150	2738	2740	2743	rVB2	227	94	0.01%	0.001%
84	10.288	2780	2783	2785	rBV	213	145	0.01%	0.002%
85	10.555	2864	2866	2871	rBV2	208	132	0.01%	0.001%
86	10.671	2892	2902	2912	rVB4	1979	2864	0.26%	0.032%
87	10.761	2915	2930	2950	rBV	426641	693551	62.97%	7.642%
88	10.970	2993	2995	2997	rBV	165	99	0.01%	0.001%
89	11.012	3006	3008	3010	rBV	191	91	0.01%	0.001%
90	11.089	3029	3032	3034	rBV3	310	157	0.01%	0.002%
91	11.112	3035	3039	3040	rBV	479	247	0.02%	0.003%
92	11.279	3088	3091	3094	rBV2	328	280	0.03%	0.003%
93	11.330	3104	3107	3109	rBV2	293	202	0.02%	0.002%
94	11.456	3141	3146	3158	rVB4	898	1652	0.15%	0.018%
95	11.751	3229	3238	3245	rBV2	4770	6794	0.62%	0.075%
96	11.812	3245	3257	3285	rVV2	517699	963240	87.46%	10.614%
97	12.079	3337	3340	3341	rBV	335	186	0.02%	0.002%
98	12.118	3349	3352	3354	rBV2	422	255	0.02%	0.003%
99	12.195	3362	3376	3397	rBV2	503399	908483	82.49%	10.011%
100	13.848	3883	3890	3900	rBV2	5549	8651	0.79%	0.095%




Sum of corrected areas: 9075043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048236.D
Acq On : 22 Apr 2022 19:43
Operator : SY/MD
Sample : N2486-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

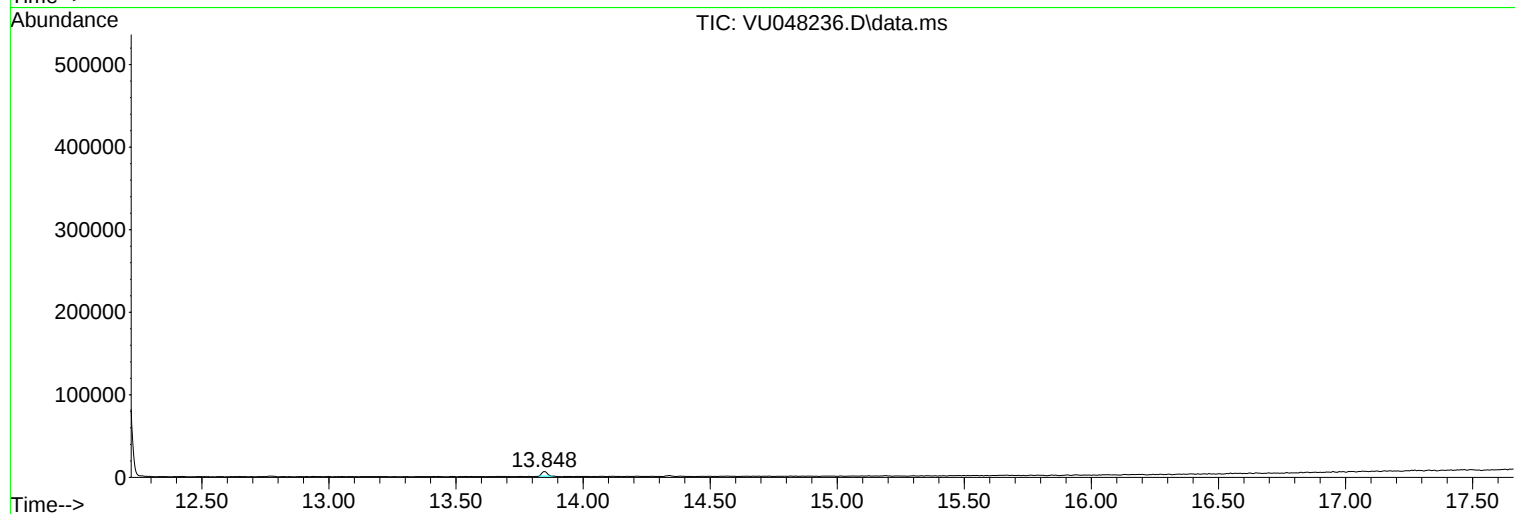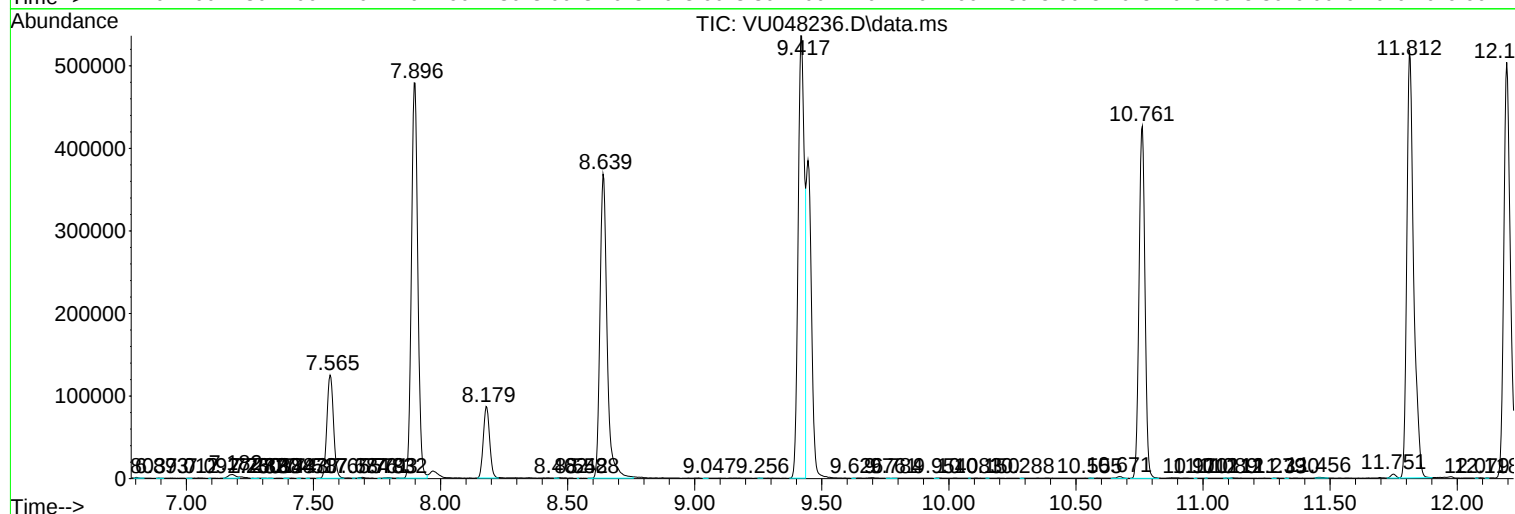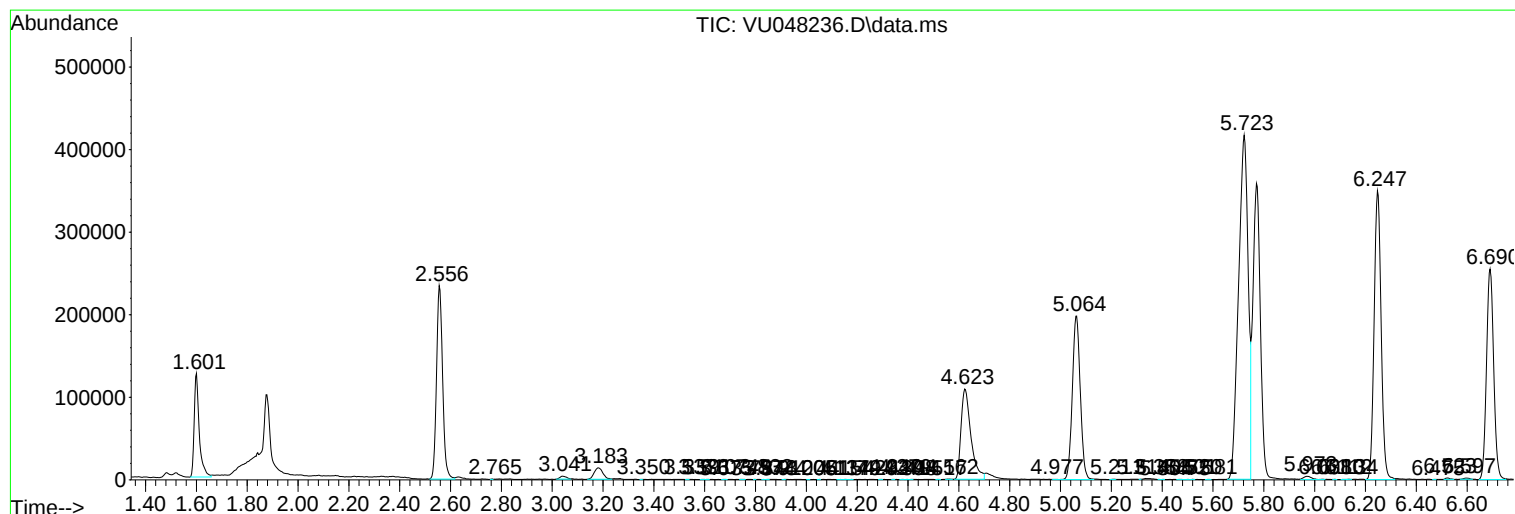

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048236.D
Acq On : 22 Apr 2022 19:43
Operator : SY/MD
Sample : N2486-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048236.D
Acq On : 22 Apr 2022 19:43
Operator : SY/MD
Sample : N2486-15DL 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------