

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048237.D
 Acq On : 22 Apr 2022 20:07
 Operator : SY/MD
 Sample : N2486-08 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	48	rBV	4445	4967	0.06%	0.020%
2	1.601	73	81	102	rBV	115709	164389	1.91%	0.670%
3	1.880	163	168	196	rVB	94474	153001	1.78%	0.623%
4	2.556	365	378	395	rBV	223294	368709	4.29%	1.502%
5	2.781	439	448	450	rBV6	2078	2793	0.03%	0.011%
6	2.838	457	466	483	rVB2	13297	28963	0.34%	0.118%
7	2.948	497	500	502	rBV2	303	232	0.00%	0.001%
8	3.041	519	529	551	rVV2	14897	31617	0.37%	0.129%
9	3.118	551	553	558	rVB2	482	265	0.00%	0.001%
10	3.183	558	573	589	rBV2	16446	39919	0.46%	0.163%
11	3.340	619	622	625	rVV2	228	185	0.00%	0.001%
12	3.433	649	651	657	rVB2	235	204	0.00%	0.001%
13	3.578	694	696	700	rVB	259	184	0.00%	0.001%
14	3.601	700	703	705	rBV2	353	248	0.00%	0.001%
15	3.613	705	707	713	rVB2	383	290	0.00%	0.001%
16	3.674	724	726	732	rVB2	271	243	0.00%	0.001%
17	3.742	742	747	752	rBV2	315	420	0.00%	0.002%
18	3.768	752	755	758	rVV	291	249	0.00%	0.001%
19	3.871	785	787	794	rVB2	318	331	0.00%	0.001%
20	3.909	794	799	803	rBV	271	316	0.00%	0.001%
21	3.941	803	809	812	rVB2	285	270	0.00%	0.001%
22	3.977	817	820	825	rVB2	189	212	0.00%	0.001%
23	4.006	825	829	833	rBV2	228	221	0.00%	0.001%
24	4.044	835	841	843	rBV	258	238	0.00%	0.001%
25	4.449	963	967	971	rBV2	257	259	0.00%	0.001%
26	4.514	983	987	990	rBV	527	447	0.01%	0.002%
27	4.626	1009	1022	1068	rBV	102706	301385	3.50%	1.228%
28	4.922	1112	1114	1117	rVB	273	182	0.00%	0.001%
29	4.954	1122	1124	1129	rBV3	226	241	0.00%	0.001%
30	5.063	1142	1158	1179	rVV	187702	411124	4.78%	1.675%
31	5.282	1219	1226	1228	rBV4	487	436	0.01%	0.002%
32	5.343	1234	1245	1246	rBV2	728	1010	0.01%	0.004%
33	5.723	1342	1363	1376	rBV2	399962	1077442	12.52%	4.389%
34	5.970	1431	1440	1453	rVB4	2709	5672	0.07%	0.023%
35	6.035	1456	1460	1464	rBV3	195	196	0.00%	0.001%
36	6.108	1478	1483	1485	rBV2	284	253	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048237.D
 Acq On : 22 Apr 2022 20:07
 Operator : SY/MD
 Sample : N2486-08 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.247	1511	1526	1550	rBV	355843	674213	7.84%	2.746%
38	6.530	1608	1614	1619	rBV5	837	928	0.01%	0.004%
39	6.591	1625	1633	1640	rBV3	1473	2269	0.03%	0.009%
40	6.690	1649	1664	1692	rVB	251412	487539	5.67%	1.986%
41	6.803	1696	1699	1701	rBV2	343	243	0.00%	0.001%
42	7.179	1805	1816	1825	rBV4	3986	8179	0.10%	0.033%
43	7.424	1889	1892	1897	rVB3	304	280	0.00%	0.001%
44	7.449	1897	1900	1902	rBV2	355	256	0.00%	0.001%
45	7.565	1923	1936	1953	rBV	117376	208576	2.42%	0.850%
46	7.652	1958	1963	1967	rVB4	490	567	0.01%	0.002%
47	7.694	1970	1976	1984	rBV4	716	1210	0.01%	0.005%
48	7.751	1989	1994	2001	rBV2	377	411	0.00%	0.002%
49	7.899	2025	2040	2055	rBV	458592	793456	9.22%	3.232%
50	8.041	2082	2084	2088	rVB2	444	341	0.00%	0.001%
51	8.179	2113	2127	2143	rBV	82361	143632	1.67%	0.585%
52	8.305	2160	2166	2169	rBV3	363	388	0.00%	0.002%
53	8.472	2208	2218	2228	rVB5	1103	2105	0.02%	0.009%
54	8.523	2228	2234	2237	rBV2	198	238	0.00%	0.001%
55	8.642	2258	2271	2305	rBV	359421	682568	7.93%	2.780%
56	8.787	2311	2316	2320	rBV4	717	764	0.01%	0.003%
57	8.899	2347	2351	2354	rBV2	278	242	0.00%	0.001%
58	9.063	2397	2402	2406	rBV2	279	346	0.00%	0.001%
59	9.121	2416	2420	2424	rVB2	335	214	0.00%	0.001%
60	9.140	2424	2426	2429	rBV	276	202	0.00%	0.001%
61	9.160	2429	2432	2440	rVB4	618	543	0.01%	0.002%
62	9.272	2465	2467	2472	rVB2	305	247	0.00%	0.001%
63	9.369	2494	2497	2500	rVV2	261	227	0.00%	0.001%
64	9.449	2500	2522	2557	rVV2	1931792	4110666	47.78%	16.743%
65	9.674	2590	2592	2594	rVV	379	220	0.00%	0.001%
66	9.694	2594	2598	2604	rVB3	785	750	0.01%	0.003%
67	9.803	2629	2632	2635	rBV3	334	251	0.00%	0.001%
68	10.253	2769	2772	2779	rVB	247	192	0.00%	0.001%
69	10.546	2857	2863	2869	rVB2	228	381	0.00%	0.002%
70	10.581	2869	2874	2877	rBV2	242	291	0.00%	0.001%
71	10.671	2893	2902	2909	rBV5	2217	2814	0.03%	0.011%
72	10.758	2917	2929	2946	rBV	429942	694966	8.08%	2.831%
73	10.867	2960	2963	2964	rBV2	334	215	0.00%	0.001%
74	10.899	2965	2973	2979	rVB5	1401	2164	0.03%	0.009%
75	11.099	3031	3035	3038	rBV3	257	214	0.00%	0.001%
76	11.456	3140	3146	3155	rBV5	1346	2094	0.02%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048237.D
 Acq On : 22 Apr 2022 20:07
 Operator : SY/MD
 Sample : N2486-08 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.510	3160	3163	3166	rVB	299	198	0.00%	0.001%
78	11.533	3166	3170	3175	rBV3	354	340	0.00%	0.001%
79	11.571	3177	3182	3184	rBV2	542	522	0.01%	0.002%
80	11.693	3217	3220	3223	rBV3	659	400	0.00%	0.002%
81	11.748	3225	3237	3246	rVV	178274	279357	3.25%	1.138%
82	11.835	3246	3264	3286	rVB2	942125	2320138	26.97%	9.450%
83	12.076	3337	3339	3342	rVB	428	210	0.00%	0.001%
84	12.214	3360	3382	3405	rBV2	5094323	8602935	100.00%	35.041%
85	12.378	3431	3433	3436	rBV2	430	234	0.00%	0.001%
86	12.607	3500	3504	3507	rBV2	419	366	0.00%	0.001%
87	12.632	3509	3512	3520	rVV4	505	583	0.01%	0.002%
88	12.970	3608	3617	3627	rVB2	10663	16403	0.19%	0.067%
89	13.153	3664	3674	3686	rVB7	3885	8502	0.10%	0.035%
90	13.227	3691	3697	3703	rVB4	1370	1705	0.02%	0.007%
91	13.279	3711	3713	3716	rBV3	394	280	0.00%	0.001%
92	13.330	3721	3729	3742	rVB5	4741	7908	0.09%	0.032%
93	13.841	3875	3888	3912	rBV	1528471	2350001	27.32%	9.572%
94	13.999	3933	3937	3941	rBV3	589	658	0.01%	0.003%
95	14.256	4014	4017	4021	rBV3	445	477	0.01%	0.002%
96	14.330	4028	4040	4055	rBV	305122	475665	5.53%	1.937%
97	14.957	4232	4235	4239	rBV3	666	559	0.01%	0.002%
98	15.414	4367	4377	4388	rVB3	10002	19319	0.22%	0.079%
99	15.539	4414	4416	4420	rVB2	861	459	0.01%	0.002%
100	15.999	4551	4559	4575	rVB2	26033	41372	0.48%	0.169%




Sum of corrected areas: 24551106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048237.D
Acq On : 22 Apr 2022 20:07
Operator : SY/MD
Sample : N2486-08 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

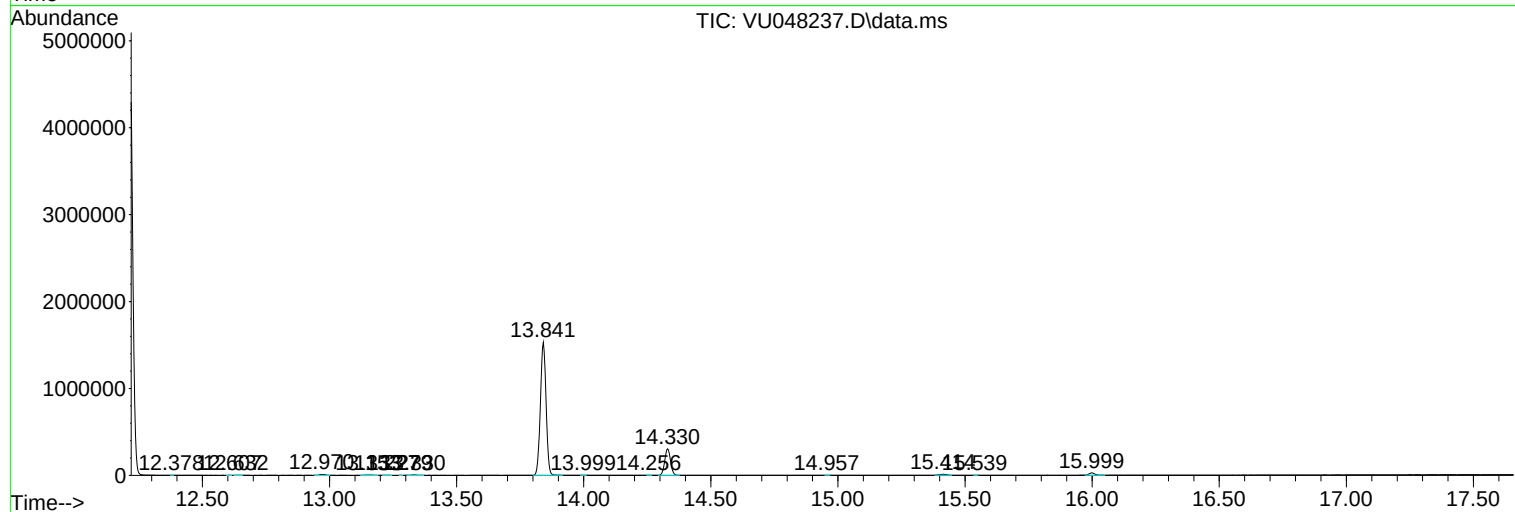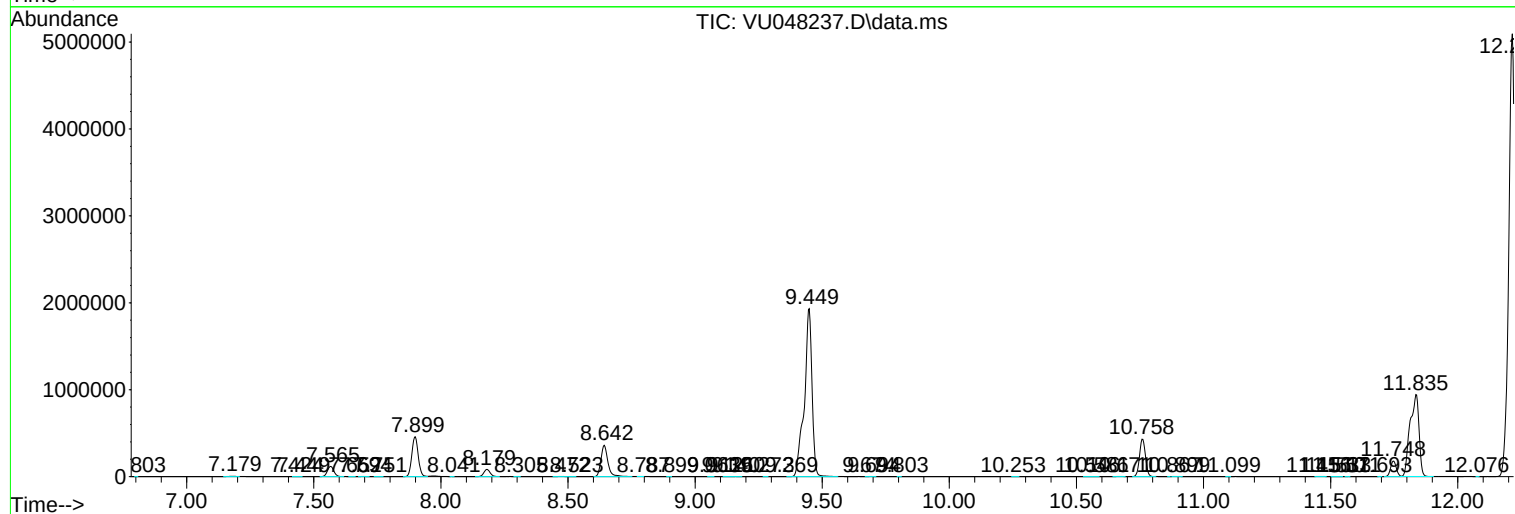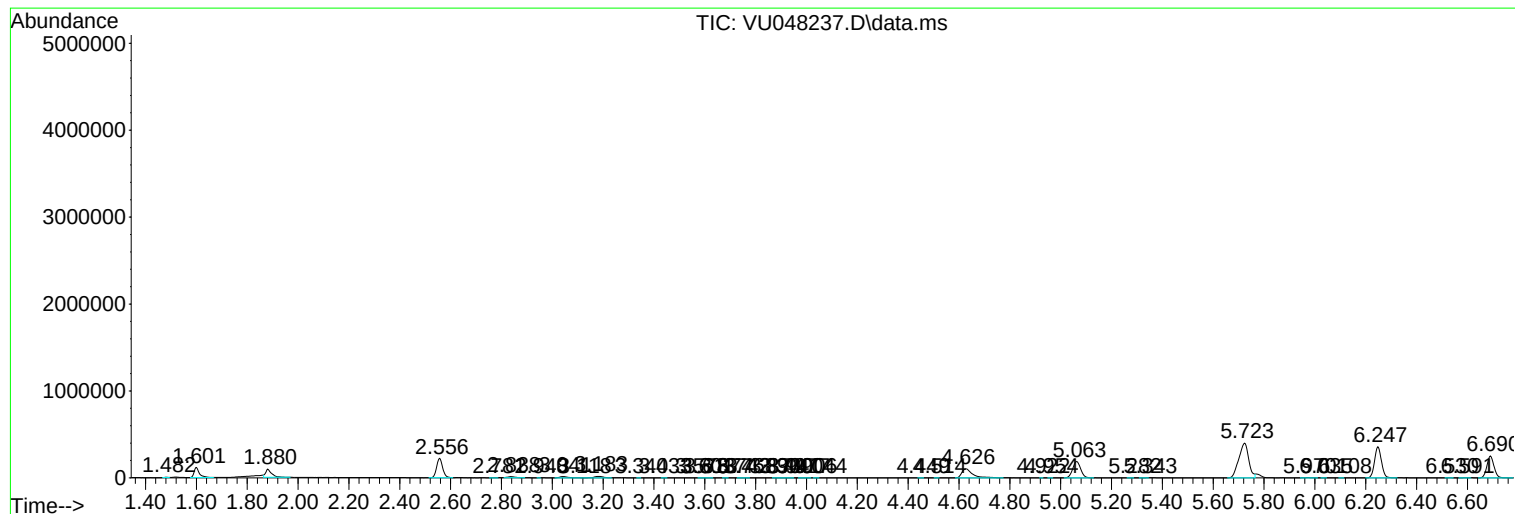

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048237.D
Acq On : 22 Apr 2022 20:07
Operator : SY/MD
Sample : N2486-08 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048237.D
Acq On : 22 Apr 2022 20:07
Operator : SY/MD
Sample : N2486-08 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc