


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048211.D
 Acq On : 22 Apr 2022 08:52
 Operator : SY/MD
 Sample : BFB070
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB070

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 25 01:24:32 2022

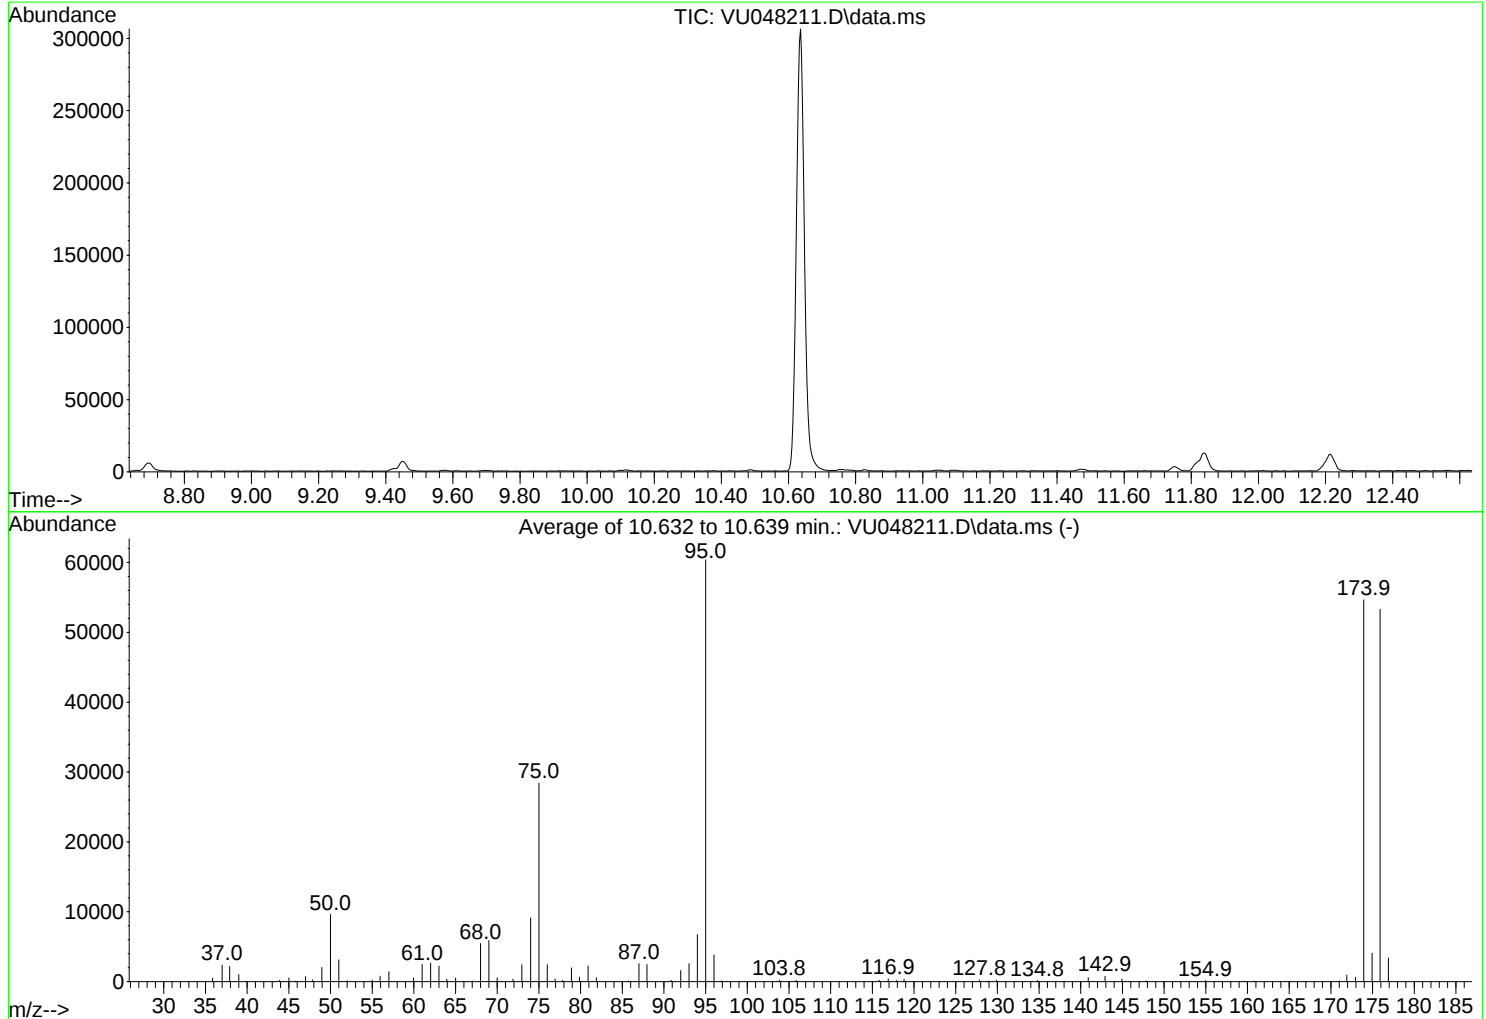

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9609	PASS
75	95	30	80	47.1	28421	PASS
95	95	100	100	100.0	60379	PASS
96	95	5	9	6.4	3836	PASS
173	174	0.00	2	1.1	607	PASS
174	95	50	120	90.5	54645	PASS
175	174	5	9	7.5	4077	PASS
176	174	95	101	97.6	53307	PASS
177	176	5	9	6.3	3371	PASS

m/z	Abundance
39.90	149.0
43.90	503.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.80	438.0
37.00	2388.0
37.90	2173.0
39.00	987.0
39.90	200.0
43.90	777.0
45.00	558.0
45.80	136.0
47.00	641.0
47.80	244.0
49.00	2181.0
50.00	9851.0
51.00	2990.0
52.10	143.0
55.00	253.0
56.00	850.0
57.00	1433.0
60.00	454.0
61.00	2440.0
62.00	2757.0
63.00	2310.0
64.00	339.0
65.00	510.0
68.00	5555.0
69.00	6050.0
70.00	579.0
71.90	372.0
72.90	2483.0
74.00	9148.0
75.00	28520.0
76.00	2389.0
77.00	350.0
77.80	177.0
78.90	1937.0
79.90	630.0
80.90	2300.0
81.90	546.0
85.70	121.0
86.10	101.0
87.00	2579.0
87.90	2606.0
90.80	200.0
92.00	1566.0
93.00	2553.0
94.00	6758.0
95.00	60416.0
96.00	3902.0
96.90	102.0
103.80	194.0
105.80	176.0
115.80	185.0
116.90	417.0
117.90	153.0
118.80	332.0
127.80	231.0
128.90	118.0
129.90	181.0
134.80	168.0
140.90	585.0
142.90	770.0
145.00	369.0
145.70	100.0
147.90	133.0
155.00	175.0
157.00	107.0
171.00	135.0
171.90	951.0
173.00	662.0
174.00	53872.0
175.00	4226.0
175.90	52688.0
176.90	3338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.80	515.0
37.00	2380.0
37.90	2276.0
39.00	1078.0
39.90	178.0
43.90	731.0
45.00	570.0
45.80	108.0
47.00	752.0
47.90	237.0
49.00	2126.0
50.00	9889.0
51.00	3204.0
52.00	137.0
55.00	235.0
55.90	818.0
57.00	1430.0
59.90	535.0
61.00	2549.0
62.00	2727.0
63.00	2289.0
64.00	343.0
65.00	502.0
67.00	127.0
68.00	5601.0
69.00	6056.0
70.00	554.0
71.90	377.0
72.90	2494.0
74.00	9447.0
75.00	29320.0
76.00	2481.0
76.90	375.0
77.80	194.0
78.90	2045.0
79.90	665.0
80.90	2333.0
81.90	581.0
85.70	120.0
87.00	2586.0
88.00	2506.0
90.90	175.0
92.00	1679.0
93.00	2648.0
94.00	6939.0
95.00	62320.0
96.00	3939.0
96.90	126.0
103.80	213.0
105.90	174.0
115.80	204.0
116.90	417.0
117.90	174.0
118.80	352.0
127.80	226.0
128.90	135.0
129.90	225.0
134.80	163.0
140.90	589.0
142.90	760.0
144.90	377.0
147.90	123.0
155.00	179.0
156.90	104.0
160.80	108.0
171.00	140.0
171.90	983.0
173.00	593.0
173.90	56240.0
175.00	4213.0
175.90	54992.0
176.90	3498.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	527.0
37.00	2297.0
37.90	2075.0
39.00	966.0
39.90	203.0
43.90	639.0
45.00	458.0
47.00	825.0
47.90	258.0
48.90	1847.0
50.00	9086.0
51.00	3151.0
52.00	124.0
55.00	174.0
55.90	706.0
57.00	1402.0
59.90	566.0
61.00	2420.0
62.00	2466.0
63.00	2039.0
63.90	325.0
65.00	488.0
67.00	170.0
68.00	5227.0
69.00	5549.0
70.00	428.0
71.90	360.0
73.00	2339.0
74.00	8784.0
75.00	27424.0
76.00	2390.0
77.00	368.0
77.90	215.0
78.90	1947.0
79.80	641.0
80.90	2123.0
81.90	556.0
85.80	109.0
87.00	2562.0
88.00	2258.0
90.90	153.0
92.00	1530.0
93.00	2535.0
94.00	6503.0
95.00	58400.0
96.00	3666.0
97.00	125.0
103.90	233.0
105.90	212.0
115.80	236.0
116.90	364.0
117.90	181.0
118.80	324.0
127.90	232.0
128.90	128.0
129.90	237.0
131.00	106.0
134.80	169.0
140.90	530.0
142.90	765.0
144.90	366.0
147.80	119.0
154.90	160.0
160.80	101.0
171.00	105.0
171.90	900.0
172.90	567.0
174.00	53824.0
174.90	3791.0
175.90	52240.0
176.90	3278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070