

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048246.D
 Acq On : 23 Apr 2022 15:14
 Operator : SY/MD
 Sample : N2488-06DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX4DL

Quant Time: Apr 25 01:26:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 25 01:24:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	321561	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	315827	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	144325	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	108986	46.738	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.480%
7) Chloroethane-d5	1.903	69	86958	47.294	ug/L	0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.580%
11) 1,1-Dichloroethene-d2	2.565	63	128956	30.227	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.460%
21) 2-Butanone-d5	4.620	46	174451	87.161	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.160%
24) Chloroform-d	5.063	84	185505	43.478	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.960%
26) 1,2-Dichloroethane-d4	5.703	65	117289	44.821	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.640%
32) Benzene-d6	5.729	84	383924	48.310	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.620%
36) 1,2-Dichloropropane-d6	6.690	67	126488	51.826	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.660%
41) Toluene-d8	7.899	98	321262	41.492	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.980%
43) trans-1,3-Dichloroprop...	8.179	79	46484	37.594	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.180%
47) 2-Hexanone-d5	8.632	63	114200	79.930	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.930%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	194968	46.548	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.100%
66) 1,2-Dichlorobenzene-d4	12.195	152	127792	49.769	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.540%
Target Compounds						
					Qvalue	
33) Benzene	5.774	78	150677	16.482	ug/L	100
51) Chlorobenzene	9.446	112	164136	24.100	ug/L	99
64) 1,3-Dichlorobenzene	11.748	146	27592	6.364	ug/L	99
65) 1,4-Dichlorobenzene	11.838	146	142342	31.698	ug/L	97
67) 1,2-Dichlorobenzene	12.214	146	306624	70.683	ug/L	99
70) 1,2,4-trichlorobenzene	13.844	180	20306	6.584	ug/L	97
72) 1,2,3-Trichlorobenzene	14.333	180	9272	2.999	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048246.D
Acq On : 23 Apr 2022 15:14
Operator : SY/MD
Sample : N2488-06DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX4DL

Quant Time: Apr 25 01:26:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 25 01:24:32 2022
Response via : Initial Calibration




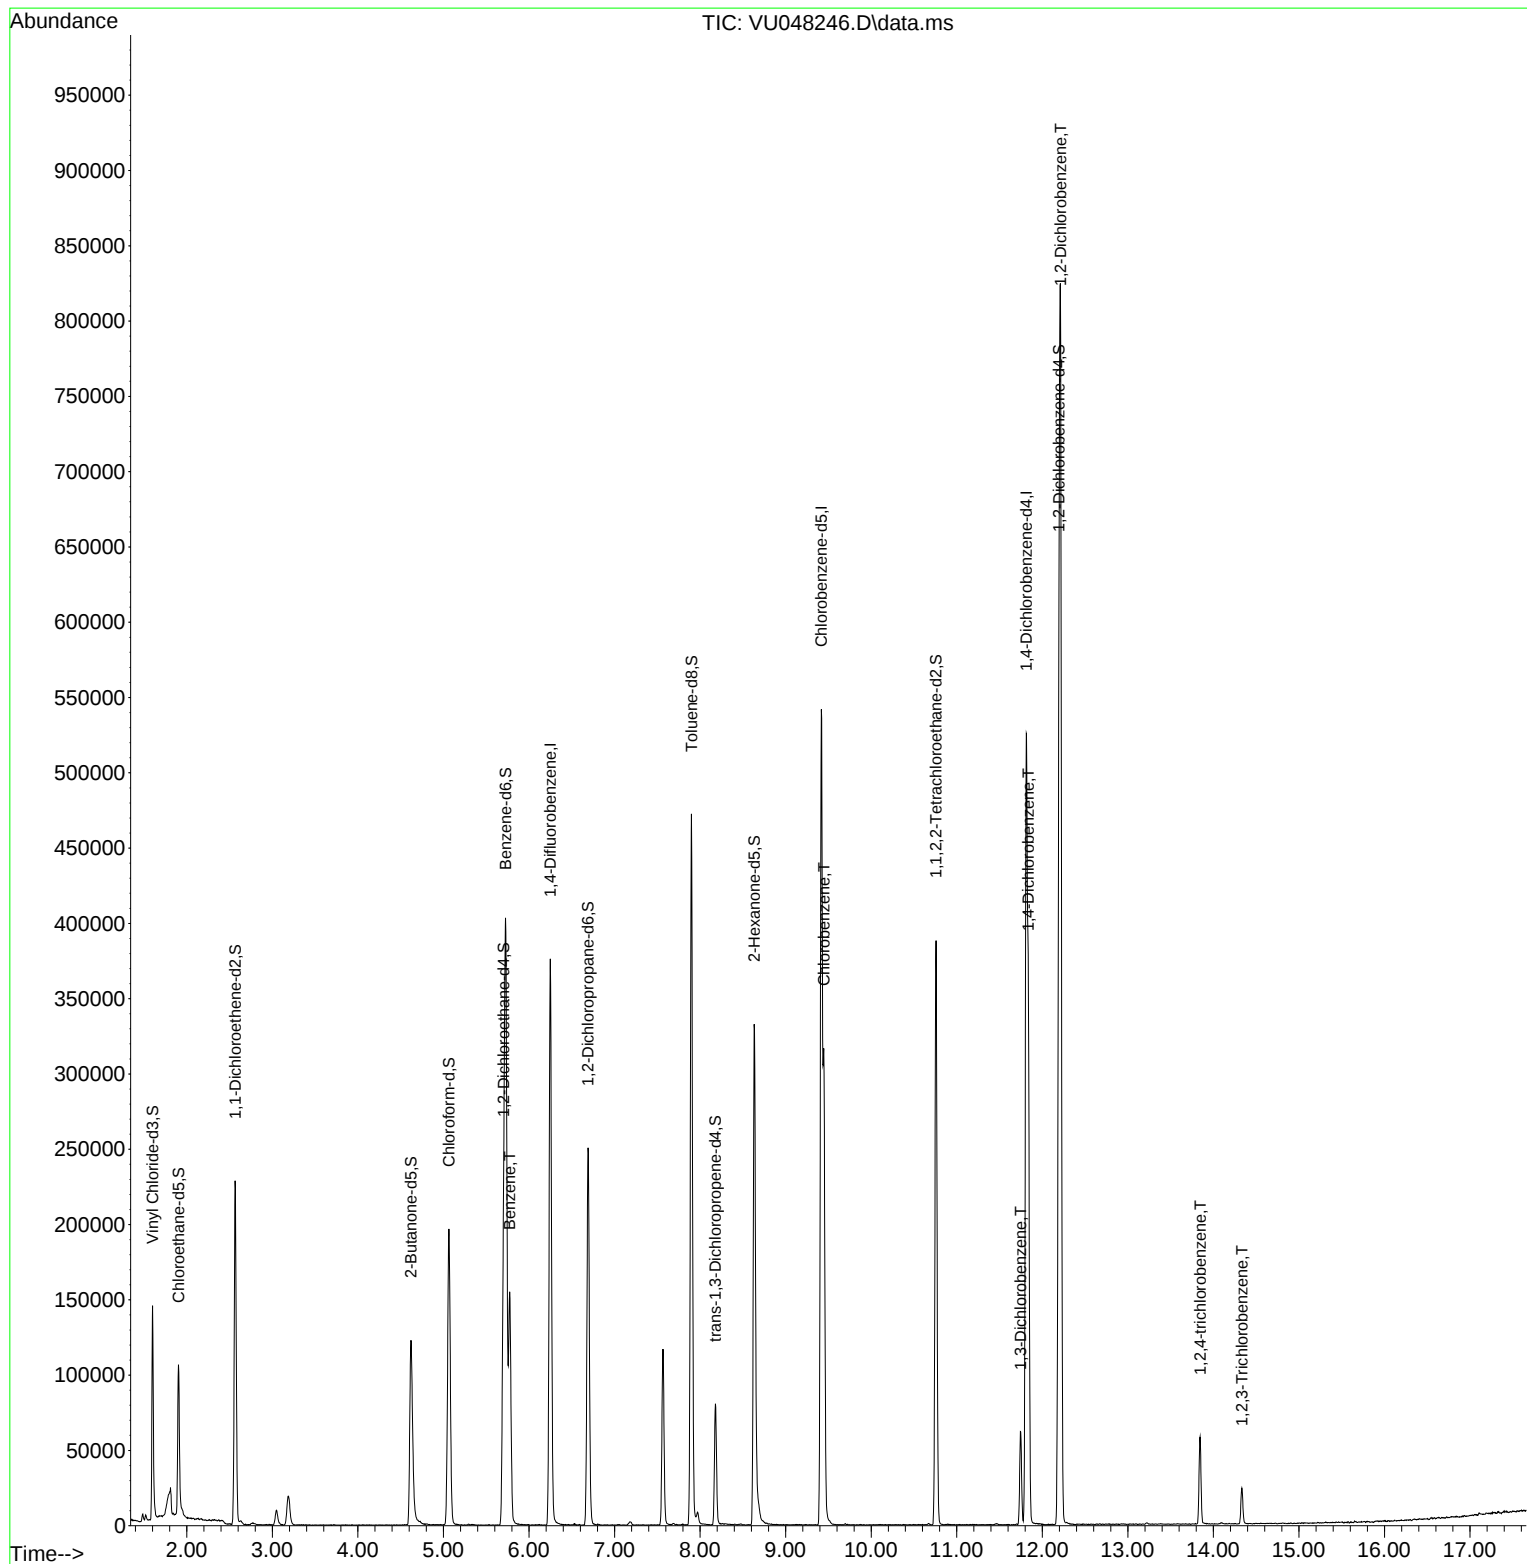


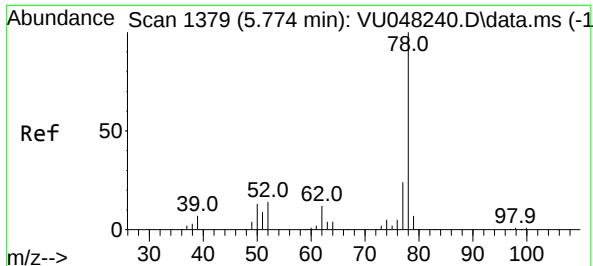

#33
Benzene
Concen: 16.482 ug/L
RT: 5.774 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU048246.D
Acq: 23 Apr 2022 15:14

Instrument :
MSVOA_U
ClientSampleId :
C0HX4DL




Tgt Ion: 78 Resp: 150677

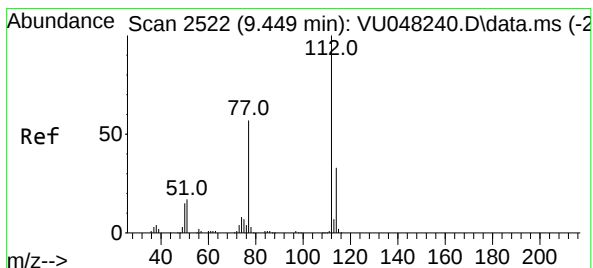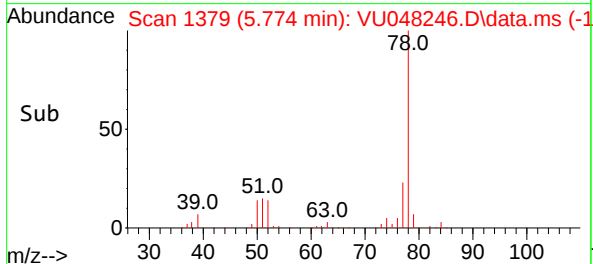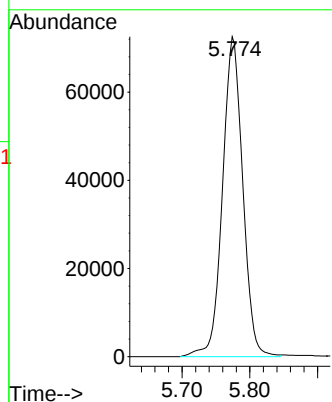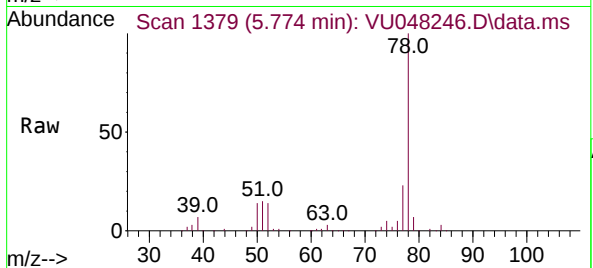


#51
Chlorobenzene
Concen: 24.100 ug/L
RT: 9.446 min Scan# 2521
Delta R.T. -0.003 min
Lab File: VU048246.D
Acq: 23 Apr 2022 15:14

Tgt Ion: 112 Resp: 164136

Ion	Ratio	Lower	Upper
112	100		
114	31.7	22.1	41.1
77	55.1	43.4	65.0


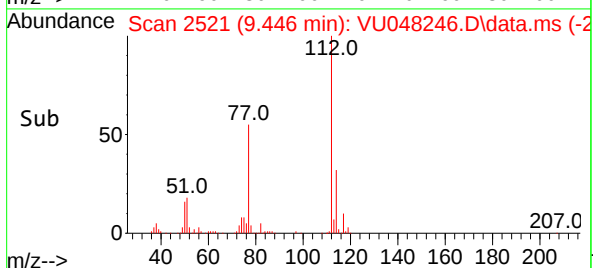
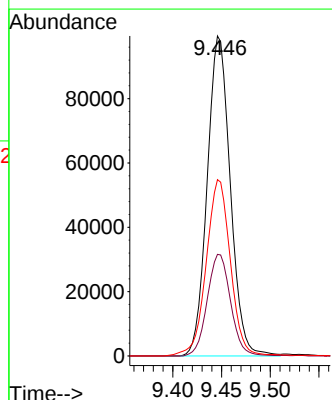
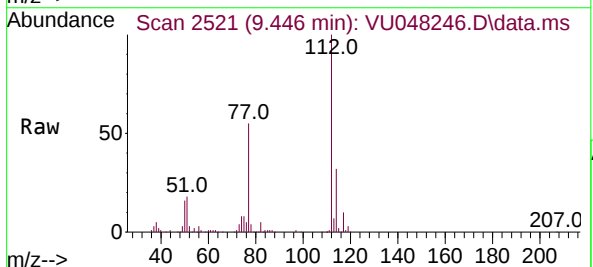


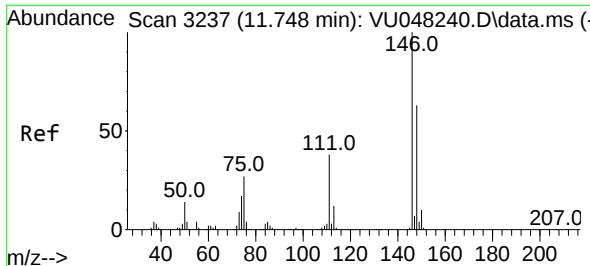

#64
1,3-Dichlorobenzene
Concen: 6.364 ug/L
RT: 11.748 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU048246.D
Acq: 23 Apr 2022 15:14




Instrument :
MSVOA_U
ClientSampleId :
C0HX4DL


Tgt Ion:146 Resp: 27592
Ion Ratio Lower Upper
146 100
111 37.2 26.7 49.7
148 62.7 44.4 82.5

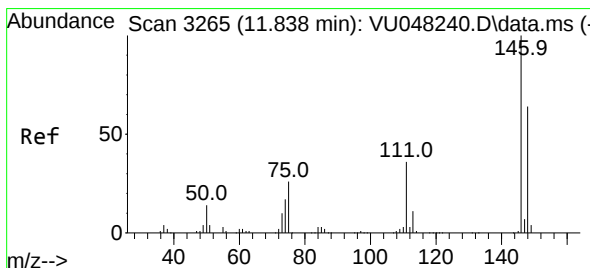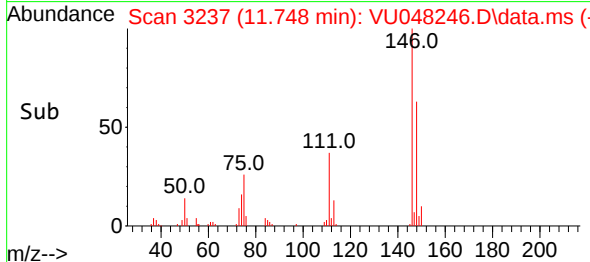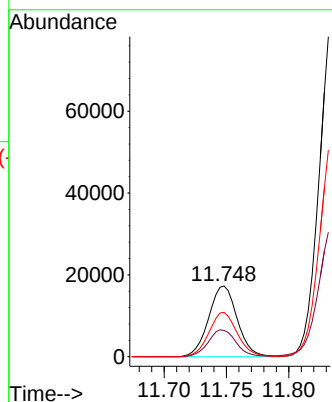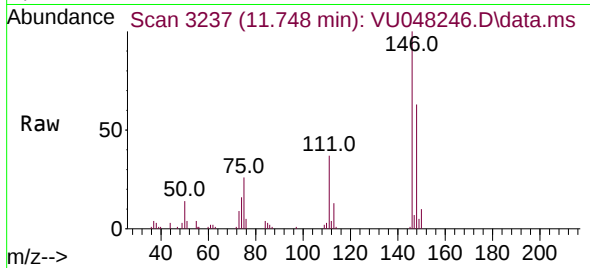

#65
1,4-Dichlorobenzene
Concen: 31.698 ug/L
RT: 11.838 min Scan# 3265
Delta R.T. 0.000 min
Lab File: VU048246.D
Acq: 23 Apr 2022 15:14

Tgt Ion:146 Resp: 142342
Ion Ratio Lower Upper
146 100
111 36.7 25.3 47.1
148 66.5 44.5 82.7

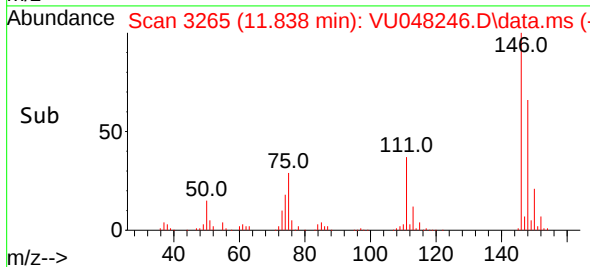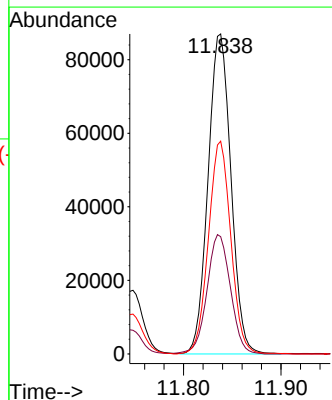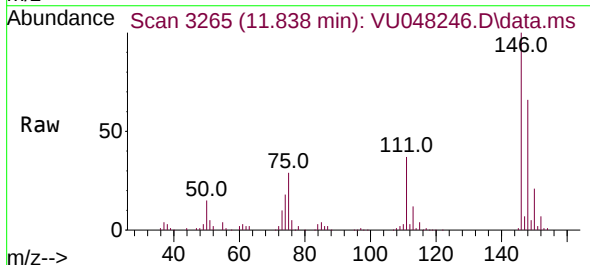

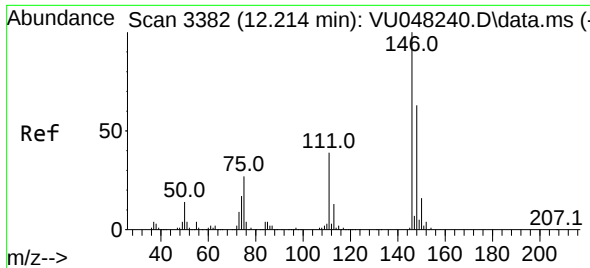

#67

1,2-Dichlorobenzene

Concen: 70.683 ug/L

RT: 12.214 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU048246.D

Acq: 23 Apr 2022 15:14

Instrument :

MSVOA_U

ClientSampleId :

C0HX4DL





Tgt Ion:146 Resp: 306624

Ion Ratio Lower Upper

146 100

111 40.6 31.7 47.5

148 65.2 51.4 77.2

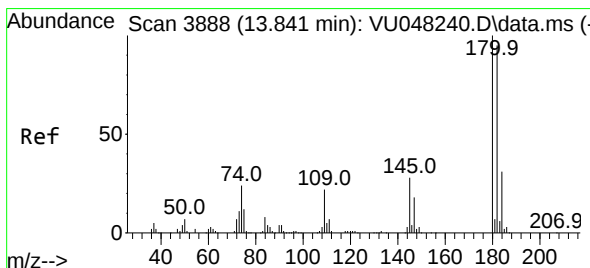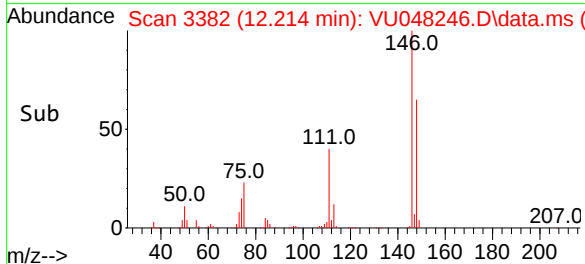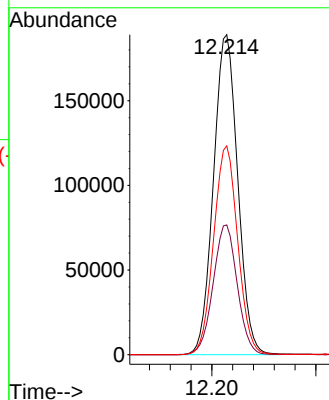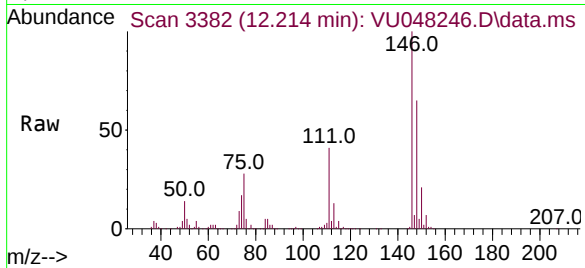

#70

1,2,4-trichlorobenzene

Concen: 6.584 ug/L

RT: 13.844 min Scan# 3889

Delta R.T. 0.003 min

Lab File: VU048246.D

Acq: 23 Apr 2022 15:14




Tgt Ion:180 Resp: 20306


Ion Ratio Lower Upper

180 100

182 98.2 76.2 114.2


145 27.0 21.8 32.8

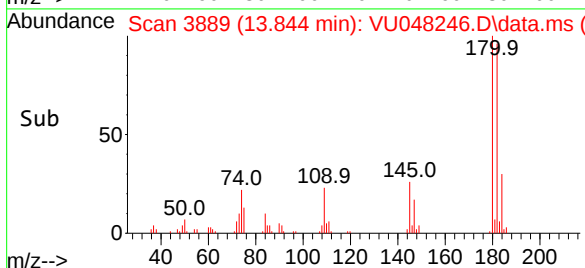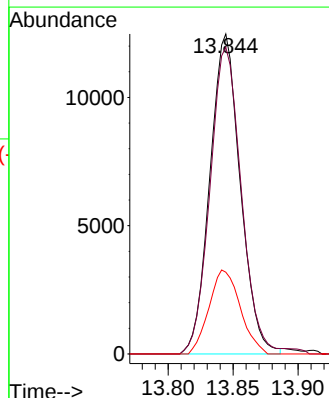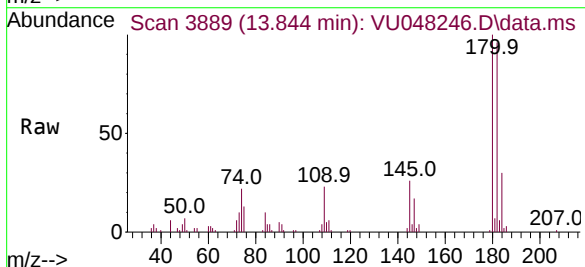

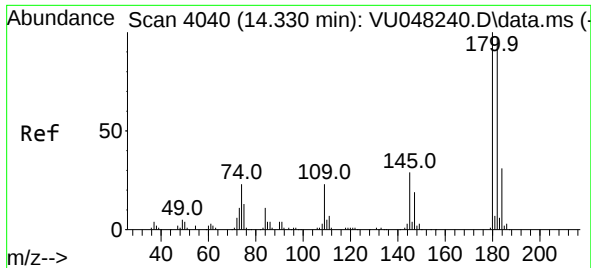

#72
 1,2,3-Trichlorobenzene
 Concen: 2.999 ug/L
 RT: 14.333 min Scan# 4041
 Delta R.T. 0.003 min
 Lab File: VU048246.D
 Acq: 23 Apr 2022 15:14

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX4DL

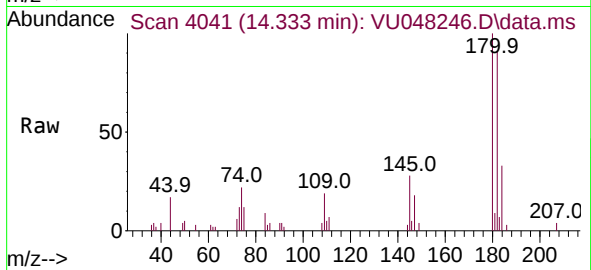

Tgt Ion:180 Resp: 9272

Ion	Ratio	Lower	Upper
180	100		
182	89.4	77.4	116.0
145	27.8	22.8	34.2

