

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048241.D
 Acq On : 23 Apr 2022 13:13
 Operator : SY/MD
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	51	rBV2	5790	7303	0.67%	0.084%
2	1.601	73	81	100	rBV	133197	173212	15.92%	1.984%
3	1.880	162	168	190	rVB	91103	150570	13.84%	1.725%
4	2.514	361	365	367	rBV2	373	298	0.03%	0.003%
5	2.559	367	379	397	rVV	228387	381757	35.09%	4.373%
6	2.684	416	418	421	rVB	403	206	0.02%	0.002%
7	2.874	474	477	479	rBV	264	158	0.01%	0.002%
8	2.893	480	483	489	rVV4	336	438	0.04%	0.005%
9	3.128	554	556	559	rVB2	294	134	0.01%	0.002%
10	3.183	559	573	587	rBV	8220	18694	1.72%	0.214%
11	3.285	602	605	610	rBV2	321	363	0.03%	0.004%
12	3.321	614	616	619	rVV	321	237	0.02%	0.003%
13	3.350	623	625	628	rVB	338	174	0.02%	0.002%
14	3.449	653	656	659	rBV	191	160	0.01%	0.002%
15	3.703	732	735	738	rVB2	210	131	0.01%	0.002%
16	3.765	748	754	758	rVB	365	304	0.03%	0.003%
17	3.797	762	764	767	rVB	357	178	0.02%	0.002%
18	3.816	767	770	772	rBV	192	157	0.01%	0.002%
19	3.858	781	783	786	rBV2	199	139	0.01%	0.002%
20	3.951	808	812	815	rBV2	204	161	0.01%	0.002%
21	4.176	879	882	885	rBV	250	193	0.02%	0.002%
22	4.311	921	924	927	rVB2	301	188	0.02%	0.002%
23	4.353	935	937	942	rVB3	290	175	0.02%	0.002%
24	4.527	988	991	995	rVB2	188	137	0.01%	0.002%
25	4.623	1007	1021	1045	rBV	112278	284756	26.17%	3.261%
26	5.002	1135	1139	1141	rVV2	221	168	0.02%	0.002%
27	5.063	1141	1158	1184	rVV	189222	414559	38.10%	4.748%
28	5.189	1195	1197	1200	rVV	261	197	0.02%	0.002%
29	5.205	1200	1202	1206	rVV2	253	173	0.02%	0.002%
30	5.289	1223	1228	1232	rBV3	338	426	0.04%	0.005%
31	5.330	1236	1241	1243	rBV3	968	911	0.08%	0.010%
32	5.398	1259	1262	1266	rVB	196	155	0.01%	0.002%
33	5.427	1266	1271	1272	rBV	147	130	0.01%	0.001%
34	5.723	1342	1363	1392	rBV2	406211	1088009	100.00%	12.462%
35	5.838	1396	1399	1401	rVV4	230	146	0.01%	0.002%
36	5.967	1433	1439	1442	rBV4	1640	1761	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048241.D
 Acq On : 23 Apr 2022 13:13
 Operator : SY/MD
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.041	1460	1462	1465	rVB3	321	162	0.01%	0.002%
38	6.157	1494	1498	1504	rBV3	343	461	0.04%	0.005%
39	6.247	1511	1526	1547	rBV	356827	679284	62.43%	7.780%
40	6.398	1571	1573	1576	rVB3	322	148	0.01%	0.002%
41	6.462	1590	1593	1599	rBV2	201	174	0.02%	0.002%
42	6.530	1605	1614	1623	rBV6	1234	2170	0.20%	0.025%
43	6.597	1628	1635	1637	rBV3	469	503	0.05%	0.006%
44	6.690	1648	1664	1682	rBV	251598	486577	44.72%	5.573%
45	6.800	1694	1698	1702	rVB4	391	359	0.03%	0.004%
46	6.864	1714	1718	1720	rBV	178	157	0.01%	0.002%
47	7.044	1771	1774	1775	rBV	294	160	0.01%	0.002%
48	7.079	1782	1785	1788	rBV2	302	175	0.02%	0.002%
49	7.176	1803	1815	1829	rBV5	4366	10114	0.93%	0.116%
50	7.282	1844	1848	1849	rBV	233	140	0.01%	0.002%
51	7.292	1849	1851	1854	rVV	321	190	0.02%	0.002%
52	7.324	1858	1861	1865	rVV2	297	242	0.02%	0.003%
53	7.565	1921	1936	1955	rBV	116553	204528	18.80%	2.343%
54	7.697	1968	1977	1983	rBV4	1022	1603	0.15%	0.018%
55	7.796	2000	2008	2011	rBV3	1179	1359	0.12%	0.016%
56	7.899	2026	2040	2056	rBV	461826	802798	73.79%	9.195%
57	8.179	2114	2127	2142	rVV	81605	138025	12.69%	1.581%
58	8.568	2245	2248	2252	rBV3	186	175	0.02%	0.002%
59	8.636	2256	2269	2311	rBV	360505	692370	63.64%	7.930%
60	9.063	2398	2402	2403	rBV	275	163	0.01%	0.002%
61	9.115	2416	2418	2423	rBV3	330	289	0.03%	0.003%
62	9.166	2429	2434	2438	rVB	264	205	0.02%	0.002%
63	9.243	2456	2458	2464	rVB3	265	241	0.02%	0.003%
64	9.282	2467	2470	2474	rVB2	190	166	0.02%	0.002%
65	9.417	2498	2512	2533	rBV	535468	892121	82.00%	10.218%
66	9.575	2553	2561	2566	rVV4	581	762	0.07%	0.009%
67	9.597	2566	2568	2572	rVB2	315	182	0.02%	0.002%
68	9.697	2592	2599	2606	rVV3	815	1140	0.10%	0.013%
69	9.941	2672	2675	2677	rBV2	220	152	0.01%	0.002%
70	10.108	2720	2727	2731	rBV4	786	1089	0.10%	0.012%
71	10.256	2768	2773	2777	rBV2	283	340	0.03%	0.004%
72	10.288	2780	2783	2790	rBV3	435	546	0.05%	0.006%
73	10.581	2869	2874	2876	rBV2	345	266	0.02%	0.003%
74	10.665	2896	2900	2902	rBV2	1012	879	0.08%	0.010%
75	10.758	2916	2929	2946	rBV	421152	680562	62.55%	7.795%
76	10.861	2958	2961	2962	rBV	263	146	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048241.D
 Acq On : 23 Apr 2022 13:13
 Operator : SY/MD
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK109

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.967	2990	2994	2998	rBV2	257	276	0.03%	0.003%
78	10.999	3002	3004	3007	rVV2	212	141	0.01%	0.002%
79	11.304	3097	3099	3104	rVB	303	215	0.02%	0.002%
80	11.452	3143	3145	3146	rBV	413	231	0.02%	0.003%
81	11.462	3146	3148	3159	rVB4	1198	1616	0.15%	0.019%
82	11.539	3168	3172	3176	rBV2	274	262	0.02%	0.003%
83	11.693	3217	3220	3225	rBV3	490	463	0.04%	0.005%
84	11.716	3225	3227	3231	rVB	307	180	0.02%	0.002%
85	11.745	3231	3236	3245	rBV3	1217	1672	0.15%	0.019%
86	11.812	3245	3257	3279	rBV	497294	812071	74.64%	9.301%
87	11.944	3296	3298	3302	rVB3	663	358	0.03%	0.004%
88	12.041	3326	3328	3330	rBV	264	133	0.01%	0.002%
89	12.195	3362	3376	3391	rBV	457721	747310	68.69%	8.559%
90	12.391	3434	3437	3440	rBV	331	262	0.02%	0.003%
91	12.542	3481	3484	3488	rBV2	288	252	0.02%	0.003%
92	12.619	3502	3508	3510	rBV2	477	518	0.05%	0.006%
93	12.771	3549	3555	3561	rBV3	1018	1269	0.12%	0.015%
94	12.999	3623	3626	3629	rBV	367	260	0.02%	0.003%
95	13.169	3675	3679	3682	rBV3	358	306	0.03%	0.004%
96	13.227	3690	3697	3705	rBV3	1402	1957	0.18%	0.022%
97	13.468	3769	3772	3773	rBV	310	204	0.02%	0.002%
98	13.848	3882	3890	3898	rBV3	5021	7147	0.66%	0.082%
99	14.092	3958	3966	3978	rVB2	11095	17875	1.64%	0.205%
100	14.333	4034	4041	4052	rVB2	5452	7871	0.72%	0.090%




Sum of corrected areas: 8730830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048241.D
Acq On : 23 Apr 2022 13:13
Operator : SY/MD
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

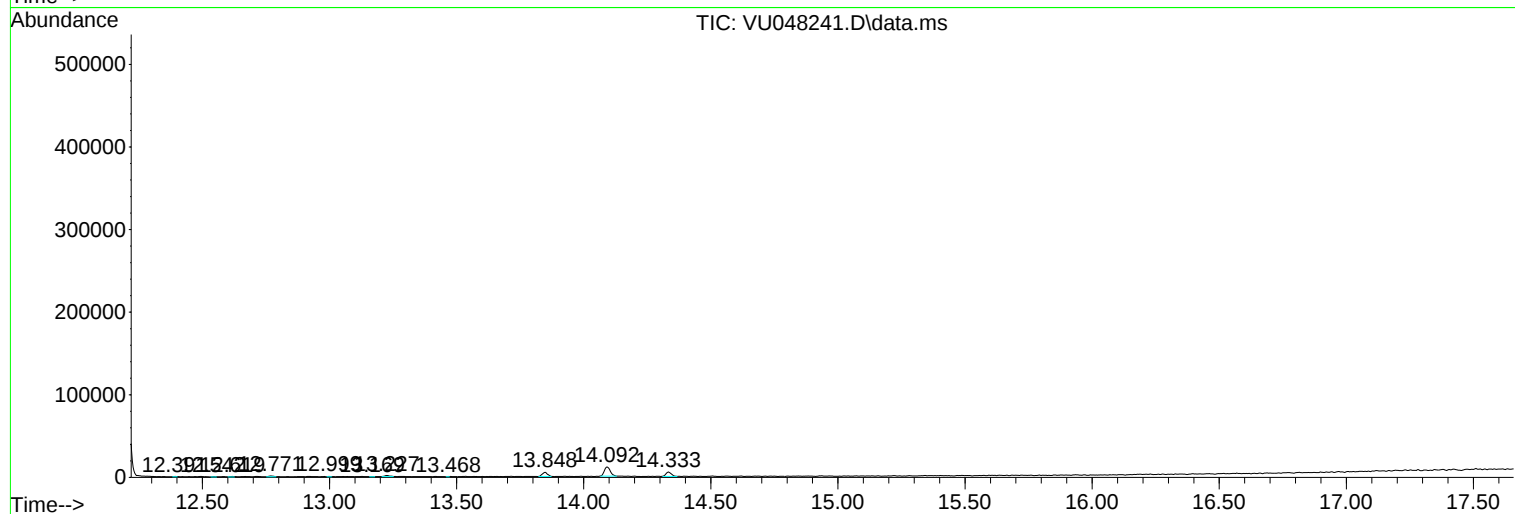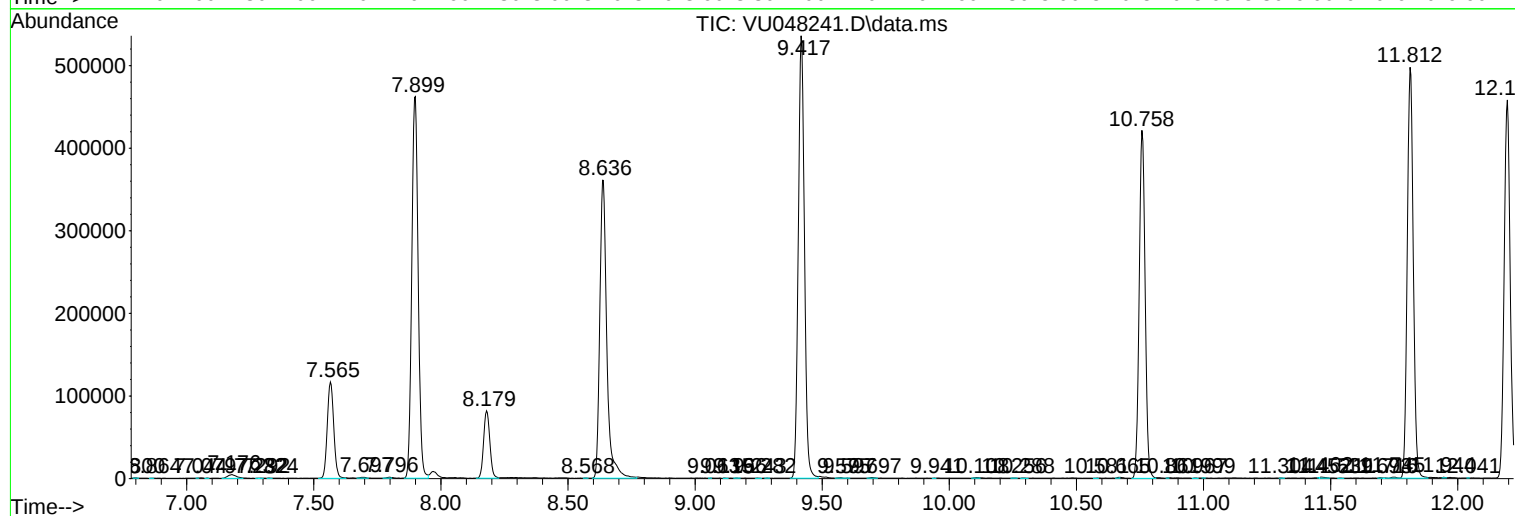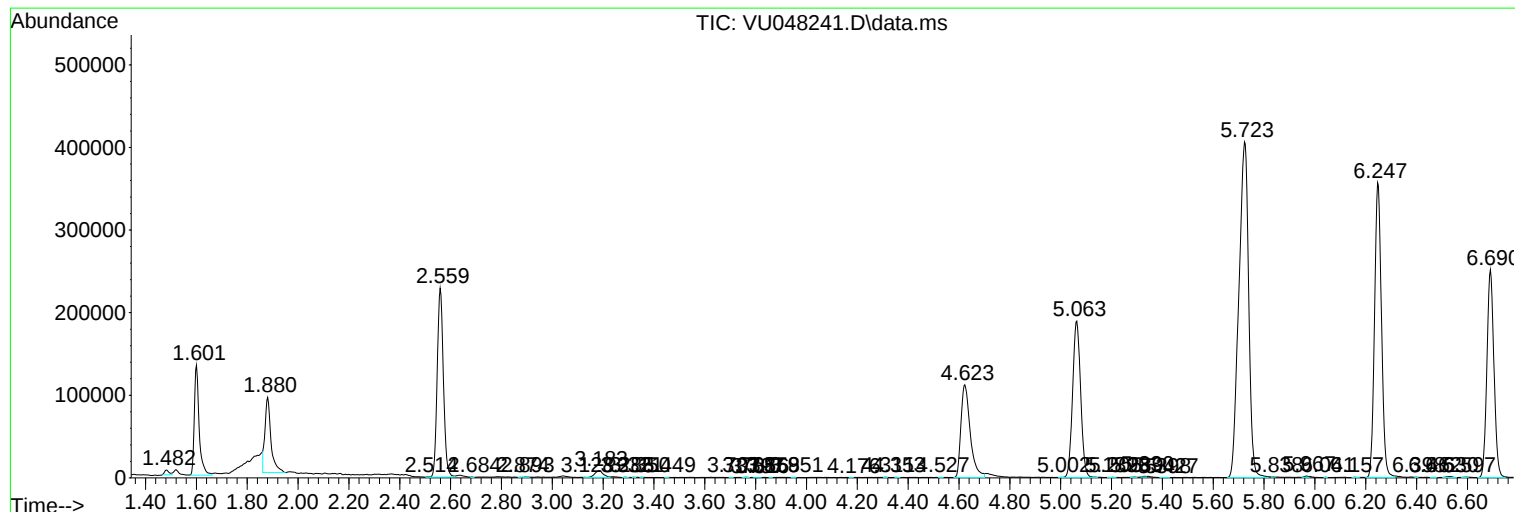

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048241.D
Acq On : 23 Apr 2022 13:13
Operator : SY/MD
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048241.D
Acq On : 23 Apr 2022 13:13
Operator : SY/MD
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
