

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048242.D
 Acq On : 23 Apr 2022 13:40
 Operator : SY/MD
 Sample : N2486-18 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	51	rBV3	4916	7537	0.21%	0.063%
2	1.601	73	81	100	rBV	128080	167618	4.73%	1.396%
3	1.887	164	170	192	rVB	87049	137501	3.88%	1.145%
4	2.562	367	380	396	rBV	221828	366047	10.34%	3.049%
5	2.687	414	419	421	rBV2	317	246	0.01%	0.002%
6	2.765	437	443	445	rBV3	1255	1324	0.04%	0.011%
7	2.880	478	479	484	rVB2	314	251	0.01%	0.002%
8	3.044	518	530	541	rBV2	4741	9429	0.27%	0.079%
9	3.183	558	573	602	rBV	18268	45712	1.29%	0.381%
10	3.369	628	631	636	rBV2	231	253	0.01%	0.002%
11	3.806	764	767	776	rVB2	257	290	0.01%	0.002%
12	4.009	825	830	832	rBV2	218	219	0.01%	0.002%
13	4.064	842	847	850	rVV2	198	247	0.01%	0.002%
14	4.141	865	871	878	rBV2	280	304	0.01%	0.003%
15	4.337	926	932	937	rBV2	196	248	0.01%	0.002%
16	4.430	957	961	967	rVB2	154	200	0.01%	0.002%
17	4.555	995	1000	1004	rBV3	326	409	0.01%	0.003%
18	4.623	1008	1021	1059	rBV	107195	277570	7.84%	2.312%
19	4.925	1108	1115	1119	rVB3	253	349	0.01%	0.003%
20	5.063	1141	1158	1178	rVV2	186485	403959	11.41%	3.364%
21	5.285	1222	1227	1228	rBV	462	367	0.01%	0.003%
22	5.327	1235	1240	1241	rBV2	771	589	0.02%	0.005%
23	5.453	1275	1279	1283	rBV2	300	340	0.01%	0.003%
24	5.723	1338	1363	1387	rBV2	391848	1048650	29.62%	8.734%
25	5.935	1425	1429	1430	rBV2	381	213	0.01%	0.002%
26	5.973	1435	1441	1448	rVV3	956	1412	0.04%	0.012%
27	6.067	1466	1470	1473	rBV	243	249	0.01%	0.002%
28	6.118	1483	1486	1489	rVB2	365	263	0.01%	0.002%
29	6.182	1503	1506	1512	rVB2	231	235	0.01%	0.002%
30	6.250	1512	1527	1557	rBV	355535	674726	19.06%	5.620%
31	6.414	1574	1578	1581	rVB2	383	273	0.01%	0.002%
32	6.475	1593	1597	1601	rVB2	287	225	0.01%	0.002%
33	6.530	1607	1614	1621	rVB2	651	1057	0.03%	0.009%
34	6.594	1631	1634	1636	rBV2	334	238	0.01%	0.002%
35	6.690	1650	1664	1683	rBV	248109	479415	13.54%	3.993%
36	6.806	1696	1700	1703	rBV2	319	256	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048242.D
 Acq On : 23 Apr 2022 13:40
 Operator : SY/MD
 Sample : N2486-18 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.822	1703	1705	1709	rVB3	391	256	0.01%	0.002%
38	6.989	1753	1757	1764	rVB2	209	246	0.01%	0.002%
39	7.028	1764	1769	1773	rBV2	232	259	0.01%	0.002%
40	7.054	1773	1777	1782	rVB2	348	373	0.01%	0.003%
41	7.137	1797	1803	1805	rBV2	286	258	0.01%	0.002%
42	7.176	1805	1815	1827	rBV3	3657	8006	0.23%	0.067%
43	7.234	1827	1833	1836	rVB2	281	258	0.01%	0.002%
44	7.305	1849	1855	1859	rBV2	305	233	0.01%	0.002%
45	7.343	1859	1867	1871	rBV2	169	271	0.01%	0.002%
46	7.565	1923	1936	1953	rVV	112515	196512	5.55%	1.637%
47	7.639	1956	1959	1966	rVB4	827	944	0.03%	0.008%
48	7.690	1968	1975	1982	rBV4	1036	1549	0.04%	0.013%
49	7.739	1987	1990	1993	rVB2	267	205	0.01%	0.002%
50	7.768	1996	1999	2002	rBV2	242	218	0.01%	0.002%
51	7.800	2003	2009	2013	rBV4	1030	1034	0.03%	0.009%
52	7.899	2025	2040	2055	rBV	458928	794963	22.45%	6.621%
53	8.112	2102	2106	2108	rBV2	235	183	0.01%	0.002%
54	8.179	2113	2127	2146	rBV	82013	136069	3.84%	1.133%
55	8.250	2146	2149	2152	rBV2	349	276	0.01%	0.002%
56	8.285	2157	2160	2163	rVV2	390	246	0.01%	0.002%
57	8.475	2213	2219	2222	rBV3	324	336	0.01%	0.003%
58	8.639	2257	2270	2307	rBV	339062	654810	18.49%	5.454%
59	9.009	2381	2385	2387	rVB	397	279	0.01%	0.002%
60	9.041	2393	2395	2401	rVB2	218	219	0.01%	0.002%
61	9.070	2401	2404	2407	rBV3	301	220	0.01%	0.002%
62	9.115	2414	2418	2421	rBV2	293	261	0.01%	0.002%
63	9.420	2499	2513	2517	rBV	547253	894311	25.26%	7.448%
64	9.613	2570	2573	2578	rBV2	196	198	0.01%	0.002%
65	9.694	2595	2598	2610	rVB3	934	1109	0.03%	0.009%
66	10.108	2722	2727	2728	rBV2	567	312	0.01%	0.003%
67	10.221	2754	2762	2765	rBV2	224	308	0.01%	0.003%
68	10.668	2896	2901	2908	rBV2	1063	1189	0.03%	0.010%
69	10.758	2916	2929	2951	rBV	401331	648046	18.30%	5.397%
70	10.935	2980	2984	2987	rBV2	291	221	0.01%	0.002%
71	11.121	3038	3042	3045	rVB2	444	301	0.01%	0.003%
72	11.163	3045	3055	3062	rBV2	315	499	0.01%	0.004%
73	11.298	3092	3097	3105	rVV2	270	490	0.01%	0.004%
74	11.340	3106	3110	3114	rVB	239	249	0.01%	0.002%
75	11.465	3140	3149	3163	rVB6	1253	2744	0.08%	0.023%
76	11.523	3163	3167	3173	rBV	285	322	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048242.D
 Acq On : 23 Apr 2022 13:40
 Operator : SY/MD
 Sample : N2486-18 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.619	3194	3197	3199	rVV	365	205	0.01%	0.002%
78	11.700	3214	3222	3226	rBV3	495	639	0.02%	0.005%
79	11.748	3226	3237	3246	rBV	42620	65961	1.86%	0.549%
80	11.812	3246	3257	3284	rVB2	556527	1117554	31.56%	9.308%
81	11.931	3290	3294	3295	rBV2	384	298	0.01%	0.002%
82	12.211	3361	3381	3399	rBV2	1812565	3540577	100.00%	29.488%
83	12.353	3421	3425	3426	rBV2	338	257	0.01%	0.002%
84	12.484	3463	3466	3468	rBV3	331	255	0.01%	0.002%
85	12.684	3520	3528	3533	rBV2	468	905	0.03%	0.008%
86	12.774	3554	3556	3561	rBV4	639	408	0.01%	0.003%
87	12.947	3607	3610	3613	rVB2	340	269	0.01%	0.002%
88	12.976	3613	3619	3627	rVB4	1642	2317	0.07%	0.019%
89	13.012	3627	3630	3633	rBV2	417	418	0.01%	0.003%
90	13.079	3648	3651	3654	rBV	309	309	0.01%	0.003%
91	13.227	3692	3697	3698	rBV2	553	479	0.01%	0.004%
92	13.333	3727	3730	3732	rBV3	480	337	0.01%	0.003%
93	13.722	3848	3851	3854	rBV	419	310	0.01%	0.003%
94	13.738	3854	3856	3862	rVB2	421	338	0.01%	0.003%
95	13.767	3862	3865	3868	rBV3	398	299	0.01%	0.002%
96	13.841	3877	3888	3902	rBV	154743	246731	6.97%	2.055%
97	13.970	3925	3928	3933	rBV3	488	433	0.01%	0.004%
98	14.092	3958	3966	3975	rBV	6691	10192	0.29%	0.085%
99	14.243	4012	4013	4018	rBV	314	195	0.01%	0.002%
100	14.333	4031	4041	4055	rBV2	25235	40156	1.13%	0.334%




Sum of corrected areas: 12006846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048242.D
Acq On : 23 Apr 2022 13:40
Operator : SY/MD
Sample : N2486-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

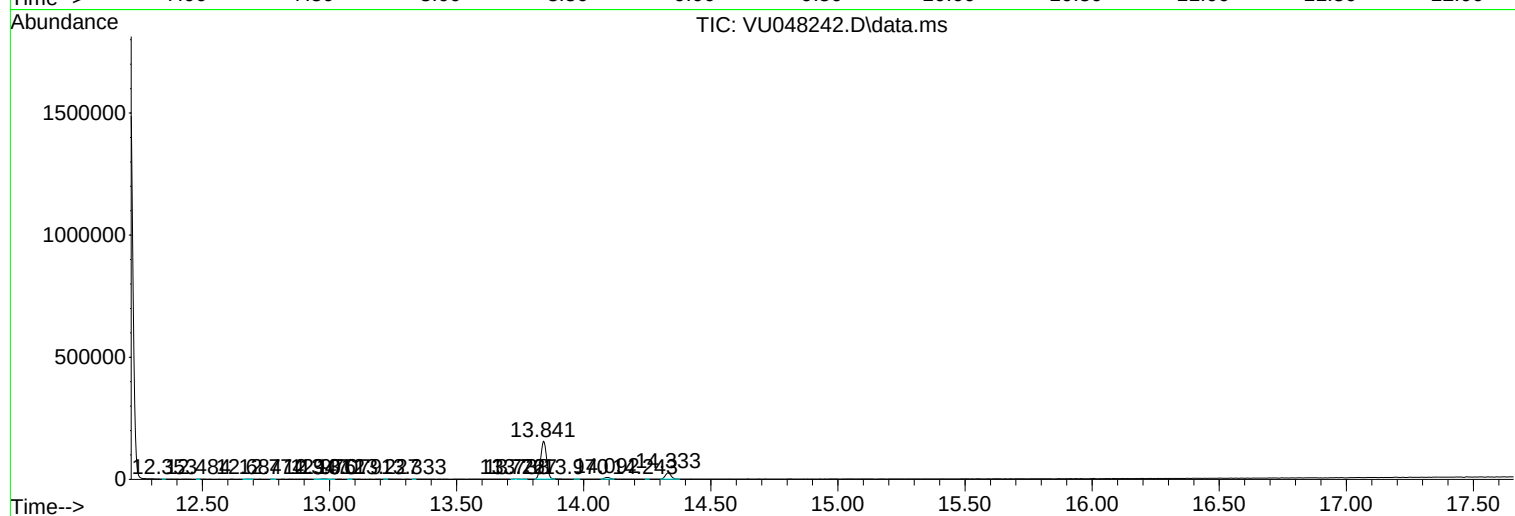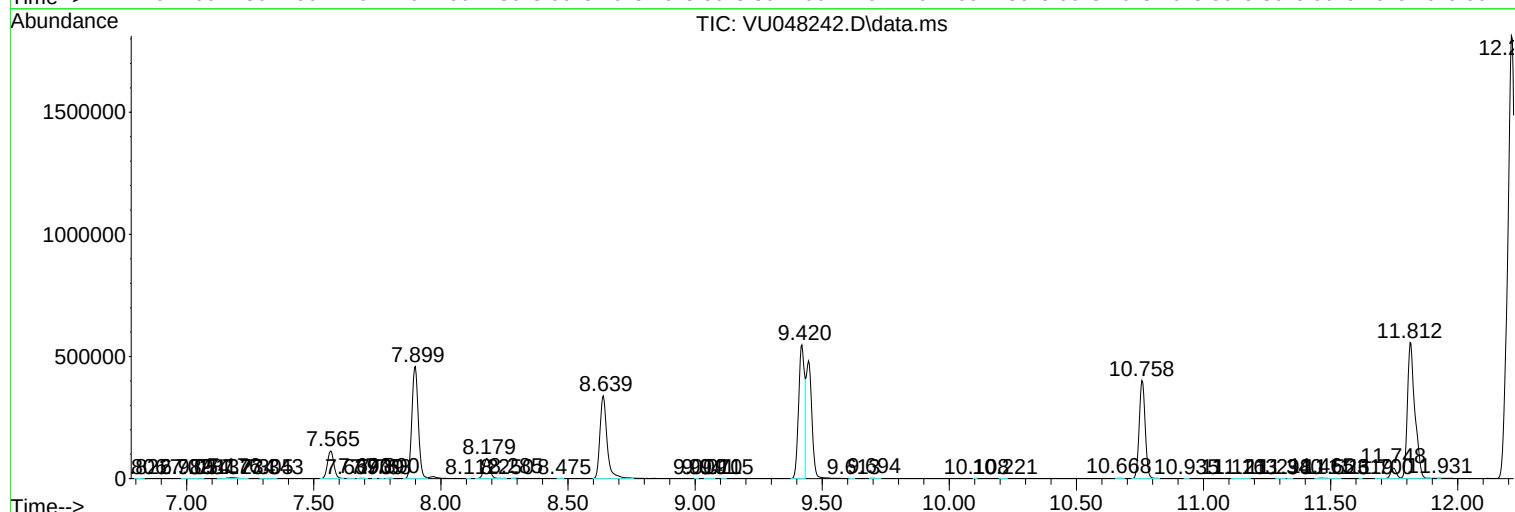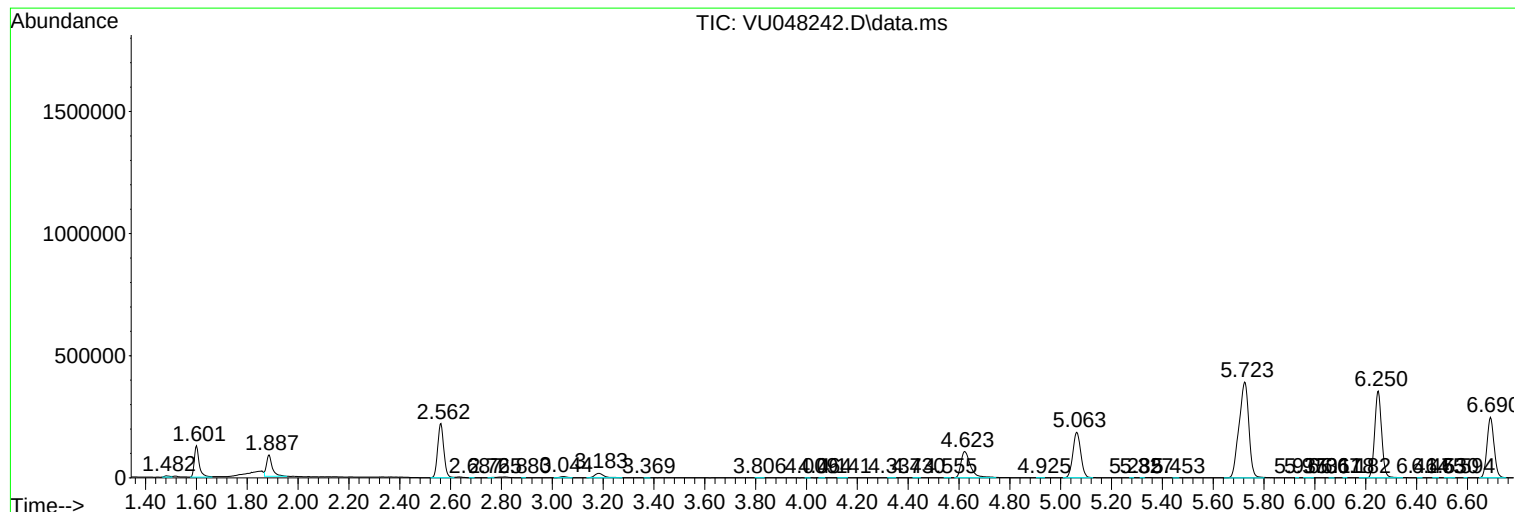

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048242.D
Acq On : 23 Apr 2022 13:40
Operator : SY/MD
Sample : N2486-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048242.D
Acq On : 23 Apr 2022 13:40
Operator : SY/MD
Sample : N2486-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc