

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048245.D
 Acq On : 23 Apr 2022 14:51
 Operator : SY/MD
 Sample : N2488-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	4039	4347	0.19%	0.040%
2	1.601	73	81	100	rBV	141239	176743	7.70%	1.623%
3	1.906	168	176	196	rVB	103974	154097	6.71%	1.415%
4	2.501	359	361	364	rBV2	301	203	0.01%	0.002%
5	2.565	369	381	397	rBV	235126	393449	17.13%	3.613%
6	2.674	411	415	418	rVB	581	366	0.02%	0.003%
7	2.700	421	423	427	rVB2	456	220	0.01%	0.002%
8	2.739	431	435	437	rBV2	325	235	0.01%	0.002%
9	2.797	442	453	456	rBV3	920	1405	0.06%	0.013%
10	2.819	456	460	463	rBV3	589	512	0.02%	0.005%
11	2.967	501	506	507	rBV3	325	239	0.01%	0.002%
12	3.047	520	531	546	rBV2	9273	18568	0.81%	0.170%
13	3.105	546	549	552	rVB2	402	305	0.01%	0.003%
14	3.192	560	576	595	rBV2	9277	28723	1.25%	0.264%
15	3.379	632	634	639	rVB2	425	328	0.01%	0.003%
16	3.469	657	662	668	rBV2	252	264	0.01%	0.002%
17	3.710	735	737	740	rVB	401	218	0.01%	0.002%
18	3.935	802	807	814	rVB3	317	365	0.02%	0.003%
19	4.218	889	895	899	rBV3	243	324	0.01%	0.003%
20	4.491	972	980	983	rBV2	230	340	0.01%	0.003%
21	4.565	997	1003	1005	rVV2	292	307	0.01%	0.003%
22	4.626	1009	1022	1063	rVV	124681	329280	14.34%	3.024%
23	5.067	1141	1159	1181	rBV	203438	459070	19.99%	4.215%
24	5.231	1206	1210	1214	rBV2	261	223	0.01%	0.002%
25	5.298	1223	1231	1238	rVB3	625	960	0.04%	0.009%
26	5.346	1243	1246	1249	rVB3	336	208	0.01%	0.002%
27	5.369	1249	1253	1259	rBV2	217	236	0.01%	0.002%
28	5.517	1292	1299	1301	rBV3	419	461	0.02%	0.004%
29	5.726	1342	1364	1373	rBV2	427888	1145662	49.89%	10.520%
30	6.105	1480	1482	1485	rVV3	333	265	0.01%	0.002%
31	6.121	1485	1487	1493	rVB2	454	295	0.01%	0.003%
32	6.150	1493	1496	1501	rBV	256	203	0.01%	0.002%
33	6.250	1511	1527	1561	rBV	372975	712844	31.04%	6.545%
34	6.523	1608	1612	1613	rBV3	660	392	0.02%	0.004%
35	6.533	1613	1615	1618	rVB4	489	270	0.01%	0.002%
36	6.690	1650	1664	1692	rVB	260018	514705	22.42%	4.726%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048245.D
 Acq On : 23 Apr 2022 14:51
 Operator : SY/MD
 Sample : N2488-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.803	1692	1699	1701	rBV4	718	747	0.03%	0.007%
38	7.047	1771	1775	1782	rBV2	491	509	0.02%	0.005%
39	7.186	1808	1818	1832	rVV3	2639	5274	0.23%	0.048%
40	7.340	1863	1866	1871	rBV2	200	234	0.01%	0.002%
41	7.565	1924	1936	1955	rBV	121782	214468	9.34%	1.969%
42	7.690	1971	1975	1979	rVV4	729	790	0.03%	0.007%
43	7.793	1998	2007	2009	rBV4	479	670	0.03%	0.006%
44	7.899	2025	2040	2055	rBV	498311	863028	37.59%	7.924%
45	8.179	2112	2127	2142	rBV	84346	142005	6.18%	1.304%
46	8.465	2213	2216	2218	rBV2	294	225	0.01%	0.002%
47	8.536	2234	2238	2241	rBV2	281	206	0.01%	0.002%
48	8.555	2241	2244	2251	rVB2	383	438	0.02%	0.004%
49	8.636	2256	2269	2300	rBV	374750	678337	29.54%	6.229%
50	9.025	2386	2390	2395	rVB2	363	315	0.01%	0.003%
51	9.160	2429	2432	2435	rBV	351	292	0.01%	0.003%
52	9.317	2478	2481	2486	rBV2	342	302	0.01%	0.003%
53	9.366	2493	2496	2499	rBV	413	323	0.01%	0.003%
54	9.420	2499	2513	2517	rBV	544502	913830	39.80%	8.391%
55	9.607	2567	2571	2574	rBV4	522	448	0.02%	0.004%
56	9.697	2597	2599	2605	rVB2	1108	961	0.04%	0.009%
57	9.732	2605	2610	2612	rBV3	355	312	0.01%	0.003%
58	9.906	2660	2664	2669	rVB2	245	233	0.01%	0.002%
59	10.028	2699	2702	2704	rBV	269	213	0.01%	0.002%
60	10.156	2739	2742	2748	rVB2	312	238	0.01%	0.002%
61	10.279	2774	2780	2783	rBV2	188	212	0.01%	0.002%
62	10.330	2793	2796	2800	rBV2	200	230	0.01%	0.002%
63	10.565	2864	2869	2872	rBV2	236	260	0.01%	0.002%
64	10.594	2872	2878	2883	rVB	259	290	0.01%	0.003%
65	10.674	2896	2903	2907	rBV3	792	984	0.04%	0.009%
66	10.758	2912	2929	2949	rBV	404108	653832	28.47%	6.004%
67	10.870	2961	2964	2966	rVV	302	235	0.01%	0.002%
68	10.893	2966	2971	2979	rVB4	1195	1543	0.07%	0.014%
69	11.118	3038	3041	3047	rVB3	542	553	0.02%	0.005%
70	11.150	3047	3051	3053	rBV2	319	281	0.01%	0.003%
71	11.182	3059	3061	3065	rVB3	315	192	0.01%	0.002%
72	11.462	3141	3148	3149	rBV3	1082	1020	0.04%	0.009%
73	11.700	3218	3222	3225	rVB3	742	557	0.02%	0.005%
74	11.745	3225	3236	3246	rBV	111511	173733	7.57%	1.595%
75	11.816	3246	3258	3260	rBV	543740	758981	33.05%	6.969%
76	12.021	3318	3322	3327	rVB4	289	288	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048245.D
 Acq On : 23 Apr 2022 14:51
 Operator : SY/MD
 Sample : N2488-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	12.086	3335	3342	3348	rBV5	706	1034	0.05%	0.009%
78	12.211	3362	3381	3404	rBV2	1059619	2296178	100.00%	21.084%
79	12.327	3415	3417	3425	rVB4	721	686	0.03%	0.006%
80	12.365	3425	3429	3430	rBV2	364	261	0.01%	0.002%
81	12.427	3446	3448	3453	rBV2	313	218	0.01%	0.002%
82	12.497	3467	3470	3473	rBV3	332	222	0.01%	0.002%
83	12.526	3476	3479	3485	rVB2	459	424	0.02%	0.004%
84	12.558	3485	3489	3491	rBV2	340	216	0.01%	0.002%
85	12.700	3530	3533	3535	rBV3	307	185	0.01%	0.002%
86	12.742	3540	3546	3548	rBV	461	554	0.02%	0.005%
87	12.758	3549	3551	3558	rVB3	589	632	0.03%	0.006%
88	12.854	3577	3581	3585	rBV	293	304	0.01%	0.003%
89	12.890	3588	3592	3595	rBV2	414	371	0.02%	0.003%
90	12.986	3615	3622	3628	rBV6	537	730	0.03%	0.007%
91	13.057	3637	3644	3647	rBV4	437	655	0.03%	0.006%
92	13.124	3662	3665	3669	rVB	304	223	0.01%	0.002%
93	13.147	3670	3672	3680	rVB2	305	262	0.01%	0.002%
94	13.221	3687	3695	3701	rBV5	1838	2517	0.11%	0.023%
95	13.349	3732	3735	3737	rBV2	291	222	0.01%	0.002%
96	13.568	3800	3803	3806	rBV2	508	391	0.02%	0.004%
97	13.841	3877	3888	3904	rBV	97863	152608	6.65%	1.401%
98	14.092	3962	3966	3974	rBV3	1740	1780	0.08%	0.016%
99	14.214	4001	4004	4008	rBV2	485	403	0.02%	0.004%
100	14.330	4030	4040	4056	rBV	41543	65371	2.85%	0.600%




Sum of corrected areas: 10890668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048245.D
Acq On : 23 Apr 2022 14:51
Operator : SY/MD
Sample : N2488-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

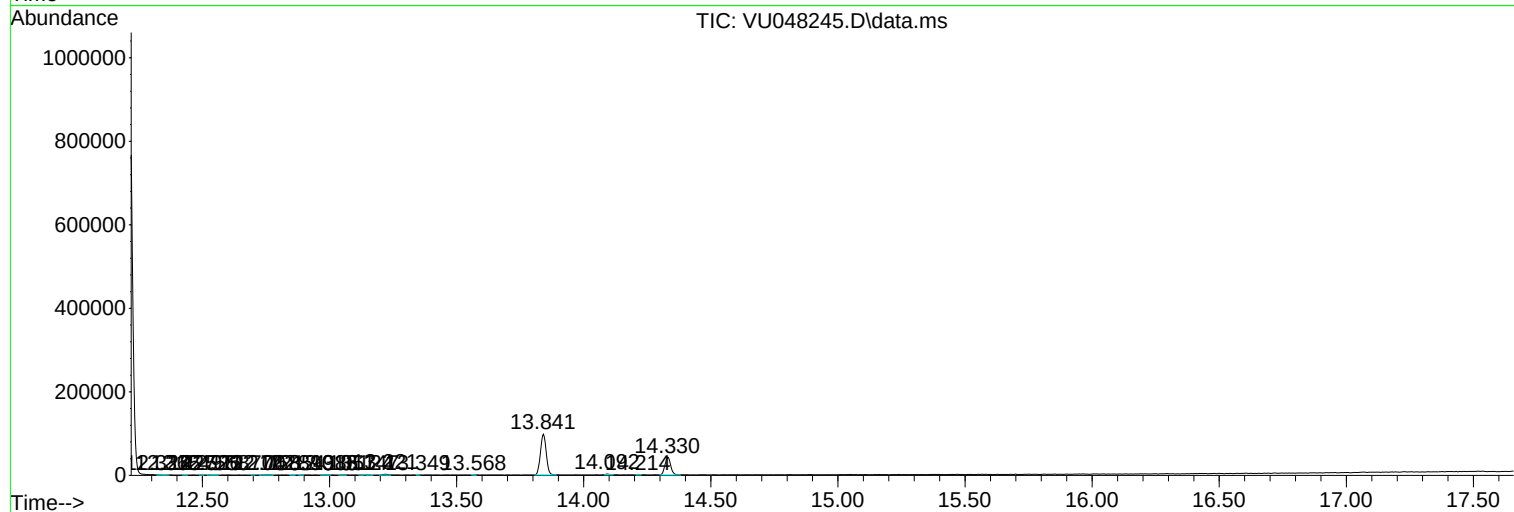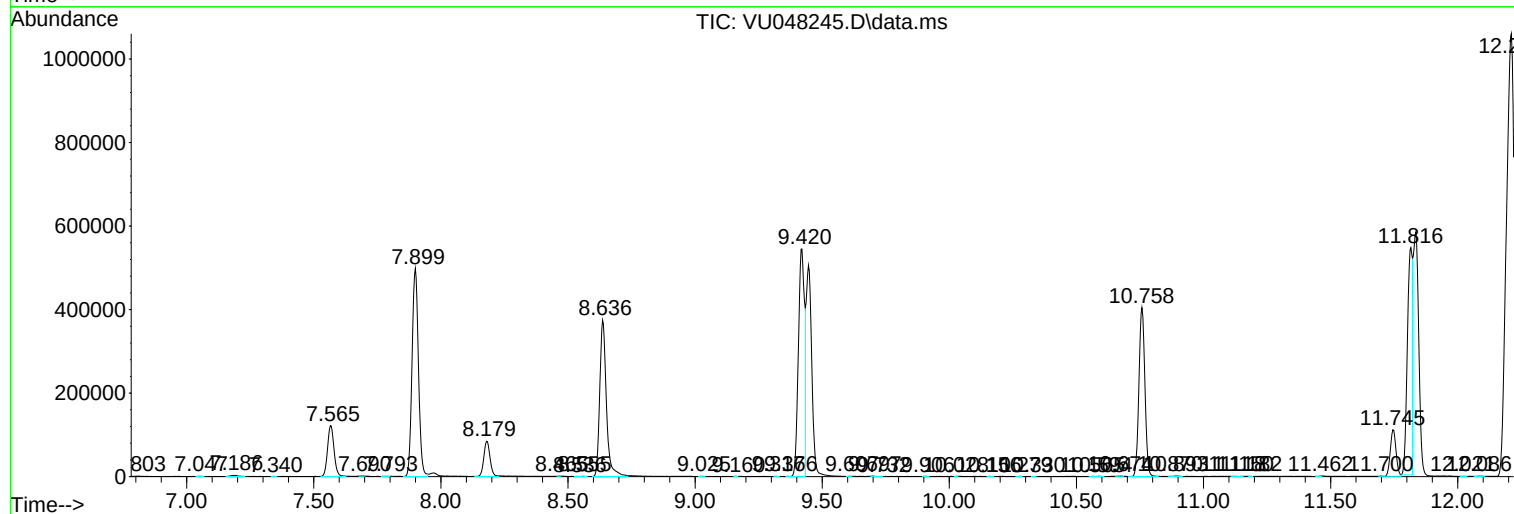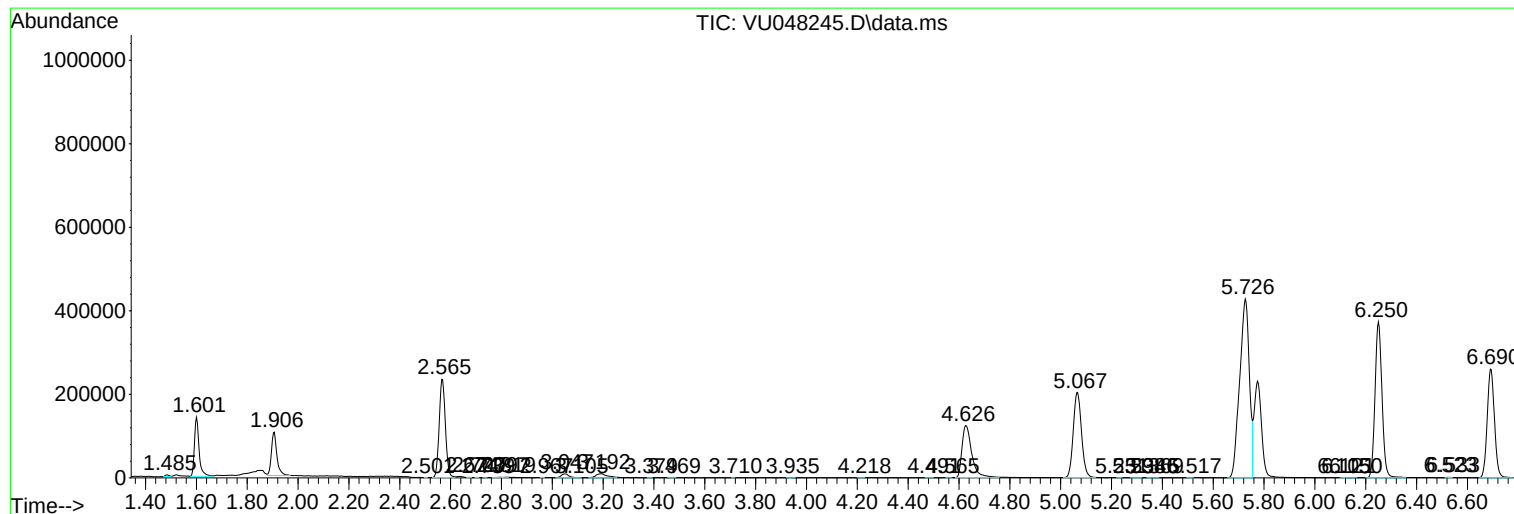

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048245.D
Acq On : 23 Apr 2022 14:51
Operator : SY/MD
Sample : N2488-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048245.D
Acq On : 23 Apr 2022 14:51
Operator : SY/MD
Sample : N2488-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------