

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048247.D
 Acq On : 23 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2488-03DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	4270	4748	0.45%	0.055%
2	1.523	51	57	64	rBV3	4685	6818	0.65%	0.079%
3	1.601	73	81	101	rBV	126686	161135	15.25%	1.877%
4	1.900	168	174	197	rVB	93999	146812	13.89%	1.710%
5	2.565	368	381	398	rBV	214948	360125	34.08%	4.195%
6	2.633	400	402	414	rVV4	2595	4146	0.39%	0.048%
7	2.684	415	418	424	rVB3	475	380	0.04%	0.004%
8	2.742	433	436	439	rBV3	329	306	0.03%	0.004%
9	2.777	441	447	449	rBV5	995	1085	0.10%	0.013%
10	2.954	498	502	504	rBV	346	221	0.02%	0.003%
11	3.048	521	531	544	rVB4	3488	6263	0.59%	0.073%
12	3.125	551	555	558	rBV3	242	172	0.02%	0.002%
13	3.186	560	574	607	rVV	11069	36448	3.45%	0.425%
14	3.298	607	609	613	rVB	224	154	0.01%	0.002%
15	3.446	651	655	661	rBV3	180	179	0.02%	0.002%
16	3.601	701	703	710	rVB3	569	560	0.05%	0.007%
17	3.658	718	721	725	rVB2	242	178	0.02%	0.002%
18	4.086	850	854	861	rBV2	185	227	0.02%	0.003%
19	4.292	913	918	920	rBV2	181	163	0.02%	0.002%
20	4.523	986	990	993	rBV2	206	196	0.02%	0.002%
21	4.556	997	1000	1002	rBV	477	332	0.03%	0.004%
22	4.629	1009	1023	1051	rBV	121099	320569	30.33%	3.734%
23	5.064	1138	1158	1175	rBV2	190120	418505	39.60%	4.875%
24	5.215	1201	1205	1208	rBV2	348	234	0.02%	0.003%
25	5.276	1219	1224	1227	rBV2	502	423	0.04%	0.005%
26	5.726	1343	1364	1372	rBV2	394265	1056812	100.00%	12.311%
27	5.912	1420	1422	1426	rVB2	513	256	0.02%	0.003%
28	5.977	1438	1442	1448	rBV5	684	634	0.06%	0.007%
29	6.047	1460	1464	1466	rVB3	370	237	0.02%	0.003%
30	6.115	1483	1485	1489	rVB2	269	187	0.02%	0.002%
31	6.250	1512	1527	1557	rBV	357342	677031	64.06%	7.887%
32	6.379	1565	1567	1570	rBV	526	381	0.04%	0.004%
33	6.481	1597	1599	1603	rVB	329	169	0.02%	0.002%
34	6.526	1605	1613	1621	rBV6	893	1540	0.15%	0.018%
35	6.597	1632	1635	1637	rBV	375	234	0.02%	0.003%
36	6.690	1649	1664	1685	rBV	242639	480359	45.45%	5.596%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048247.D
 Acq On : 23 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2488-03DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.051	1772	1776	1778	rBV2	346	271	0.03%	0.003%
38	7.182	1805	1817	1830	rBV5	3531	7386	0.70%	0.086%
39	7.411	1884	1888	1892	rVB	222	193	0.02%	0.002%
40	7.443	1892	1898	1902	rBV2	178	203	0.02%	0.002%
41	7.472	1902	1907	1914	rBV2	220	259	0.02%	0.003%
42	7.565	1923	1936	1957	rBV	111395	196797	18.62%	2.293%
43	7.671	1965	1969	1970	rBV2	350	235	0.02%	0.003%
44	7.690	1971	1975	1984	rVB5	1305	1515	0.14%	0.018%
45	7.797	2002	2008	2013	rBV3	1205	1456	0.14%	0.017%
46	7.819	2013	2015	2019	rVB2	575	331	0.03%	0.004%
47	7.899	2026	2040	2055	rBV	443827	764707	72.36%	8.908%
48	8.179	2115	2127	2141	rBV	74786	128162	12.13%	1.493%
49	8.446	2207	2210	2212	rBV2	280	180	0.02%	0.002%
50	8.472	2212	2218	2221	rBV3	416	424	0.04%	0.005%
51	8.559	2241	2245	2248	rBV2	220	168	0.02%	0.002%
52	8.639	2257	2270	2294	rBV	357297	661109	62.56%	7.702%
53	8.809	2321	2323	2327	rVB4	698	438	0.04%	0.005%
54	8.912	2352	2355	2363	rVB5	812	874	0.08%	0.010%
55	9.015	2383	2387	2389	rBV	263	221	0.02%	0.003%
56	9.102	2411	2414	2422	rVB2	204	226	0.02%	0.003%
57	9.160	2430	2432	2440	rVB3	371	325	0.03%	0.004%
58	9.420	2499	2513	2516	rBV	526963	800199	75.72%	9.322%
59	9.607	2569	2571	2574	rBV2	269	154	0.01%	0.002%
60	9.649	2580	2584	2590	rVB3	475	432	0.04%	0.005%
61	9.697	2592	2599	2608	rVB3	725	1052	0.10%	0.012%
62	9.758	2613	2618	2621	rBV2	191	187	0.02%	0.002%
63	9.800	2628	2631	2635	rBV2	287	233	0.02%	0.003%
64	9.870	2650	2653	2656	rBV	294	208	0.02%	0.002%
65	10.025	2697	2701	2704	rVB	223	194	0.02%	0.002%
66	10.272	2775	2778	2782	rVB2	250	179	0.02%	0.002%
67	10.468	2833	2839	2840	rBV	429	378	0.04%	0.004%
68	10.571	2869	2871	2874	rBV2	328	208	0.02%	0.002%
69	10.668	2895	2901	2910	rVB3	1261	1487	0.14%	0.017%
70	10.758	2916	2929	2948	rBV	390425	628059	59.43%	7.317%
71	10.851	2955	2958	2959	rBV	328	179	0.02%	0.002%
72	10.890	2968	2970	2972	rBV	381	220	0.02%	0.003%
73	11.121	3038	3042	3047	rBV3	599	529	0.05%	0.006%
74	11.192	3060	3064	3065	rBV	251	166	0.02%	0.002%
75	11.385	3120	3124	3127	rBV3	238	182	0.02%	0.002%
76	11.407	3128	3131	3135	rVB3	404	277	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048247.D
 Acq On : 23 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2488-03DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.439	3135	3141	3142	rBV2	404	311	0.03%	0.004%
78	11.520	3162	3166	3171	rVB2	316	338	0.03%	0.004%
79	11.636	3199	3202	3206	rBV3	395	283	0.03%	0.003%
80	11.693	3217	3220	3222	rBV	280	211	0.02%	0.002%
81	11.748	3227	3237	3245	rVV	15372	22673	2.15%	0.264%
82	11.812	3245	3257	3283	rVB2	467947	866036	81.95%	10.089%
83	11.976	3306	3308	3312	rVB2	884	469	0.04%	0.005%
84	11.999	3312	3315	3318	rBV	325	283	0.03%	0.003%
85	12.144	3356	3360	3363	rBV	321	294	0.03%	0.003%
86	12.195	3363	3376	3404	rBV2	426319	777823	73.60%	9.061%
87	12.340	3418	3421	3426	rVB2	437	292	0.03%	0.003%
88	12.433	3447	3450	3453	rBV2	410	360	0.03%	0.004%
89	12.536	3480	3482	3489	rVB2	363	357	0.03%	0.004%
90	12.568	3489	3492	3495	rBV	321	259	0.02%	0.003%
91	12.610	3502	3505	3507	rBV2	245	161	0.02%	0.002%
92	12.726	3538	3541	3543	rBV2	308	202	0.02%	0.002%
93	12.771	3547	3555	3557	rBV2	639	854	0.08%	0.010%
94	12.857	3578	3582	3584	rBV	346	266	0.03%	0.003%
95	12.964	3612	3615	3617	rBV2	281	202	0.02%	0.002%
96	13.327	3722	3728	3733	rBV3	381	617	0.06%	0.007%
97	13.845	3880	3889	3899	rBV3	10321	15817	1.50%	0.184%
98	14.102	3961	3969	3975	rBV4	694	1253	0.12%	0.015%
99	14.333	4033	4041	4051	rBV3	3990	6244	0.59%	0.073%
100	15.356	4356	4359	4361	rBV2	500	306	0.03%	0.004%




Sum of corrected areas: 8584133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048247.D
Acq On : 23 Apr 2022 15:38
Operator : SY/MD
Sample : N2488-03DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

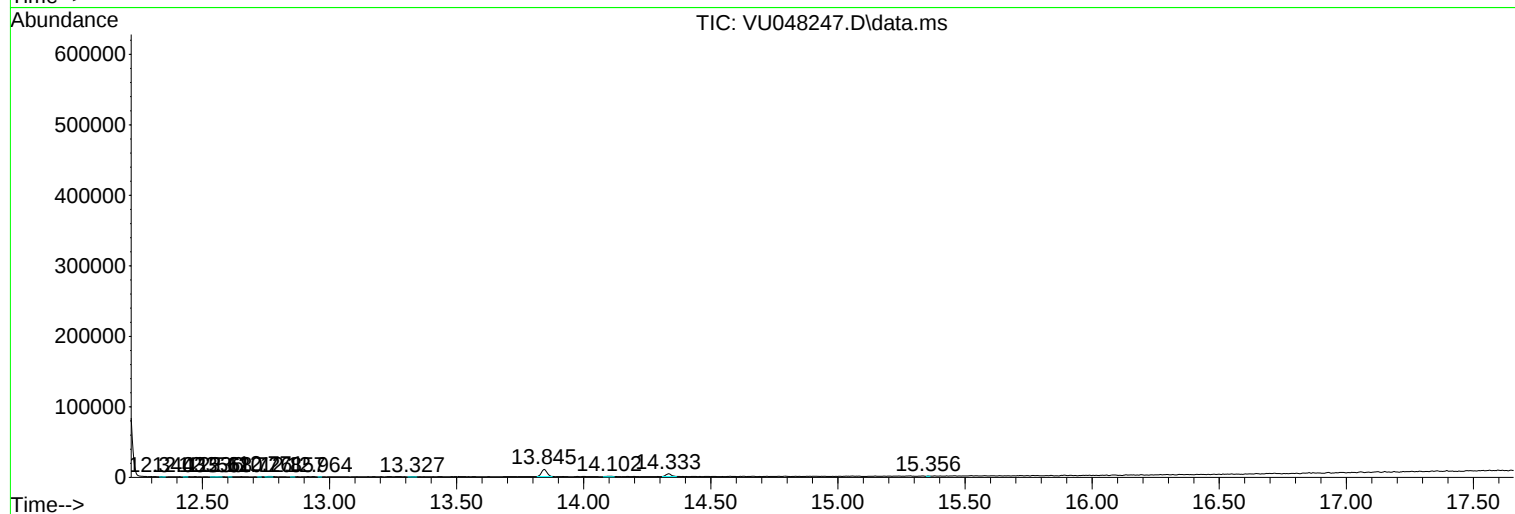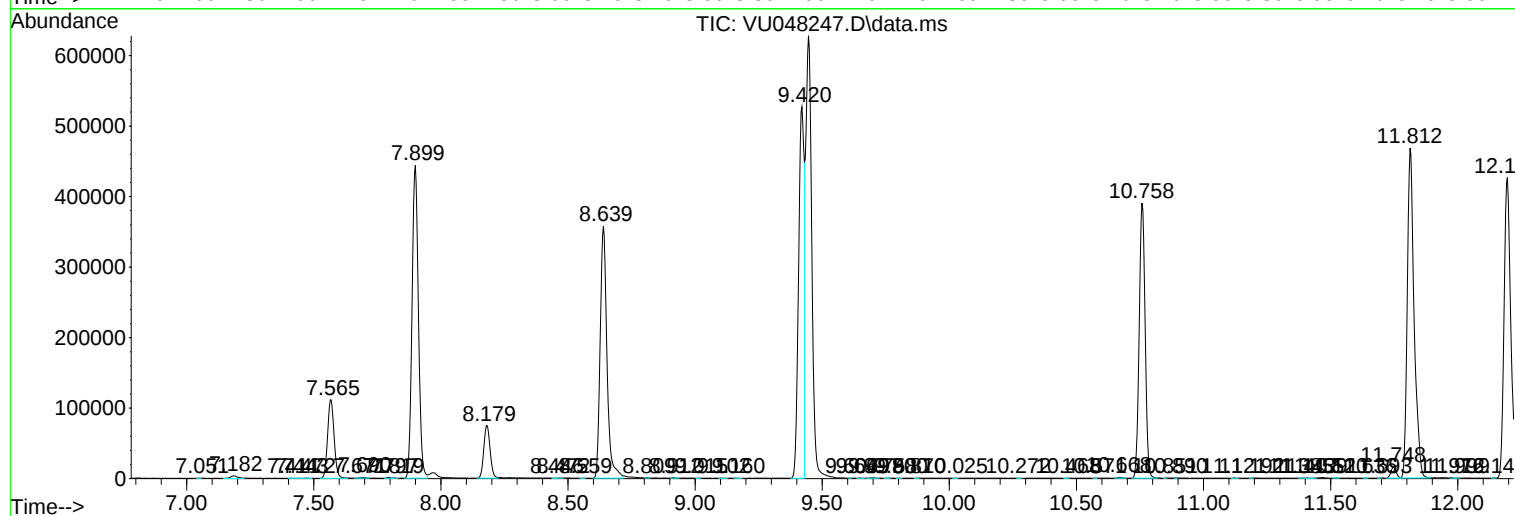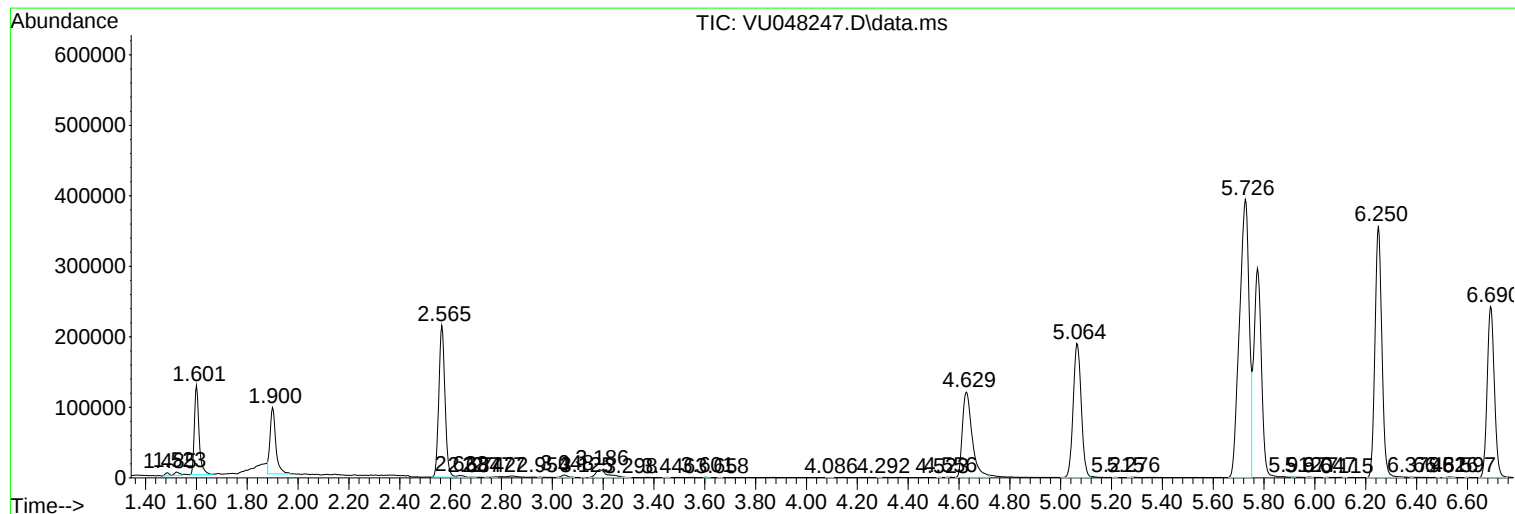

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048247.D
Acq On : 23 Apr 2022 15:38
Operator : SY/MD
Sample : N2488-03DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048247.D
Acq On : 23 Apr 2022 15:38
Operator : SY/MD
Sample : N2488-03DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------