

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048249.D
 Acq On : 23 Apr 2022 16:26
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	3360	3850	0.35%	0.044%
2	1.520	52	56	64	rVV2	4051	5084	0.46%	0.059%
3	1.601	73	81	101	rBV	135683	171357	15.55%	1.972%
4	1.900	166	174	191	rVB	98641	144936	13.15%	1.668%
5	2.565	368	381	395	rBV	229741	380912	34.57%	4.385%
6	2.794	447	452	454	rBV2	411	428	0.04%	0.005%
7	2.916	488	490	495	rVB2	201	144	0.01%	0.002%
8	2.958	501	503	506	rVV2	391	203	0.02%	0.002%
9	3.009	516	519	523	rVB2	249	202	0.02%	0.002%
10	3.051	525	532	541	rVB3	877	1167	0.11%	0.013%
11	3.186	559	574	588	rBV2	24703	67343	6.11%	0.775%
12	3.504	669	673	682	rVB3	318	422	0.04%	0.005%
13	3.552	682	688	690	rBV3	276	231	0.02%	0.003%
14	3.569	690	693	696	rBV2	278	142	0.01%	0.002%
15	3.864	782	785	790	rVB2	310	214	0.02%	0.002%
16	3.916	798	801	803	rBV	231	172	0.02%	0.002%
17	4.015	827	832	835	rBV	238	266	0.02%	0.003%
18	4.118	860	864	866	rBV2	243	207	0.02%	0.002%
19	4.263	906	909	916	rBV2	169	202	0.02%	0.002%
20	4.298	917	920	925	rVB	224	156	0.01%	0.002%
21	4.443	960	965	969	rBV2	204	240	0.02%	0.003%
22	4.469	969	973	975	rBV2	248	182	0.02%	0.002%
23	4.626	1007	1022	1065	rBV	123118	333356	30.25%	3.837%
24	5.064	1142	1158	1183	rBV	193928	428185	38.85%	4.929%
25	5.167	1188	1190	1194	rVB4	423	269	0.02%	0.003%
26	5.215	1200	1205	1208	rBV2	164	153	0.01%	0.002%
27	5.260	1213	1219	1223	rBV2	192	213	0.02%	0.002%
28	5.292	1223	1229	1233	rBV2	532	805	0.07%	0.009%
29	5.334	1239	1242	1244	rBV3	365	239	0.02%	0.003%
30	5.501	1286	1294	1296	rBV	314	381	0.03%	0.004%
31	5.639	1332	1337	1342	rBV	196	231	0.02%	0.003%
32	5.726	1342	1364	1394	rBV2	408101	1102016	100.00%	12.685%
33	5.967	1435	1439	1445	rVV4	753	1017	0.09%	0.012%
34	6.112	1482	1484	1485	rBV	251	144	0.01%	0.002%
35	6.157	1494	1498	1503	rBV2	516	440	0.04%	0.005%
36	6.250	1511	1527	1552	rBV	348801	665635	60.40%	7.662%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048249.D
 Acq On : 23 Apr 2022 16:26
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.359	1558	1561	1565	rVB2	393	242	0.02%	0.003%
38	6.440	1584	1586	1591	rVB3	370	302	0.03%	0.003%
39	6.485	1598	1600	1602	rBV	208	141	0.01%	0.002%
40	6.533	1608	1615	1620	rBV4	797	1048	0.10%	0.012%
41	6.691	1647	1664	1686	rVV	257381	500066	45.38%	5.756%
42	6.771	1686	1689	1693	rVV5	716	509	0.05%	0.006%
43	6.803	1697	1699	1703	rVB4	580	348	0.03%	0.004%
44	6.851	1710	1714	1717	rBV2	168	165	0.01%	0.002%
45	6.884	1720	1724	1725	rBV2	850	467	0.04%	0.005%
46	6.922	1734	1736	1740	rVB	238	138	0.01%	0.002%
47	7.035	1768	1771	1772	rBV	341	171	0.02%	0.002%
48	7.121	1796	1798	1802	rBV2	154	150	0.01%	0.002%
49	7.141	1802	1804	1806	rVV	261	143	0.01%	0.002%
50	7.186	1806	1818	1833	rVV6	3058	6560	0.60%	0.076%
51	7.253	1834	1839	1843	rVV2	259	258	0.02%	0.003%
52	7.356	1866	1871	1874	rBV	320	223	0.02%	0.003%
53	7.565	1923	1936	1957	rBV	115372	203906	18.50%	2.347%
54	7.694	1967	1976	1983	rBV4	1297	2004	0.18%	0.023%
55	7.900	2025	2040	2056	rBV	476736	823633	74.74%	9.481%
56	8.179	2116	2127	2142	rBV	79159	132648	12.04%	1.527%
57	8.475	2210	2219	2232	rVB4	2991	5225	0.47%	0.060%
58	8.546	2237	2241	2244	rBV3	224	207	0.02%	0.002%
59	8.639	2257	2270	2308	rBV	355070	664976	60.34%	7.655%
60	8.790	2308	2317	2330	rVV6	7292	13811	1.25%	0.159%
61	8.864	2337	2340	2343	rBV3	405	244	0.02%	0.003%
62	8.977	2370	2375	2381	rBV3	377	432	0.04%	0.005%
63	9.237	2449	2456	2465	rBV2	387	531	0.05%	0.006%
64	9.417	2498	2512	2534	rBV	509946	859771	78.02%	9.897%
65	9.572	2556	2560	2565	rVB	482	373	0.03%	0.004%
66	9.597	2565	2568	2571	rVB2	366	247	0.02%	0.003%
67	9.620	2571	2575	2577	rBV2	210	192	0.02%	0.002%
68	9.690	2594	2597	2606	rVB	793	913	0.08%	0.011%
69	9.938	2670	2674	2676	rBV	243	148	0.01%	0.002%
70	10.108	2725	2727	2731	rVB3	396	234	0.02%	0.003%
71	10.170	2743	2746	2749	rBV	245	166	0.02%	0.002%
72	10.244	2766	2769	2772	rBV	185	143	0.01%	0.002%
73	10.350	2794	2802	2810	rBV6	2598	4274	0.39%	0.049%
74	10.481	2840	2843	2846	rBV2	291	234	0.02%	0.003%
75	10.671	2896	2902	2907	rBV3	1075	1005	0.09%	0.012%
76	10.758	2915	2929	2949	rBV	403717	645188	58.55%	7.427%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048249.D
 Acq On : 23 Apr 2022 16:26
 Operator : SY/MD
 Sample : N2488-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.890	2961	2970	2981	rVB3	4910	7673	0.70%	0.088%
78	10.967	2986	2994	2995	rBV2	290	366	0.03%	0.004%
79	11.192	3061	3064	3069	rBV2	311	292	0.03%	0.003%
80	11.350	3108	3113	3115	rBV2	271	301	0.03%	0.003%
81	11.436	3137	3140	3142	rBV2	485	236	0.02%	0.003%
82	11.478	3148	3153	3162	rVB5	1362	2413	0.22%	0.028%
83	11.536	3168	3171	3176	rBV2	292	252	0.02%	0.003%
84	11.697	3212	3221	3231	rBV4	2972	4336	0.39%	0.050%
85	11.748	3231	3237	3244	rBV3	1213	1603	0.15%	0.018%
86	11.813	3244	3257	3281	rBV	457395	737740	66.94%	8.492%
87	12.067	3328	3336	3345	rBV7	2504	4354	0.40%	0.050%
88	12.141	3356	3359	3361	rVB2	415	213	0.02%	0.002%
89	12.195	3363	3376	3394	rVV	433046	728703	66.12%	8.388%
90	12.391	3434	3437	3442	rBV3	334	297	0.03%	0.003%
91	12.446	3451	3454	3458	rBV	437	330	0.03%	0.004%
92	12.497	3467	3470	3473	rBV3	413	362	0.03%	0.004%
93	12.584	3492	3497	3499	rBV2	292	287	0.03%	0.003%
94	12.771	3548	3555	3564	rVB3	1777	3015	0.27%	0.035%
95	12.893	3587	3593	3602	rVB5	2189	2671	0.24%	0.031%
96	13.845	3882	3889	3899	rBV4	3771	5662	0.51%	0.065%
97	14.308	4030	4033	4035	rBV2	475	333	0.03%	0.004%
98	14.333	4035	4041	4052	rVV4	1504	2580	0.23%	0.030%
99	14.391	4056	4059	4061	rBV	320	228	0.02%	0.003%
100	15.353	4355	4358	4361	rBV2	866	537	0.05%	0.006%


Sum of corrected areas: 8687364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048249.D
Acq On : 23 Apr 2022 16:26
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

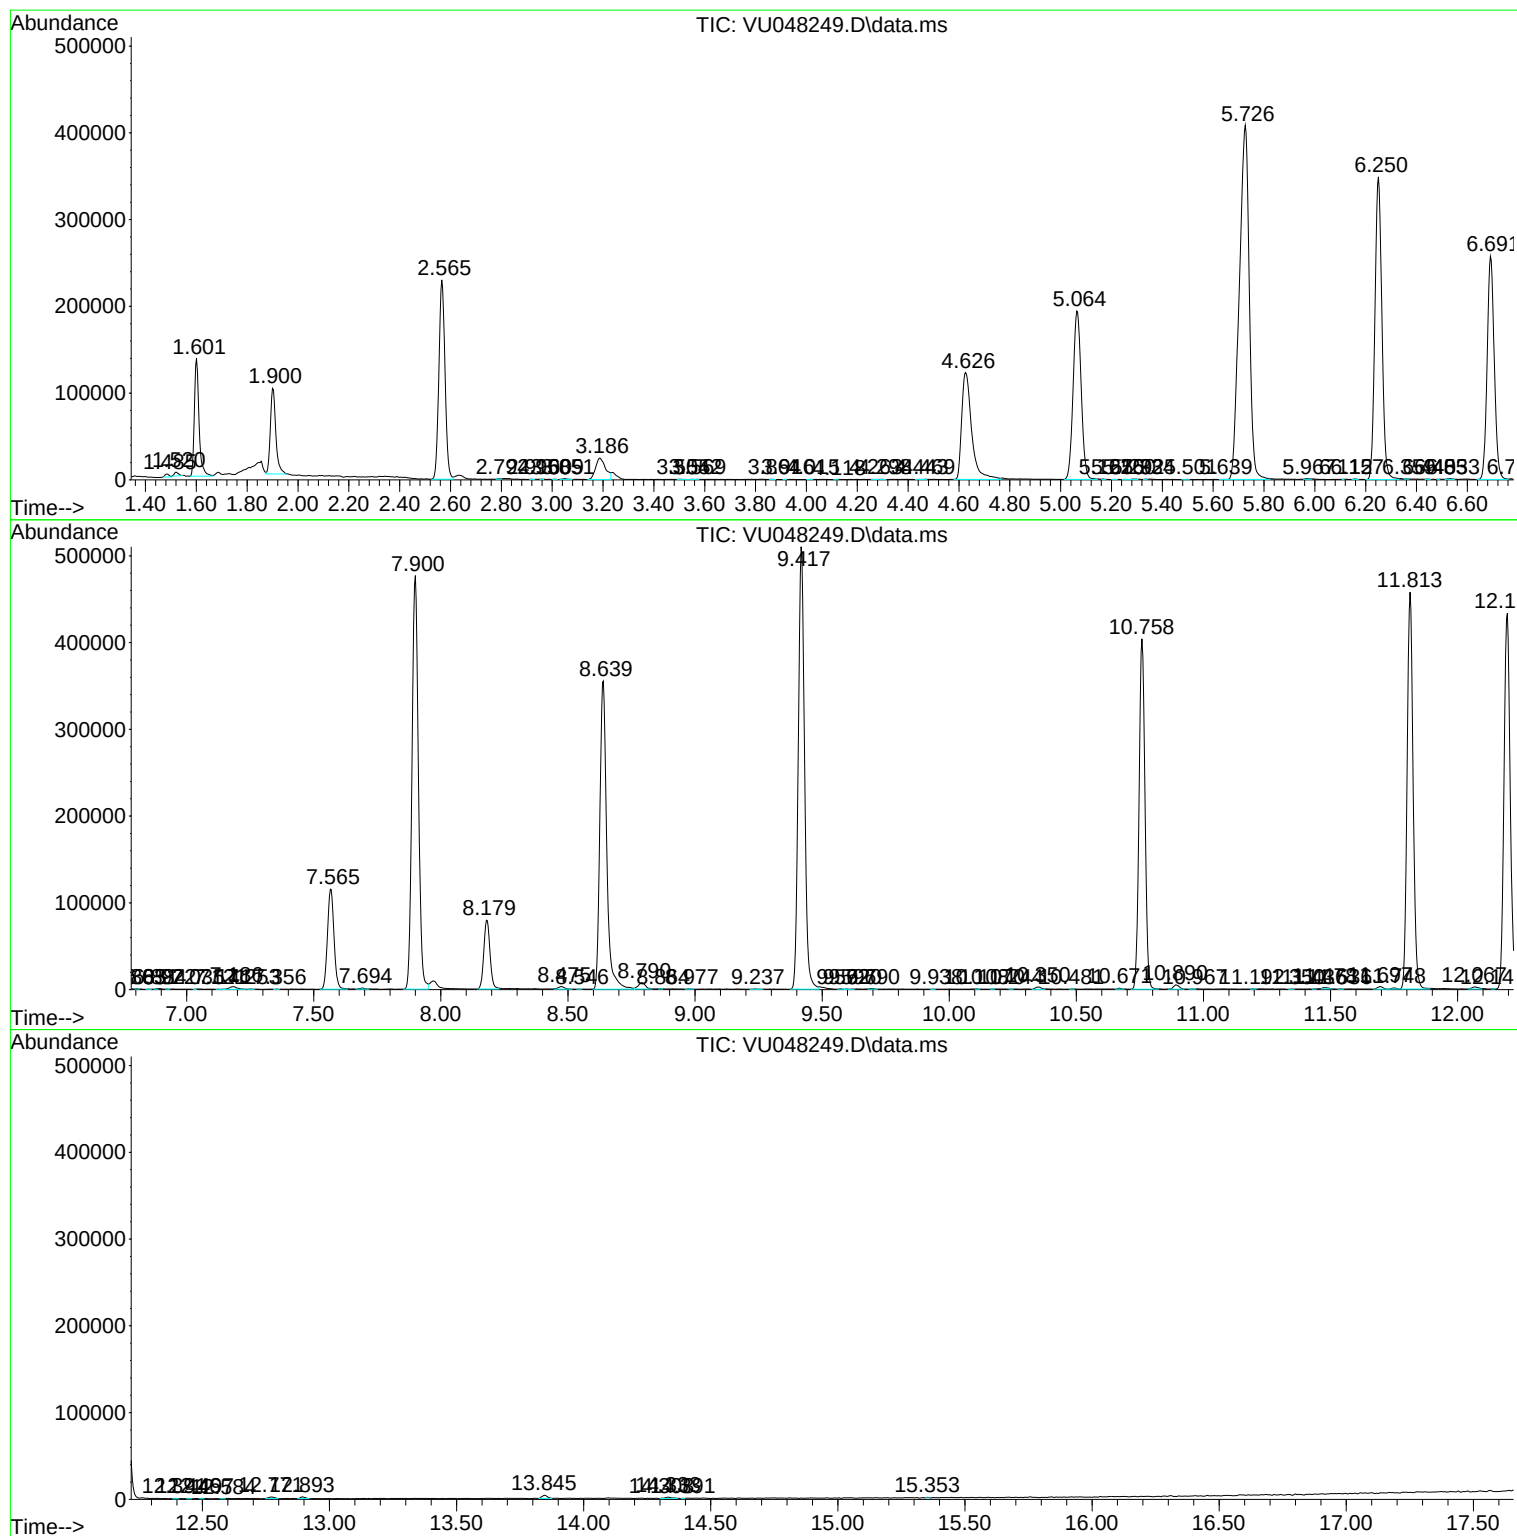

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048249.D
Acq On : 23 Apr 2022 16:26
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048249.D
Acq On : 23 Apr 2022 16:26
Operator : SY/MD
Sample : N2488-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc