

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048250.D
 Acq On : 23 Apr 2022 16:49
 Operator : SY/MD
 Sample : N2488-09DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	51	rBV2	3791	4517	0.43%	0.050%
2	1.520	51	56	68	rVV2	4329	7700	0.73%	0.085%
3	1.601	73	81	100	rVV	125272	158571	14.97%	1.747%
4	1.900	167	174	194	rVB	93653	138403	13.07%	1.525%
5	2.565	368	381	396	rBV	216328	355976	33.62%	3.922%
6	2.691	417	420	424	rVB3	310	237	0.02%	0.003%
7	2.784	447	449	451	rBV	460	225	0.02%	0.002%
8	2.842	464	467	472	rVB4	398	321	0.03%	0.004%
9	2.916	478	490	501	rBV	9496	18747	1.77%	0.207%
10	3.048	520	531	554	rVB	13608	27997	2.64%	0.308%
11	3.186	560	574	586	rBV	15746	39650	3.74%	0.437%
12	3.298	607	609	614	rVB2	343	234	0.02%	0.003%
13	3.443	652	654	660	rBV3	226	184	0.02%	0.002%
14	3.511	672	675	678	rVB2	309	217	0.02%	0.002%
15	3.855	779	782	785	rVB2	371	257	0.02%	0.003%
16	3.877	785	789	792	rBV2	290	331	0.03%	0.004%
17	4.064	842	847	850	rBV2	149	188	0.02%	0.002%
18	4.076	850	851	856	rVB	346	169	0.02%	0.002%
19	4.192	881	887	889	rBV2	226	208	0.02%	0.002%
20	4.575	1001	1006	1007	rBV2	373	299	0.03%	0.003%
21	4.629	1009	1023	1075	rVV	112510	307058	29.00%	3.383%
22	4.986	1129	1134	1138	rBV2	234	231	0.02%	0.003%
23	5.064	1142	1158	1183	rBV	184013	407432	38.47%	4.488%
24	5.227	1204	1209	1212	rBV2	196	187	0.02%	0.002%
25	5.260	1216	1219	1223	rVB2	244	166	0.02%	0.002%
26	5.292	1223	1229	1231	rBV3	389	424	0.04%	0.005%
27	5.366	1249	1252	1255	rVB2	321	224	0.02%	0.002%
28	5.530	1301	1303	1310	rVB2	538	435	0.04%	0.005%
29	5.726	1341	1364	1375	rBV2	380955	1053362	99.47%	11.604%
30	5.867	1407	1408	1413	rVB3	402	174	0.02%	0.002%
31	5.961	1431	1437	1439	rBV3	579	471	0.04%	0.005%
32	6.009	1447	1452	1456	rVB3	460	442	0.04%	0.005%
33	6.038	1456	1461	1465	rBV2	357	302	0.03%	0.003%
34	6.099	1476	1480	1483	rBV2	182	174	0.02%	0.002%
35	6.121	1483	1487	1492	rVV2	385	432	0.04%	0.005%
36	6.147	1492	1495	1498	rVV	343	201	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048250.D
 Acq On : 23 Apr 2022 16:49
 Operator : SY/MD
 Sample : N2488-09DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1559	rBV	359786	680203	64.23%	7.493%
38	6.414	1574	1578	1580	rVB2	267	164	0.02%	0.002%
39	6.530	1609	1614	1616	rBV4	1035	1007	0.10%	0.011%
40	6.600	1631	1636	1638	rBV3	301	251	0.02%	0.003%
41	6.690	1650	1664	1686	rVV	245280	477689	45.11%	5.262%
42	6.787	1691	1694	1697	rVV	403	321	0.03%	0.004%
43	6.806	1697	1700	1706	rVV3	548	707	0.07%	0.008%
44	7.044	1770	1774	1775	rBV3	217	156	0.01%	0.002%
45	7.186	1806	1818	1829	rBV6	2829	5790	0.55%	0.064%
46	7.417	1888	1890	1892	rBV	226	151	0.01%	0.002%
47	7.491	1910	1913	1916	rBV2	252	219	0.02%	0.002%
48	7.568	1924	1937	1954	rVV	106114	188061	17.76%	2.072%
49	7.629	1954	1956	1961	rVB3	641	522	0.05%	0.006%
50	7.687	1969	1974	1975	rBV2	888	693	0.07%	0.008%
51	7.793	1998	2007	2014	rVV3	1160	1865	0.18%	0.021%
52	7.899	2026	2040	2056	rBV	437886	757241	71.51%	8.342%
53	8.118	2102	2108	2111	rBV3	172	204	0.02%	0.002%
54	8.179	2116	2127	2148	rBV	75772	129287	12.21%	1.424%
55	8.340	2175	2177	2184	rBV4	278	220	0.02%	0.002%
56	8.462	2210	2215	2216	rBV	465	351	0.03%	0.004%
57	8.639	2257	2270	2297	rBV	318530	585767	55.32%	6.453%
58	8.912	2351	2355	2358	rBV3	706	622	0.06%	0.007%
59	9.420	2499	2513	2517	rBV	514779	858657	81.09%	9.459%
60	9.636	2574	2580	2581	rBV	286	228	0.02%	0.003%
61	9.645	2581	2583	2587	rVB2	305	176	0.02%	0.002%
62	9.697	2593	2599	2604	rVB2	602	680	0.06%	0.007%
63	9.726	2604	2608	2612	rBV2	207	170	0.02%	0.002%
64	9.886	2655	2658	2661	rVV	232	165	0.02%	0.002%
65	9.906	2661	2664	2667	rVV	241	172	0.02%	0.002%
66	9.980	2685	2687	2692	rVB2	303	281	0.03%	0.003%
67	10.005	2692	2695	2700	rBV2	258	318	0.03%	0.004%
68	10.102	2722	2725	2728	rVB3	286	200	0.02%	0.002%
69	10.221	2759	2762	2764	rBV	274	185	0.02%	0.002%
70	10.234	2764	2766	2771	rVB2	267	164	0.02%	0.002%
71	10.272	2771	2778	2780	rBV2	319	278	0.03%	0.003%
72	10.282	2780	2781	2785	rVB	376	191	0.02%	0.002%
73	10.308	2785	2789	2791	rBV2	286	235	0.02%	0.003%
74	10.677	2899	2904	2908	rVB3	787	773	0.07%	0.009%
75	10.758	2916	2929	2947	rVV	382026	616926	58.26%	6.796%
76	10.890	2963	2970	2980	rVB4	1396	2256	0.21%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048250.D
 Acq On : 23 Apr 2022 16:49
 Operator : SY/MD
 Sample : N2488-09DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.076	3025	3028	3031	rBV2	213	153	0.01%	0.002%
78	11.240	3076	3079	3083	rVB	222	209	0.02%	0.002%
79	11.266	3083	3087	3091	rBV2	224	268	0.03%	0.003%
80	11.439	3137	3141	3143	rBV	281	237	0.02%	0.003%
81	11.465	3143	3149	3150	rBV3	363	364	0.03%	0.004%
82	11.690	3217	3219	3223	rVB2	374	307	0.03%	0.003%
83	11.748	3226	3237	3246	rVV2	24783	38308	3.62%	0.422%
84	11.812	3246	3257	3280	rVB3	471363	1058958	100.00%	11.666%
85	11.922	3286	3291	3293	rBV3	457	363	0.03%	0.004%
86	11.954	3298	3301	3302	rBV2	460	249	0.02%	0.003%
87	12.028	3322	3324	3326	rBV	311	187	0.02%	0.002%
88	12.198	3362	3377	3399	rBV2	469385	1052527	99.39%	11.595%
89	12.427	3446	3448	3450	rBV	269	160	0.02%	0.002%
90	12.468	3459	3461	3466	rVB3	404	254	0.02%	0.003%
91	12.526	3476	3479	3481	rBV2	242	192	0.02%	0.002%
92	12.587	3495	3498	3501	rBV2	384	263	0.02%	0.003%
93	12.636	3509	3513	3515	rBV2	518	415	0.04%	0.005%
94	12.848	3576	3579	3584	rBV2	352	415	0.04%	0.005%
95	13.111	3657	3661	3662	rBV	397	256	0.02%	0.003%
96	13.160	3673	3676	3677	rBV2	420	258	0.02%	0.003%
97	13.356	3734	3737	3742	rBV2	436	482	0.05%	0.005%
98	13.841	3878	3888	3904	rBV2	42432	66108	6.24%	0.728%
99	14.333	4032	4041	4052	rVB3	10386	16458	1.55%	0.181%
100	14.578	4113	4117	4118	rBV	504	406	0.04%	0.004%




Sum of corrected areas: 9077489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048250.D
Acq On : 23 Apr 2022 16:49
Operator : SY/MD
Sample : N2488-09DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

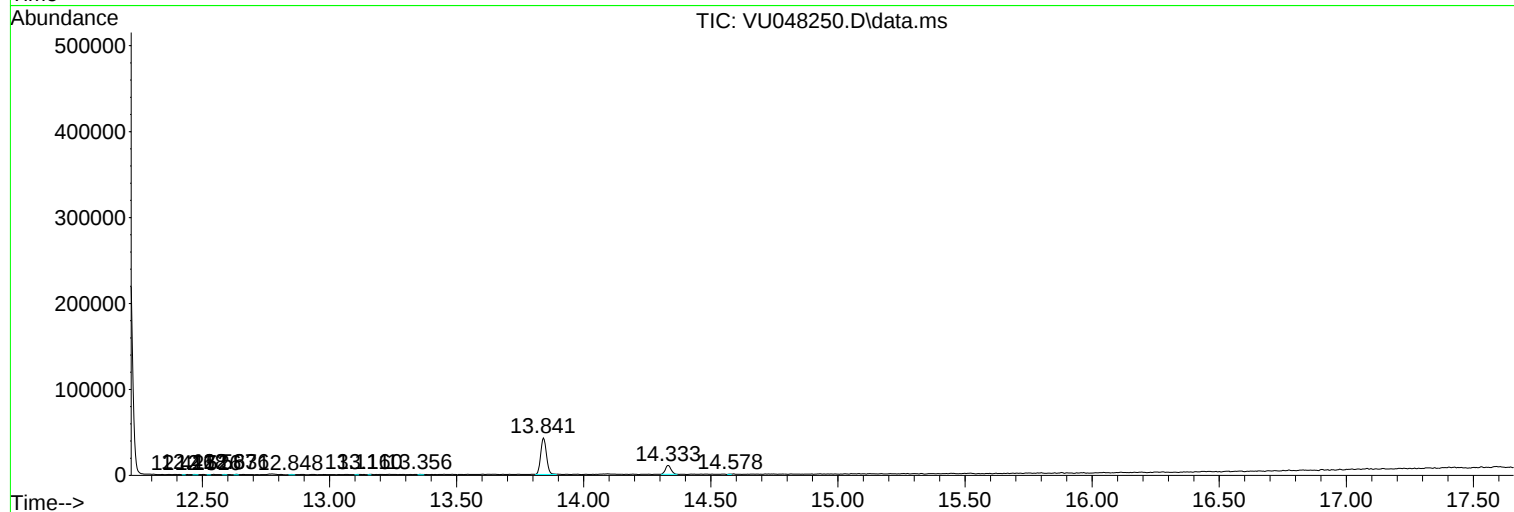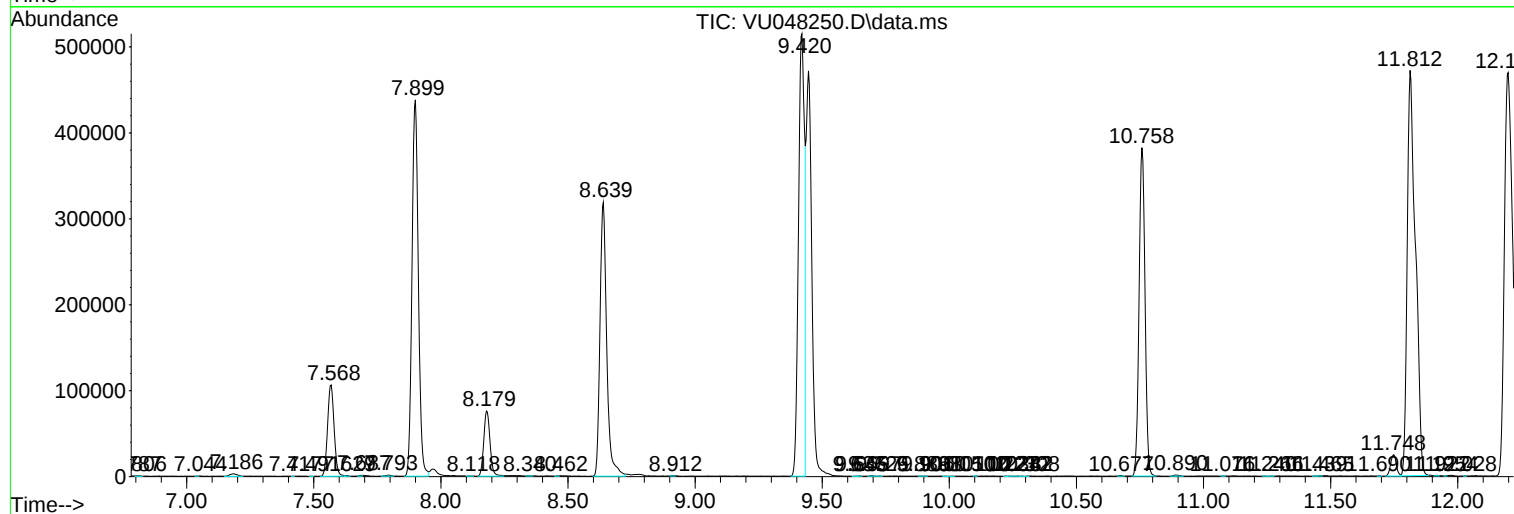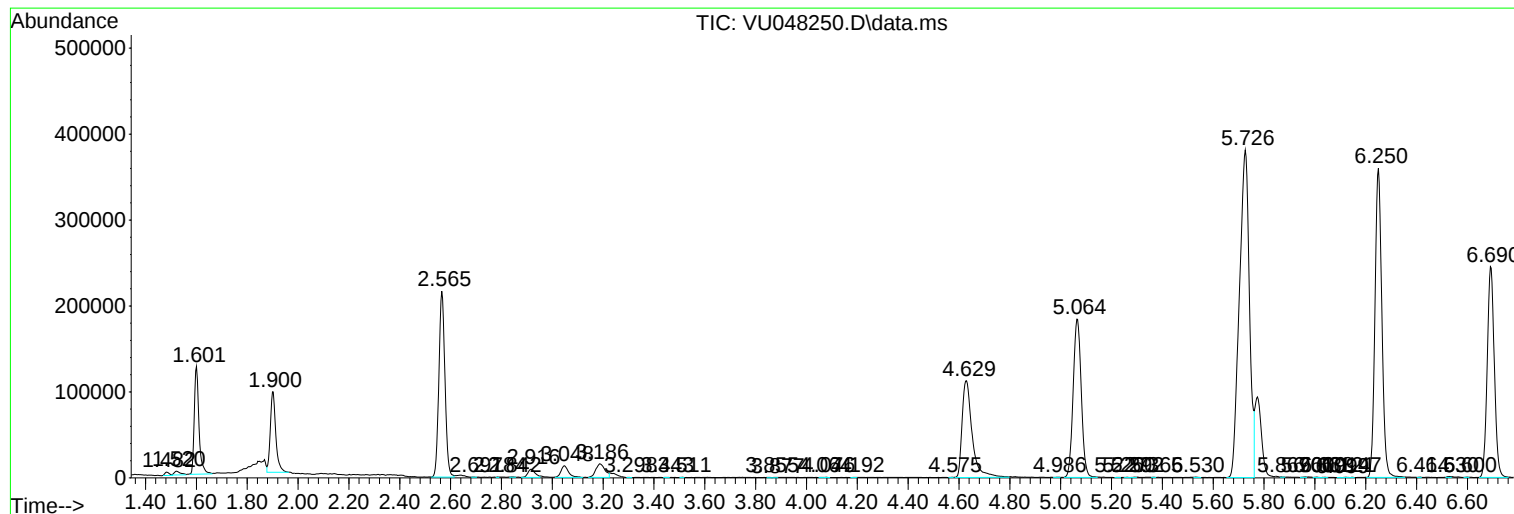

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048250.D
Acq On : 23 Apr 2022 16:49
Operator : SY/MD
Sample : N2488-09DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048250.D
Acq On : 23 Apr 2022 16:49
Operator : SY/MD
Sample : N2488-09DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc