

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048251.D
 Acq On : 23 Apr 2022 17:13
 Operator : SY/MD
 Sample : N2488-10DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	2993	2795	0.26%	0.031%
2	1.601	73	81	99	rBV	127379	161934	14.96%	1.775%
3	1.900	167	174	200	rVB	93511	142477	13.16%	1.562%
4	2.520	364	367	369	rBV3	361	253	0.02%	0.003%
5	2.565	369	381	398	rBV	217624	361165	33.36%	3.959%
6	2.732	429	433	435	rBV3	210	163	0.02%	0.002%
7	2.784	445	449	451	rBV3	546	448	0.04%	0.005%
8	2.916	479	490	508	rBV2	10910	22174	2.05%	0.243%
9	3.047	521	531	555	rVB2	13729	28416	2.62%	0.312%
10	3.189	560	575	590	rBV	14415	38989	3.60%	0.427%
11	3.395	634	639	642	rBV	230	226	0.02%	0.002%
12	3.440	650	653	658	rVB2	393	312	0.03%	0.003%
13	3.581	695	697	702	rBV2	274	182	0.02%	0.002%
14	3.790	759	762	765	rVB	248	187	0.02%	0.002%
15	3.810	765	768	770	rBV2	198	177	0.02%	0.002%
16	3.851	776	781	784	rVB2	194	162	0.01%	0.002%
17	3.954	809	813	819	rVB	347	395	0.04%	0.004%
18	3.990	819	824	828	rBV2	196	291	0.03%	0.003%
19	4.031	832	837	839	rBV	165	159	0.01%	0.002%
20	4.263	904	909	911	rBV	182	161	0.01%	0.002%
21	4.359	935	939	943	rBV2	199	217	0.02%	0.002%
22	4.507	981	985	991	rBV2	265	280	0.03%	0.003%
23	4.629	1009	1023	1061	rBV	111706	296003	27.34%	3.245%
24	4.809	1076	1079	1084	rVB4	430	305	0.03%	0.003%
25	4.851	1090	1092	1096	rBV2	417	205	0.02%	0.002%
26	5.063	1138	1158	1184	rBV	185678	409689	37.84%	4.491%
27	5.166	1188	1190	1194	rVB3	313	174	0.02%	0.002%
28	5.289	1223	1228	1232	rBV3	329	448	0.04%	0.005%
29	5.337	1240	1243	1244	rBV2	386	261	0.02%	0.003%
30	5.443	1274	1276	1285	rVB2	203	213	0.02%	0.002%
31	5.530	1295	1303	1308	rVB	552	829	0.08%	0.009%
32	5.726	1342	1364	1375	rBV2	389885	1058951	97.82%	11.609%
33	5.970	1435	1440	1441	rBV2	335	265	0.02%	0.003%
34	6.047	1458	1464	1469	rVV4	489	521	0.05%	0.006%
35	6.128	1487	1489	1493	rBV	403	231	0.02%	0.003%
36	6.250	1512	1527	1551	rBV	345690	654605	60.47%	7.176%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048251.D
 Acq On : 23 Apr 2022 17:13
 Operator : SY/MD
 Sample : N2488-10DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.456	1589	1591	1597	rVB2	303	267	0.02%	0.003%
38	6.536	1605	1616	1621	rBV6	1523	2707	0.25%	0.030%
39	6.594	1630	1634	1635	rBV	356	229	0.02%	0.003%
40	6.620	1639	1642	1647	rVB2	345	282	0.03%	0.003%
41	6.690	1650	1664	1688	rBV	242769	473346	43.72%	5.189%
42	6.813	1699	1702	1705	rBV2	575	322	0.03%	0.004%
43	6.999	1757	1760	1766	rVB2	195	229	0.02%	0.003%
44	7.044	1769	1774	1776	rVV3	330	341	0.03%	0.004%
45	7.060	1776	1779	1784	rVV2	374	423	0.04%	0.005%
46	7.092	1786	1789	1793	rVB	224	165	0.02%	0.002%
47	7.128	1793	1800	1803	rBV	250	269	0.02%	0.003%
48	7.189	1807	1819	1830	rVB7	2796	5887	0.54%	0.065%
49	7.330	1859	1863	1867	rVB2	227	222	0.02%	0.002%
50	7.382	1867	1879	1884	rBV2	341	515	0.05%	0.006%
51	7.565	1923	1936	1955	rVV	106007	189456	17.50%	2.077%
52	7.633	1955	1957	1965	rVB3	589	611	0.06%	0.007%
53	7.694	1969	1976	1986	rVB4	995	1492	0.14%	0.016%
54	7.745	1989	1992	1995	rVB2	374	218	0.02%	0.002%
55	7.768	1995	1999	2000	rBV2	356	254	0.02%	0.003%
56	7.790	2000	2006	2009	rBV4	629	762	0.07%	0.008%
57	7.899	2026	2040	2056	rBV	447570	780172	72.07%	8.552%
58	8.118	2104	2108	2110	rBV2	261	194	0.02%	0.002%
59	8.179	2113	2127	2145	rBV	74984	128516	11.87%	1.409%
60	8.478	2217	2220	2225	rVB2	306	227	0.02%	0.002%
61	8.559	2241	2245	2250	rVB2	214	218	0.02%	0.002%
62	8.581	2250	2252	2256	rBV2	451	340	0.03%	0.004%
63	8.639	2256	2270	2299	rBV	317512	584041	53.95%	6.402%
64	8.899	2347	2351	2352	rBV	238	171	0.02%	0.002%
65	8.909	2352	2354	2362	rVB3	472	552	0.05%	0.006%
66	9.054	2394	2399	2402	rBV2	224	251	0.02%	0.003%
67	9.108	2412	2416	2420	rBV2	426	448	0.04%	0.005%
68	9.160	2428	2432	2435	rBV2	343	234	0.02%	0.003%
69	9.182	2436	2439	2441	rBV3	296	172	0.02%	0.002%
70	9.308	2474	2478	2481	rVB2	238	193	0.02%	0.002%
71	9.337	2481	2487	2489	rBV	326	397	0.04%	0.004%
72	9.420	2499	2513	2517	rBV	505457	847268	78.27%	9.288%
73	9.684	2592	2595	2596	rVV	338	157	0.01%	0.002%
74	9.864	2648	2651	2654	rVB2	198	161	0.01%	0.002%
75	10.044	2703	2707	2709	rBV2	255	227	0.02%	0.002%
76	10.102	2722	2725	2731	rVB3	503	535	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048251.D
 Acq On : 23 Apr 2022 17:13
 Operator : SY/MD
 Sample : N2488-10DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.153	2736	2741	2742	rBV	234	177	0.02%	0.002%
78	10.366	2804	2807	2809	rBV	453	310	0.03%	0.003%
79	10.488	2839	2845	2849	rBV3	262	299	0.03%	0.003%
80	10.671	2898	2902	2907	rVB3	749	663	0.06%	0.007%
81	10.758	2916	2929	2947	rBV	389605	621574	57.42%	6.814%
82	10.861	2954	2961	2965	rBV2	354	462	0.04%	0.005%
83	11.137	3042	3047	3049	rBV2	382	269	0.02%	0.003%
84	11.156	3049	3053	3058	rVB2	462	380	0.04%	0.004%
85	11.218	3069	3072	3078	rVB2	285	236	0.02%	0.003%
86	11.256	3078	3084	3087	rBV3	327	346	0.03%	0.004%
87	11.337	3105	3109	3115	rVB2	344	375	0.03%	0.004%
88	11.468	3142	3150	3157	rVB4	638	1105	0.10%	0.012%
89	11.703	3219	3223	3227	rBV2	507	405	0.04%	0.004%
90	11.745	3227	3236	3245	rBV2	25514	38778	3.58%	0.425%
91	11.812	3245	3257	3285	rVB2	480772	1082556	100.00%	11.867%
92	11.970	3303	3306	3309	rBV2	544	329	0.03%	0.004%
93	12.198	3362	3377	3399	rBV3	482293	1079496	99.72%	11.834%
94	12.539	3481	3483	3489	rBV3	301	223	0.02%	0.002%
95	12.973	3616	3618	3624	rBV3	259	224	0.02%	0.002%
96	13.317	3723	3725	3728	rBV	341	219	0.02%	0.002%
97	13.841	3878	3888	3900	rBV	42835	68415	6.32%	0.750%
98	14.330	4031	4040	4055	rBV2	11095	17778	1.64%	0.195%
99	14.578	4112	4117	4120	rBV4	601	613	0.06%	0.007%
100	15.324	4347	4349	4351	rBV	438	237	0.02%	0.003%




Sum of corrected areas: 9122203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048251.D
Acq On : 23 Apr 2022 17:13
Operator : SY/MD
Sample : N2488-10DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

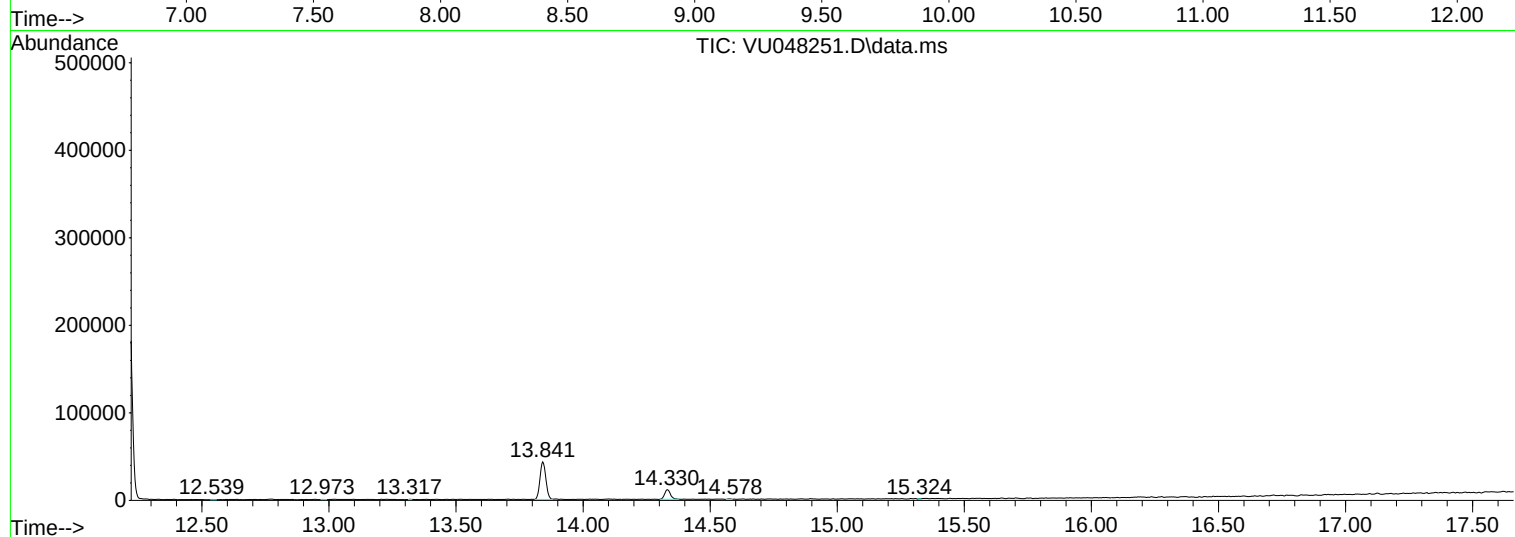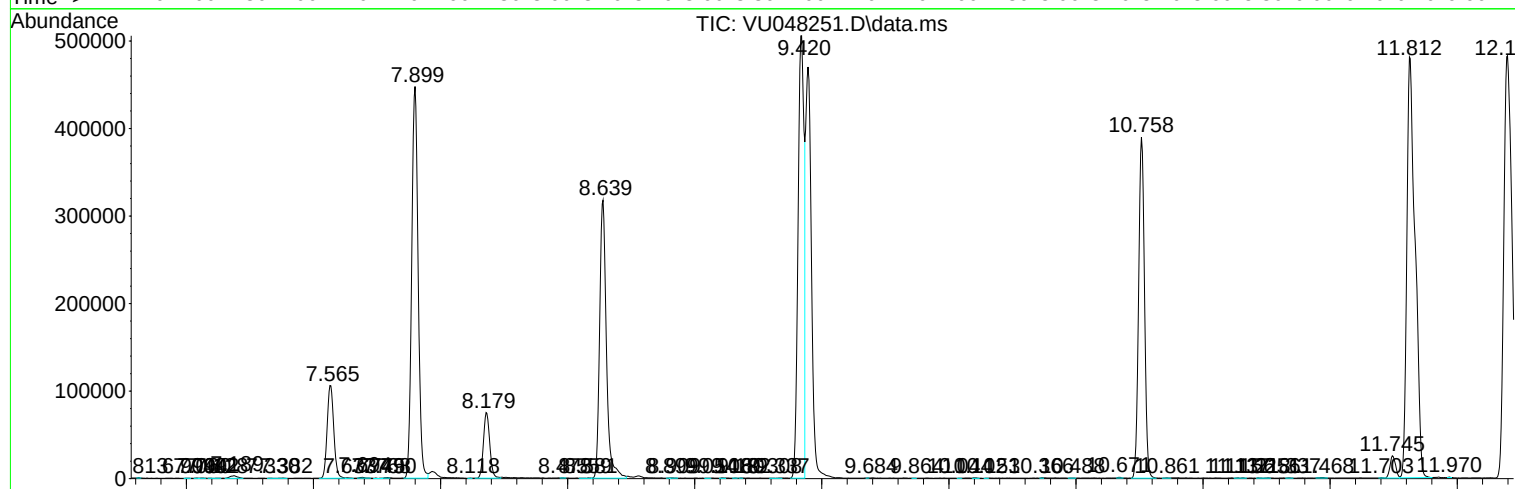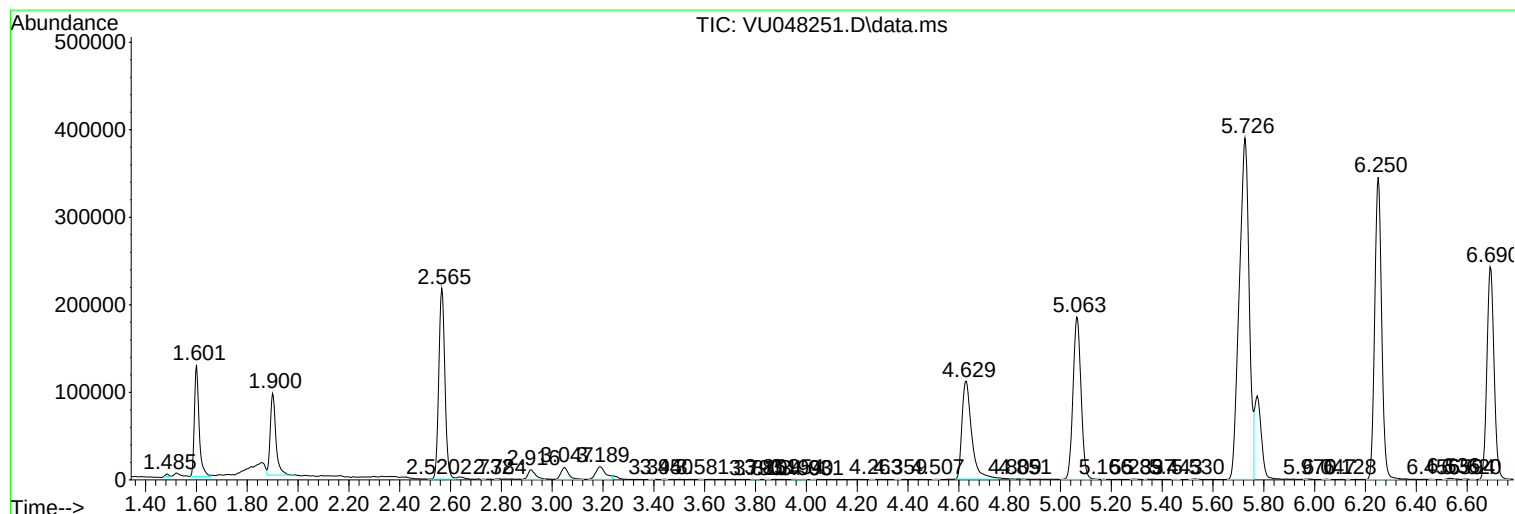

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048251.D
Acq On : 23 Apr 2022 17:13
Operator : SY/MD
Sample : N2488-10DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048251.D
Acq On : 23 Apr 2022 17:13
Operator : SY/MD
Sample : N2488-10DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc