

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048252.D
 Acq On : 23 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2488-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rBV2	3638	4054	0.15%	0.033%
2	1.520	52	56	65	rVV3	3355	4584	0.17%	0.037%
3	1.601	73	81	99	rBV	124748	161159	6.09%	1.308%
4	1.890	165	171	188	rVB	88729	136137	5.15%	1.105%
5	2.562	367	380	396	rBV	222170	367501	13.89%	2.983%
6	2.723	428	430	436	rVB3	566	379	0.01%	0.003%
7	2.758	436	441	442	rBV	298	225	0.01%	0.002%
8	2.764	442	443	446	rBV	258	160	0.01%	0.001%
9	2.793	447	452	455	rBV3	514	452	0.02%	0.004%
10	2.829	460	463	475	rVB4	913	1380	0.05%	0.011%
11	2.912	485	489	491	rBV	373	269	0.01%	0.002%
12	2.948	496	500	502	rBV2	334	234	0.01%	0.002%
13	3.047	519	531	549	rBV2	14055	29112	1.10%	0.236%
14	3.186	560	574	586	rBV	15994	36613	1.38%	0.297%
15	3.334	612	620	624	rBV3	238	326	0.01%	0.003%
16	3.391	633	638	642	rBV	249	268	0.01%	0.002%
17	3.494	667	670	673	rBV2	281	158	0.01%	0.001%
18	3.983	814	822	825	rBV	376	485	0.02%	0.004%
19	4.401	946	952	955	rBV2	172	187	0.01%	0.002%
20	4.546	994	997	1000	rBV2	184	157	0.01%	0.001%
21	4.626	1009	1022	1046	rBV	109479	287402	10.86%	2.333%
22	4.915	1109	1112	1116	rBV2	311	225	0.01%	0.002%
23	5.063	1141	1158	1183	rBV	187517	410927	15.53%	3.335%
24	5.234	1203	1211	1218	rVB2	319	494	0.02%	0.004%
25	5.292	1221	1229	1233	rBV3	443	686	0.03%	0.006%
26	5.333	1238	1242	1243	rBV	445	317	0.01%	0.003%
27	5.375	1252	1255	1258	rBV3	230	166	0.01%	0.001%
28	5.388	1258	1259	1264	rVB	304	177	0.01%	0.001%
29	5.517	1295	1299	1302	rBV4	514	507	0.02%	0.004%
30	5.591	1316	1322	1326	rBV2	164	209	0.01%	0.002%
31	5.726	1343	1364	1373	rBV2	398723	1071910	40.51%	8.700%
32	6.070	1464	1471	1472	rBV	149	162	0.01%	0.001%
33	6.108	1479	1483	1484	rBV2	269	156	0.01%	0.001%
34	6.131	1488	1490	1492	rVB2	327	165	0.01%	0.001%
35	6.169	1498	1502	1506	rBV2	208	187	0.01%	0.002%
36	6.250	1513	1527	1553	rBV	353255	678434	25.64%	5.506%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048252.D
 Acq On : 23 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2488-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.375	1564	1566	1572	rVB2	379	260	0.01%	0.002%
38	6.446	1584	1588	1590	rVB2	425	265	0.01%	0.002%
39	6.523	1607	1612	1616	rBV3	713	820	0.03%	0.007%
40	6.571	1623	1627	1629	rBV2	313	206	0.01%	0.002%
41	6.584	1629	1631	1633	rBV2	331	212	0.01%	0.002%
42	6.690	1650	1664	1681	rBV	248408	481643	18.20%	3.909%
43	6.800	1696	1698	1699	rBV	462	237	0.01%	0.002%
44	6.935	1736	1740	1746	rVB3	293	326	0.01%	0.003%
45	7.050	1773	1776	1778	rVV2	452	294	0.01%	0.002%
46	7.067	1778	1781	1785	rVB2	282	273	0.01%	0.002%
47	7.179	1806	1816	1829	rBV4	3723	7744	0.29%	0.063%
48	7.321	1858	1860	1864	rBV2	268	201	0.01%	0.002%
49	7.362	1870	1873	1877	rVV2	287	266	0.01%	0.002%
50	7.459	1900	1903	1908	rVB	258	225	0.01%	0.002%
51	7.565	1924	1936	1957	rBV	109456	192989	7.29%	1.566%
52	7.684	1967	1973	1980	rBV4	922	1395	0.05%	0.011%
53	7.796	2002	2008	2009	rBV2	494	448	0.02%	0.004%
54	7.899	2025	2040	2054	rBV	444776	773607	29.24%	6.279%
55	8.070	2090	2093	2101	rVB2	663	841	0.03%	0.007%
56	8.179	2115	2127	2148	rBV	76009	129561	4.90%	1.052%
57	8.269	2153	2155	2158	rBV	244	192	0.01%	0.002%
58	8.459	2211	2214	2217	rBV3	326	219	0.01%	0.002%
59	8.475	2217	2219	2225	rVB3	258	208	0.01%	0.002%
60	8.504	2226	2228	2235	rVB2	422	385	0.01%	0.003%
61	8.555	2240	2244	2246	rBV2	280	216	0.01%	0.002%
62	8.639	2257	2270	2304	rBV	348321	651534	24.62%	5.288%
63	8.954	2358	2368	2370	rBV	369	490	0.02%	0.004%
64	8.976	2371	2375	2379	rVV2	240	251	0.01%	0.002%
65	9.169	2430	2435	2438	rBV2	256	277	0.01%	0.002%
66	9.279	2466	2469	2479	rVB	411	461	0.02%	0.004%
67	9.420	2499	2513	2516	rBV	552636	857945	32.42%	6.963%
68	9.693	2593	2598	2605	rVB4	642	873	0.03%	0.007%
69	9.835	2634	2642	2645	rBV3	396	465	0.02%	0.004%
70	9.986	2684	2689	2691	rBV	242	203	0.01%	0.002%
71	10.086	2715	2720	2722	rBV2	265	227	0.01%	0.002%
72	10.288	2778	2783	2787	rBV2	396	408	0.02%	0.003%
73	10.391	2812	2815	2817	rBV2	258	161	0.01%	0.001%
74	10.484	2841	2844	2848	rBV2	223	192	0.01%	0.002%
75	10.597	2876	2879	2884	rBV2	276	352	0.01%	0.003%
76	10.661	2895	2899	2900	rBV2	310	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048252.D
 Acq On : 23 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2488-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.674	2900	2903	2908	rVB3	769	672	0.03%	0.005%
78	10.758	2916	2929	2952	rVB	400738	644941	24.37%	5.235%
79	10.880	2965	2967	2970	rBV2	513	309	0.01%	0.003%
80	11.118	3038	3041	3046	rBV2	481	430	0.02%	0.003%
81	11.163	3052	3055	3061	rBV2	338	304	0.01%	0.002%
82	11.230	3073	3076	3078	rBV2	242	166	0.01%	0.001%
83	11.327	3102	3106	3108	rBV	291	201	0.01%	0.002%
84	11.465	3140	3149	3156	rVB5	967	1686	0.06%	0.014%
85	11.645	3202	3205	3207	rBV2	345	222	0.01%	0.002%
86	11.748	3226	3237	3246	rBV	56117	86714	3.28%	0.704%
87	11.835	3246	3264	3287	rVB2	946322	2251110	85.08%	18.271%
88	11.944	3295	3298	3299	rBV2	562	279	0.01%	0.002%
89	12.211	3361	3381	3403	rBV2	1279815	2645945	100.00%	21.476%
90	12.533	3478	3481	3485	rBV2	368	243	0.01%	0.002%
91	12.594	3495	3500	3504	rBV3	420	454	0.02%	0.004%
92	12.764	3548	3553	3555	rBV2	810	655	0.02%	0.005%
93	12.983	3615	3621	3627	rVB4	936	1108	0.04%	0.009%
94	13.224	3693	3696	3699	rBV2	265	178	0.01%	0.001%
95	13.410	3751	3754	3756	rBV3	303	215	0.01%	0.002%
96	13.587	3806	3809	3816	rVB3	348	364	0.01%	0.003%
97	13.623	3817	3820	3824	rVV4	348	273	0.01%	0.002%
98	13.841	3876	3888	3912	rBV	204057	326811	12.35%	2.653%
99	14.330	4031	4040	4053	rVB2	33671	53904	2.04%	0.438%
100	15.301	4340	4342	4345	rVB2	863	479	0.02%	0.004%


Sum of corrected areas: 12320724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048252.D
Acq On : 23 Apr 2022 17:37
Operator : SY/MD
Sample : N2488-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

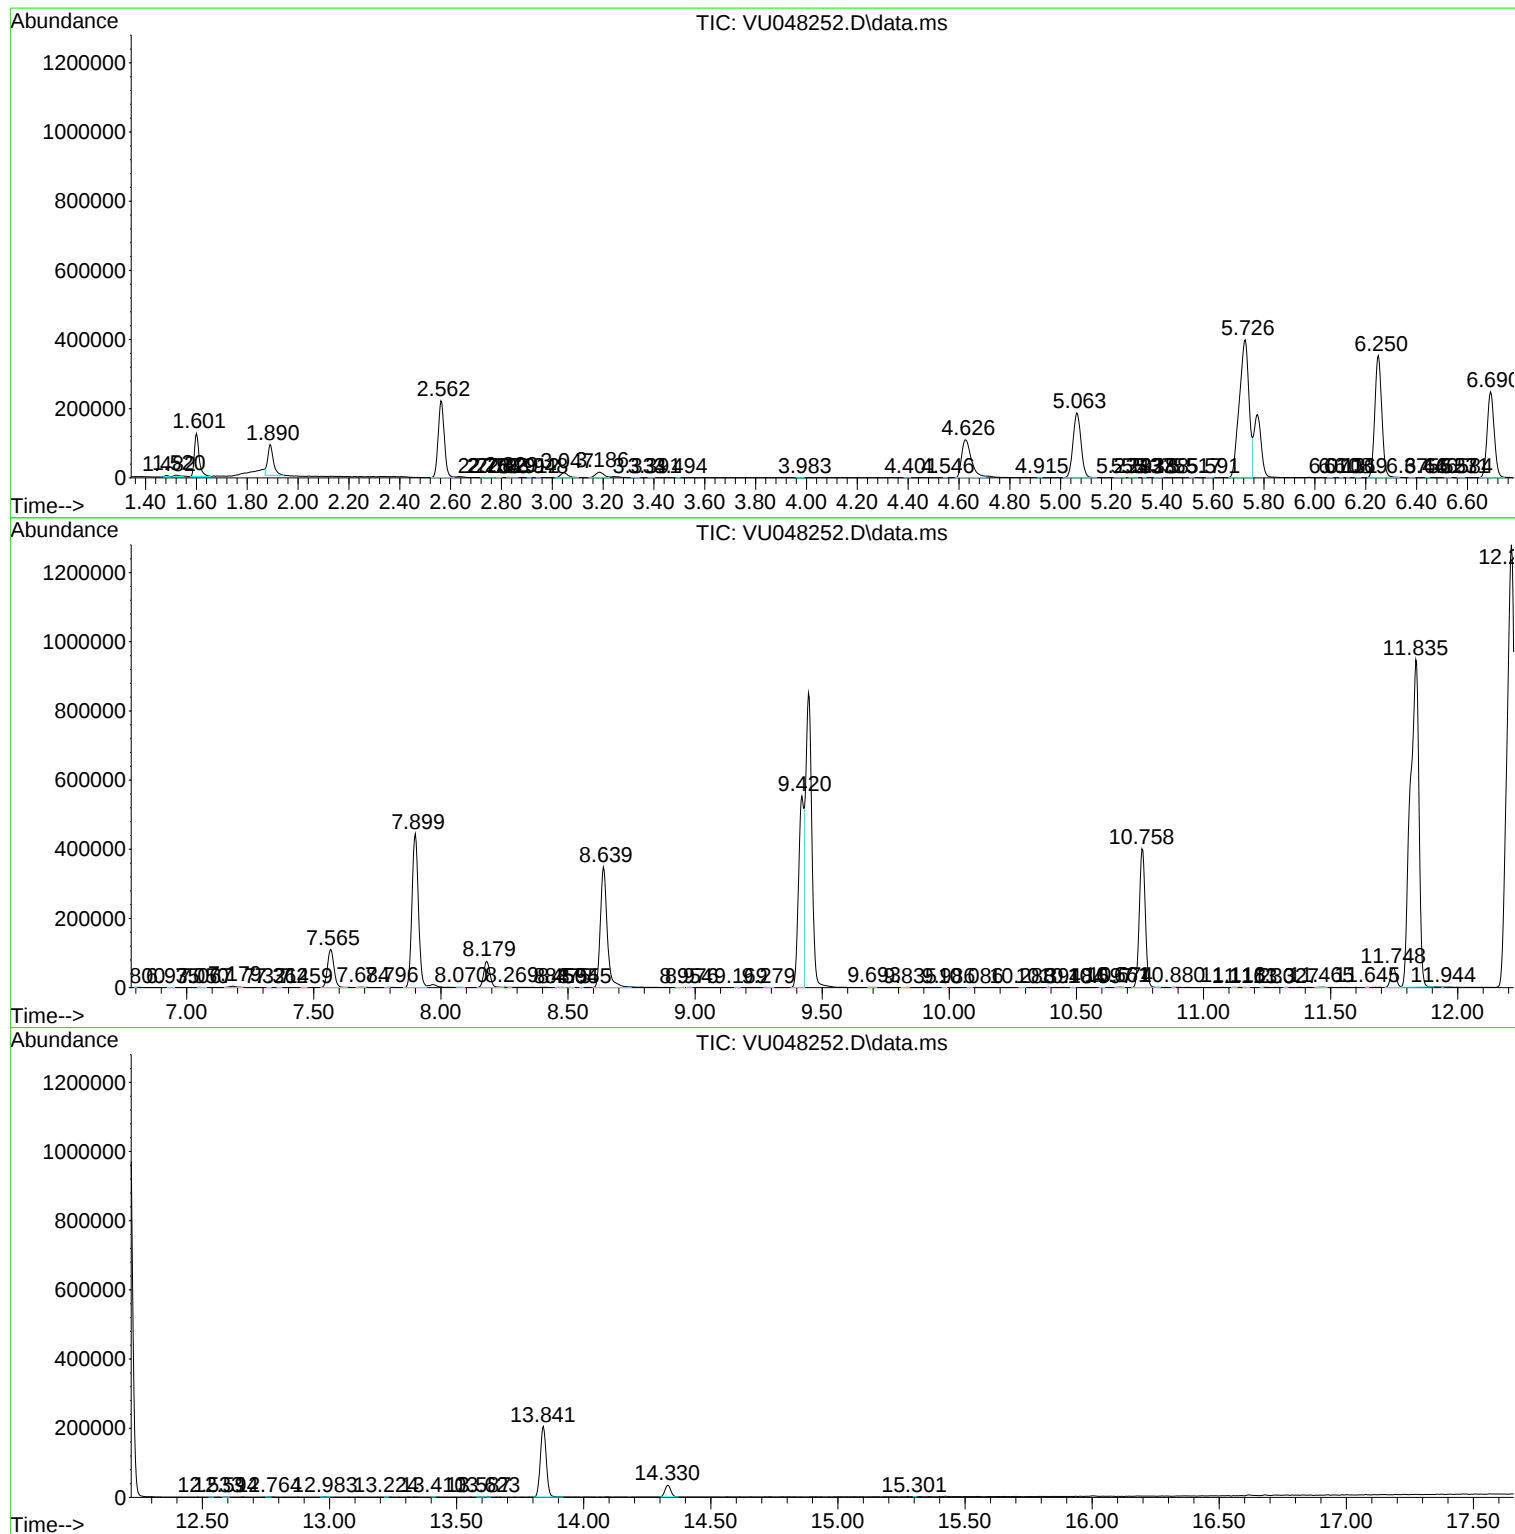

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048252.D
Acq On : 23 Apr 2022 17:37
Operator : SY/MD
Sample : N2488-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048252.D
Acq On : 23 Apr 2022 17:37
Operator : SY/MD
Sample : N2488-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------