

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048254.D
 Acq On : 23 Apr 2022 18:24
 Operator : SY/MD
 Sample : N2485-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	3575	3417	0.31%	0.040%
2	1.520	52	56	67	rVB	4262	5120	0.46%	0.059%
3	1.600	73	81	98	rBV	143070	180150	16.31%	2.083%
4	1.899	166	174	199	rVB	100409	149503	13.54%	1.729%
5	2.565	369	381	398	rBV	239786	395933	35.85%	4.578%
6	2.957	497	503	504	rBV3	697	713	0.06%	0.008%
7	3.047	521	531	538	rBV5	2205	3732	0.34%	0.043%
8	3.095	543	546	551	rVB3	397	414	0.04%	0.005%
9	3.186	560	574	603	rBV2	18791	55629	5.04%	0.643%
10	3.292	603	607	613	rBV2	265	286	0.03%	0.003%
11	3.404	636	642	645	rBV2	173	211	0.02%	0.002%
12	3.456	654	658	662	rBV3	374	370	0.03%	0.004%
13	3.552	683	688	691	rVB2	235	241	0.02%	0.003%
14	3.587	695	699	704	rVB2	371	265	0.02%	0.003%
15	3.616	704	708	711	rVB2	199	196	0.02%	0.002%
16	3.636	711	714	716	rBV	336	194	0.02%	0.002%
17	3.661	716	722	723	rBV2	189	191	0.02%	0.002%
18	3.986	817	823	824	rBV2	304	201	0.02%	0.002%
19	4.044	837	841	845	rBV2	229	252	0.02%	0.003%
20	4.083	850	853	857	rBV2	207	213	0.02%	0.002%
21	4.195	883	888	892	rVV2	163	191	0.02%	0.002%
22	4.321	923	927	930	rBV2	282	200	0.02%	0.002%
23	4.530	988	992	994	rBV	306	225	0.02%	0.003%
24	4.623	1008	1021	1047	rBV	118724	297550	26.94%	3.441%
25	4.986	1131	1134	1138	rVB2	234	238	0.02%	0.003%
26	5.063	1142	1158	1186	rVV	194908	426198	38.59%	4.928%
27	5.195	1196	1199	1202	rVB3	395	255	0.02%	0.003%
28	5.214	1202	1205	1209	rBV3	336	246	0.02%	0.003%
29	5.295	1221	1230	1233	rBV3	472	736	0.07%	0.009%
30	5.343	1237	1245	1250	rBV4	472	988	0.09%	0.011%
31	5.726	1341	1364	1390	rBV2	414886	1104493	100.00%	12.772%
32	5.960	1434	1437	1438	rBV	382	202	0.02%	0.002%
33	5.970	1438	1440	1444	rVV3	502	388	0.04%	0.004%
34	6.250	1512	1527	1553	rBV	349067	661663	59.91%	7.651%
35	6.491	1598	1602	1607	rVB2	355	282	0.03%	0.003%
36	6.529	1607	1614	1622	rBV3	945	1389	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048254.D
 Acq On : 23 Apr 2022 18:24
 Operator : SY/MD
 Sample : N2485-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.562	1622	1624	1629	rVB2	329	207	0.02%	0.002%
38	6.600	1630	1636	1641	rVB4	352	435	0.04%	0.005%
39	6.690	1649	1664	1685	rBV	252339	496133	44.92%	5.737%
40	6.806	1695	1700	1704	rBV4	793	909	0.08%	0.011%
41	7.054	1772	1777	1785	rBV3	361	612	0.06%	0.007%
42	7.179	1806	1816	1831	rBV6	2860	5983	0.54%	0.069%
43	7.565	1922	1936	1952	rBV	113825	198837	18.00%	2.299%
44	7.674	1968	1970	1971	rBV	420	195	0.02%	0.002%
45	7.690	1971	1975	1986	rVB4	1428	2150	0.19%	0.025%
46	7.793	2001	2007	2011	rBV3	648	707	0.06%	0.008%
47	7.899	2024	2040	2055	rBV	475093	818265	74.09%	9.462%
48	8.179	2115	2127	2146	rBV	79496	132806	12.02%	1.536%
49	8.349	2177	2180	2187	rVB3	488	526	0.05%	0.006%
50	8.455	2205	2213	2215	rBV3	462	645	0.06%	0.007%
51	8.516	2231	2232	2237	rVB3	374	207	0.02%	0.002%
52	8.552	2239	2243	2248	rBV	491	412	0.04%	0.005%
53	8.635	2256	2269	2305	rBV	358135	662344	59.97%	7.659%
54	8.851	2333	2336	2341	rVB4	485	287	0.03%	0.003%
55	8.957	2367	2369	2373	rVB	303	207	0.02%	0.002%
56	8.979	2373	2376	2384	rVB	383	474	0.04%	0.005%
57	9.015	2384	2387	2390	rBV	382	289	0.03%	0.003%
58	9.169	2433	2435	2439	rVB2	470	279	0.03%	0.003%
59	9.233	2453	2455	2460	rVB3	300	203	0.02%	0.002%
60	9.417	2499	2512	2553	rBV	488426	830990	75.24%	9.609%
61	9.693	2594	2598	2604	rVB2	397	453	0.04%	0.005%
62	9.870	2650	2653	2656	rBV	215	190	0.02%	0.002%
63	9.918	2666	2668	2674	rVB3	465	471	0.04%	0.005%
64	9.950	2674	2678	2681	rBV2	365	319	0.03%	0.004%
65	10.246	2762	2770	2774	rBV3	470	534	0.05%	0.006%
66	10.426	2823	2826	2832	rVB	322	360	0.03%	0.004%
67	10.462	2833	2837	2840	rBV2	371	324	0.03%	0.004%
68	10.568	2867	2870	2873	rBV	291	253	0.02%	0.003%
69	10.632	2886	2890	2894	rVV2	220	190	0.02%	0.002%
70	10.674	2896	2903	2909	rVB2	1137	1199	0.11%	0.014%
71	10.758	2917	2929	2951	rVB	408770	657457	59.53%	7.603%
72	10.844	2955	2956	2964	rVB2	266	197	0.02%	0.002%
73	10.896	2964	2972	2978	rBV2	1223	1944	0.18%	0.022%
74	10.989	2998	3001	3005	rVB2	377	268	0.02%	0.003%
75	11.024	3010	3012	3019	rVB2	338	326	0.03%	0.004%
76	11.076	3023	3028	3032	rBV2	392	394	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048254.D
 Acq On : 23 Apr 2022 18:24
 Operator : SY/MD
 Sample : N2485-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.159	3049	3054	3056	rBV	262	216	0.02%	0.002%
78	11.208	3064	3069	3071	rBV	265	198	0.02%	0.002%
79	11.401	3124	3129	3132	rBV	234	266	0.02%	0.003%
80	11.452	3138	3145	3146	rBV2	832	697	0.06%	0.008%
81	11.748	3233	3237	3240	rBV3	464	390	0.04%	0.005%
82	11.812	3245	3257	3277	rBV	477713	762789	69.06%	8.821%
83	11.938	3294	3296	3299	rVV4	510	236	0.02%	0.003%
84	11.967	3302	3305	3310	rVV5	453	374	0.03%	0.004%
85	12.195	3362	3376	3398	rBV	446142	735629	66.60%	8.507%
86	12.352	3422	3425	3429	rBV3	314	318	0.03%	0.004%
87	12.555	3485	3488	3489	rBV	393	231	0.02%	0.003%
88	12.719	3536	3539	3543	rVB2	365	273	0.02%	0.003%
89	12.751	3543	3549	3551	rBV2	435	468	0.04%	0.005%
90	12.777	3551	3557	3564	rVV3	812	1155	0.10%	0.013%
91	12.831	3571	3574	3577	rBV2	382	287	0.03%	0.003%
92	13.021	3630	3633	3636	rBV2	388	324	0.03%	0.004%
93	13.063	3643	3646	3649	rBV2	392	271	0.02%	0.003%
94	13.098	3654	3657	3660	rVV2	290	221	0.02%	0.003%
95	13.722	3848	3851	3854	rBV	332	233	0.02%	0.003%
96	13.812	3876	3879	3882	rBV3	643	554	0.05%	0.006%
97	13.844	3883	3889	3899	rVB5	3442	4994	0.45%	0.058%
98	14.333	4036	4041	4047	rBV4	989	1110	0.10%	0.013%
99	14.664	4138	4144	4148	rBV3	638	729	0.07%	0.008%
100	14.860	4197	4205	4223	rBV2	14993	24419	2.21%	0.282%


Sum of corrected areas: 8647838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048254.D
Acq On : 23 Apr 2022 18:24
Operator : SY/MD
Sample : N2485-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

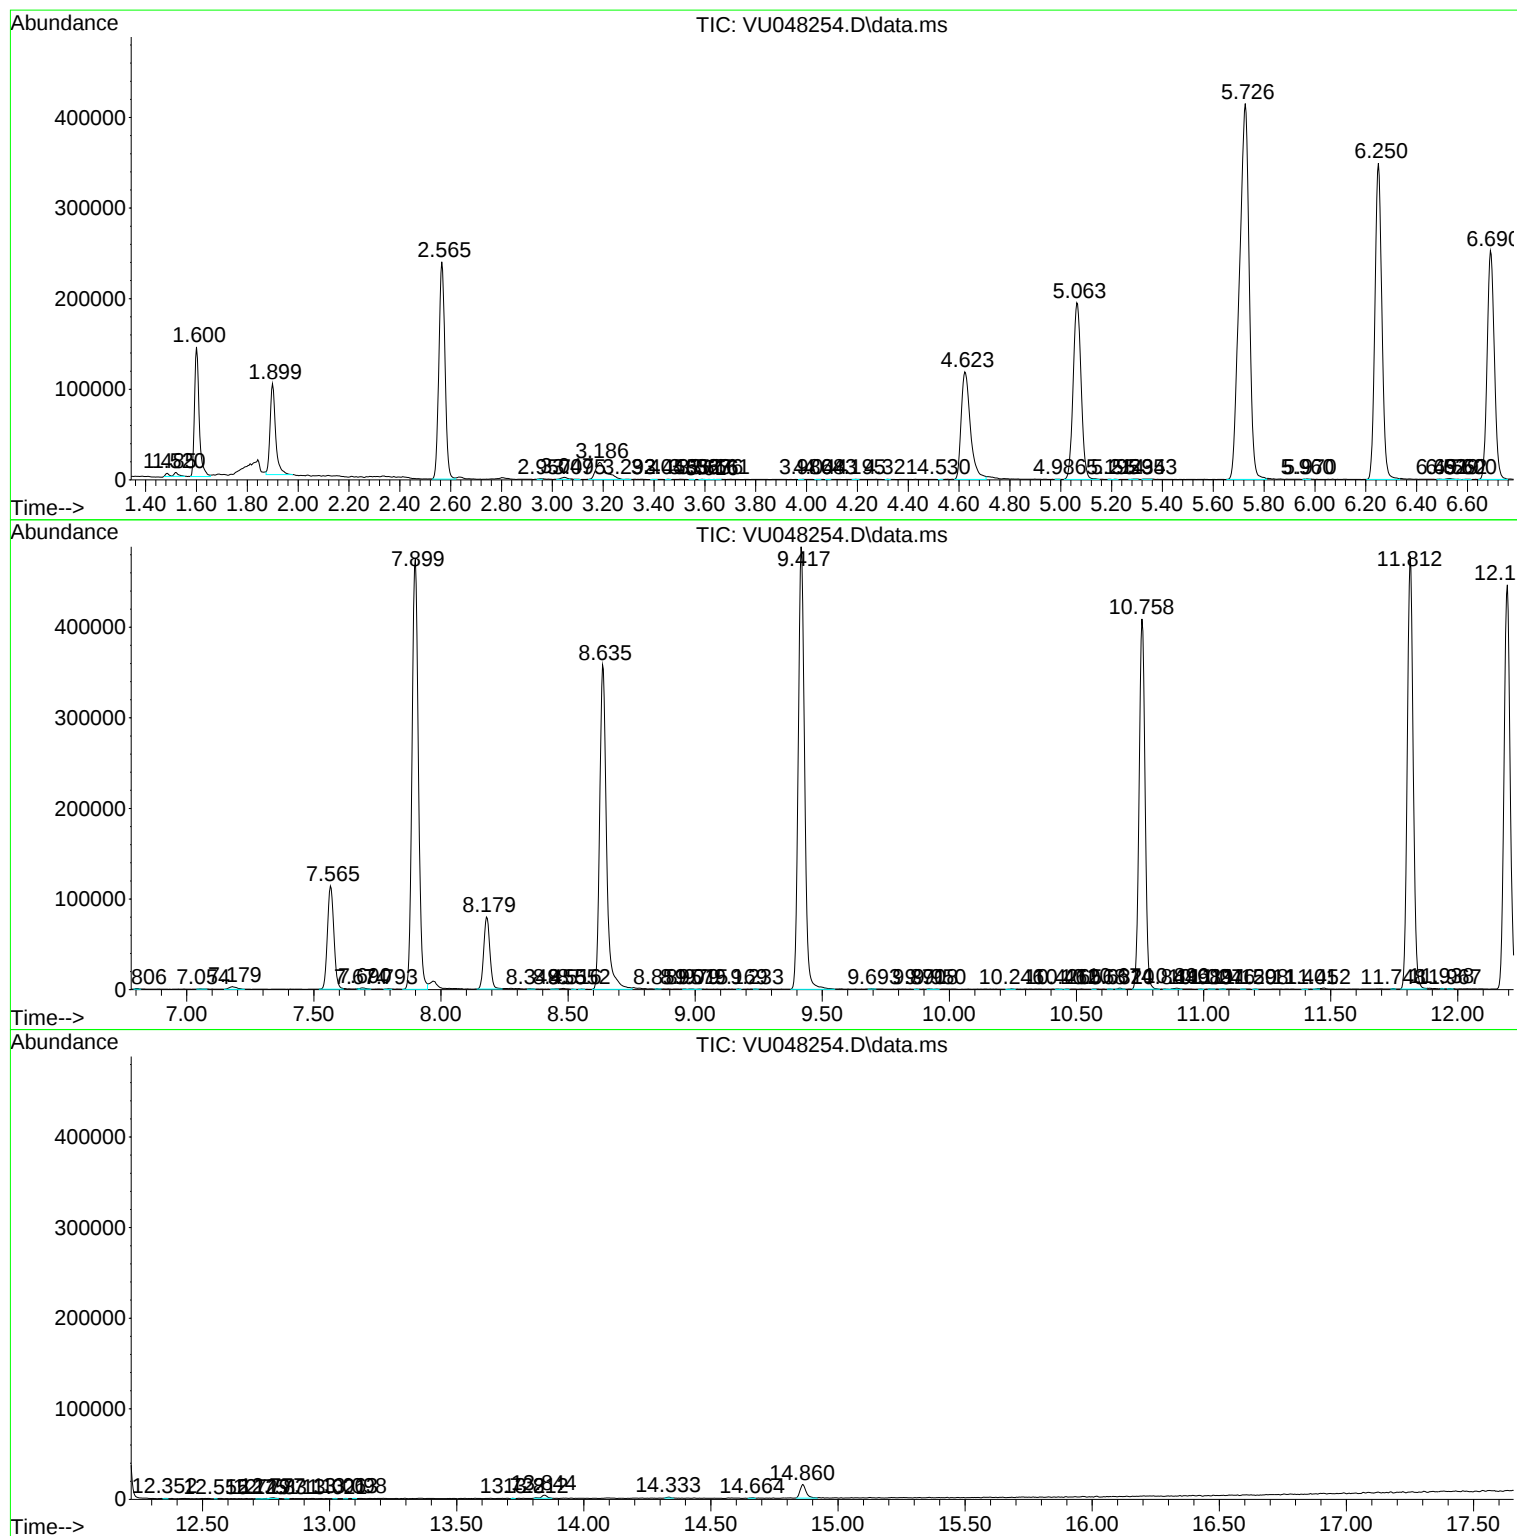

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048254.D
Acq On : 23 Apr 2022 18:24
Operator : SY/MD
Sample : N2485-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048254.D
Acq On : 23 Apr 2022 18:24
Operator : SY/MD
Sample : N2485-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc