

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048255.D
 Acq On : 23 Apr 2022 18:48
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rBV2	4325	4541	0.40%	0.051%
2	1.520	52	56	69	rVV3	4560	8515	0.76%	0.096%
3	1.601	73	81	103	rVV	137326	179097	15.89%	2.021%
4	1.893	166	172	204	rVB	99964	163864	14.54%	1.849%
5	2.562	368	380	398	rBV	239977	397531	35.27%	4.486%
6	2.784	447	449	457	rBV4	274	306	0.03%	0.003%
7	2.819	457	460	463	rBV3	533	404	0.04%	0.005%
8	2.948	496	500	504	rBV2	290	324	0.03%	0.004%
9	3.048	523	531	539	rBV3	1830	3467	0.31%	0.039%
10	3.186	561	574	586	rBV	9273	21170	1.88%	0.239%
11	3.311	609	613	615	rBV2	330	247	0.02%	0.003%
12	3.379	630	634	638	rBV2	292	255	0.02%	0.003%
13	3.449	650	656	660	rBV2	182	284	0.03%	0.003%
14	3.665	720	723	726	rBV2	277	193	0.02%	0.002%
15	3.790	758	762	765	rBV2	256	245	0.02%	0.003%
16	4.163	874	878	883	rVB2	362	329	0.03%	0.004%
17	4.626	1009	1022	1047	rBV	118906	307653	27.29%	3.472%
18	4.842	1086	1089	1093	rBV2	249	251	0.02%	0.003%
19	5.064	1141	1158	1183	rBV2	199677	438147	38.87%	4.944%
20	5.150	1183	1185	1188	rVV2	634	421	0.04%	0.005%
21	5.205	1196	1202	1206	rBV3	182	190	0.02%	0.002%
22	5.301	1222	1232	1235	rVB4	580	810	0.07%	0.009%
23	5.366	1249	1252	1259	rVB3	545	553	0.05%	0.006%
24	5.427	1268	1271	1275	rBV	228	219	0.02%	0.002%
25	5.491	1284	1291	1293	rBV	255	310	0.03%	0.003%
26	5.523	1298	1301	1306	rVV2	345	327	0.03%	0.004%
27	5.726	1343	1364	1396	rBV2	423074	1127234	100.00%	12.721%
28	5.973	1435	1441	1449	rBV4	988	1317	0.12%	0.015%
29	6.109	1480	1483	1486	rBV2	269	223	0.02%	0.003%
30	6.160	1496	1499	1503	rBV2	319	312	0.03%	0.004%
31	6.179	1503	1505	1511	rVB2	216	201	0.02%	0.002%
32	6.250	1511	1527	1556	rBV	351636	671207	59.54%	7.574%
33	6.488	1595	1601	1604	rBV2	288	292	0.03%	0.003%
34	6.526	1608	1613	1616	rBV3	964	1109	0.10%	0.013%
35	6.594	1629	1634	1636	rBV2	389	349	0.03%	0.004%
36	6.610	1637	1639	1646	rVB2	485	328	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048255.D
 Acq On : 23 Apr 2022 18:48
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1688	rBV	262531	516539	45.82%	5.829%
38	6.861	1713	1717	1721	rVB2	331	268	0.02%	0.003%
39	7.051	1774	1776	1782	rVB3	572	470	0.04%	0.005%
40	7.134	1799	1802	1807	rVB2	298	266	0.02%	0.003%
41	7.182	1807	1817	1831	rBV4	3972	8428	0.75%	0.095%
42	7.298	1848	1853	1857	rBV3	277	259	0.02%	0.003%
43	7.565	1924	1936	1960	rBV	116011	207064	18.37%	2.337%
44	7.687	1968	1974	1975	rBV3	1064	859	0.08%	0.010%
45	7.793	2004	2007	2010	rBV3	443	296	0.03%	0.003%
46	7.822	2013	2016	2020	rVB2	305	201	0.02%	0.002%
47	7.899	2023	2040	2056	rBV	483432	832573	73.86%	9.395%
48	8.131	2109	2112	2115	rBV2	241	184	0.02%	0.002%
49	8.179	2115	2127	2144	rBV	80349	135419	12.01%	1.528%
50	8.343	2175	2178	2180	rVV2	453	230	0.02%	0.003%
51	8.401	2189	2196	2199	rVB	246	305	0.03%	0.003%
52	8.514	2228	2231	2237	rBV2	271	288	0.03%	0.003%
53	8.639	2256	2270	2300	rBV	369988	692998	61.48%	7.820%
54	8.829	2327	2329	2333	rVB2	366	236	0.02%	0.003%
55	8.851	2333	2336	2338	rBV2	284	189	0.02%	0.002%
56	8.951	2361	2367	2368	rBV	444	376	0.03%	0.004%
57	9.157	2425	2431	2432	rBV2	205	190	0.02%	0.002%
58	9.221	2447	2451	2453	rBV	177	185	0.02%	0.002%
59	9.417	2499	2512	2533	rBV	510642	862885	76.55%	9.737%
60	9.571	2556	2560	2561	rBV2	400	215	0.02%	0.002%
61	9.690	2594	2597	2598	rBV	476	296	0.03%	0.003%
62	9.851	2643	2647	2652	rVB	265	245	0.02%	0.003%
63	9.877	2652	2655	2659	rBV2	215	206	0.02%	0.002%
64	9.938	2671	2674	2677	rBV2	265	221	0.02%	0.002%
65	10.240	2764	2768	2771	rVB2	378	295	0.03%	0.003%
66	10.269	2771	2777	2780	rBV2	277	305	0.03%	0.003%
67	10.382	2809	2812	2816	rVB2	283	196	0.02%	0.002%
68	10.430	2821	2827	2834	rVB	161	204	0.02%	0.002%
69	10.468	2834	2839	2842	rBV2	178	194	0.02%	0.002%
70	10.629	2885	2889	2891	rBV	231	179	0.02%	0.002%
71	10.665	2895	2900	2902	rBV5	864	638	0.06%	0.007%
72	10.758	2916	2929	2950	rVV	434901	698450	61.96%	7.882%
73	10.880	2964	2967	2968	rBV3	441	289	0.03%	0.003%
74	10.896	2968	2972	2978	rVB3	918	1038	0.09%	0.012%
75	11.292	3092	3095	3097	rBV2	237	177	0.02%	0.002%
76	11.362	3112	3117	3122	rBV2	291	327	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048255.D
 Acq On : 23 Apr 2022 18:48
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3150	rBV4	478	624	0.06%	0.007%
78	11.603	3185	3192	3194	rBV2	362	481	0.04%	0.005%
79	11.671	3207	3213	3217	rBV	215	249	0.02%	0.003%
80	11.706	3221	3224	3229	rBV2	335	276	0.02%	0.003%
81	11.812	3244	3257	3277	rBV	485630	778786	69.09%	8.788%
82	12.005	3315	3317	3322	rVB	316	193	0.02%	0.002%
83	12.134	3355	3357	3362	rBV2	214	202	0.02%	0.002%
84	12.195	3362	3376	3395	rVV	472937	771569	68.45%	8.707%
85	12.372	3425	3431	3433	rBV2	388	448	0.04%	0.005%
86	12.507	3471	3473	3477	rBV2	283	226	0.02%	0.003%
87	12.636	3510	3513	3515	rBV	237	199	0.02%	0.002%
88	12.674	3521	3525	3528	rBV2	405	314	0.03%	0.004%
89	12.732	3540	3543	3545	rBV	369	217	0.02%	0.002%
90	12.751	3545	3549	3551	rVV	297	285	0.03%	0.003%
91	12.767	3551	3554	3562	rVB3	677	954	0.08%	0.011%
92	12.800	3562	3564	3575	rVB3	404	433	0.04%	0.005%
93	12.848	3575	3579	3581	rBV3	544	428	0.04%	0.005%
94	12.992	3621	3624	3629	rBV3	291	341	0.03%	0.004%
95	13.099	3655	3657	3660	rBV2	253	191	0.02%	0.002%
96	13.629	3817	3822	3825	rBV3	448	486	0.04%	0.005%
97	13.848	3884	3890	3901	rVB3	1524	2031	0.18%	0.023%
98	14.189	3992	3996	3999	rBV2	452	416	0.04%	0.005%
99	14.333	4038	4041	4049	rBV3	704	961	0.09%	0.011%
100	14.867	4200	4207	4217	rBV7	3102	4822	0.43%	0.054%




Sum of corrected areas: 8861540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048255.D
Acq On : 23 Apr 2022 18:48
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

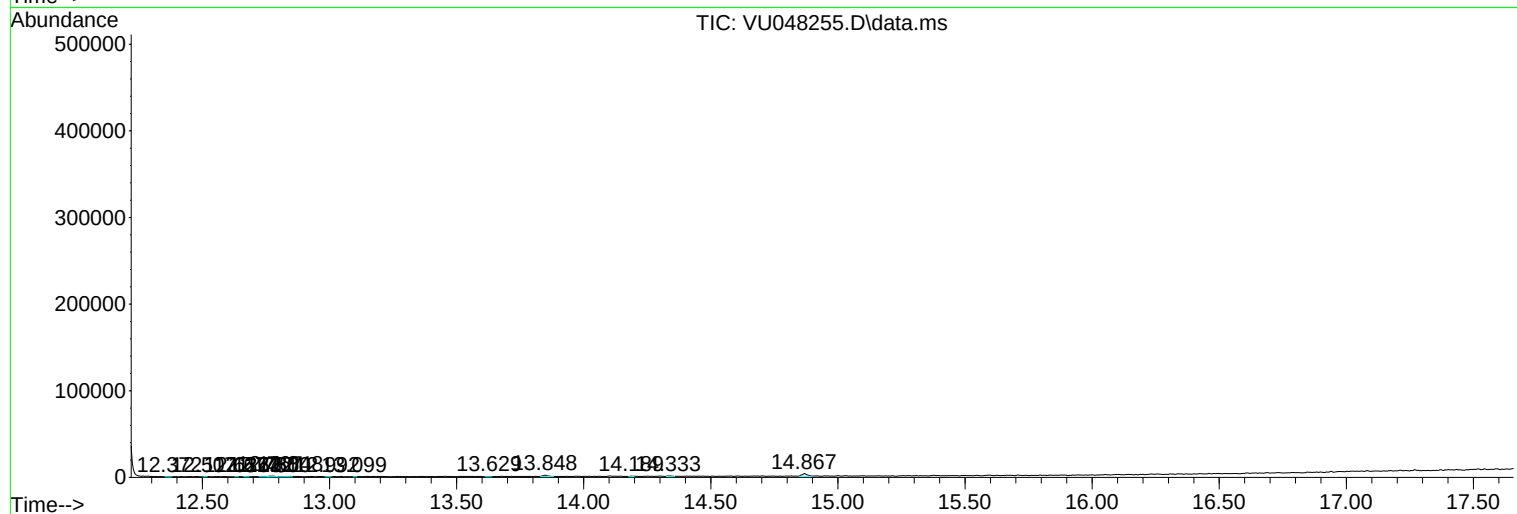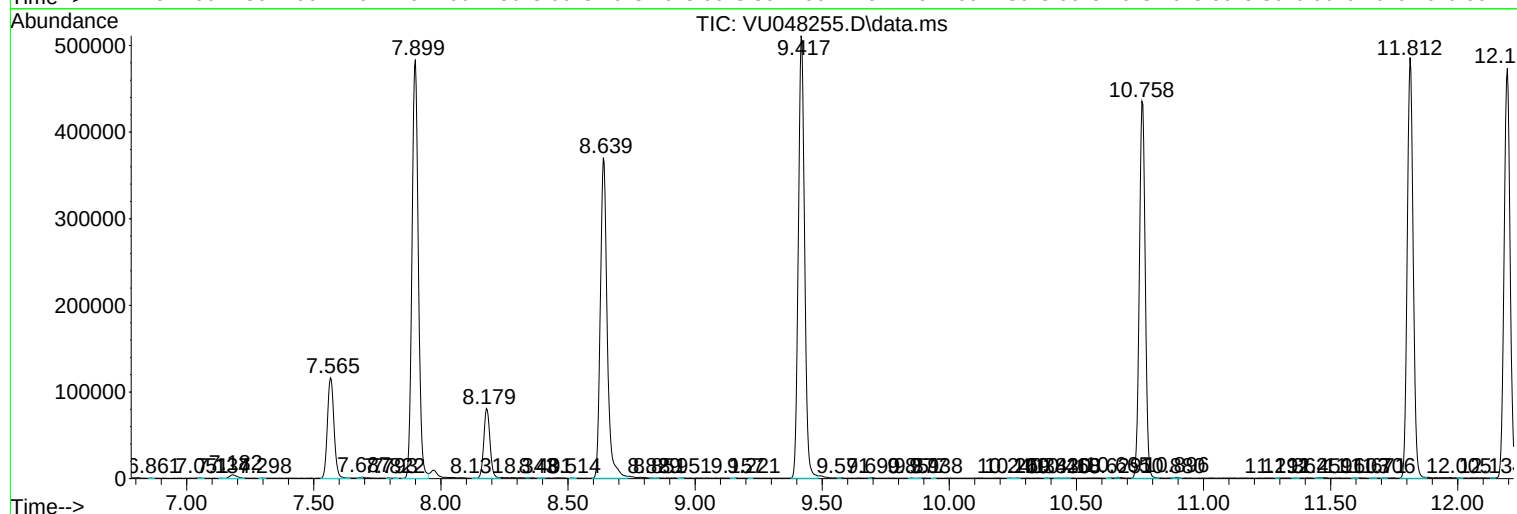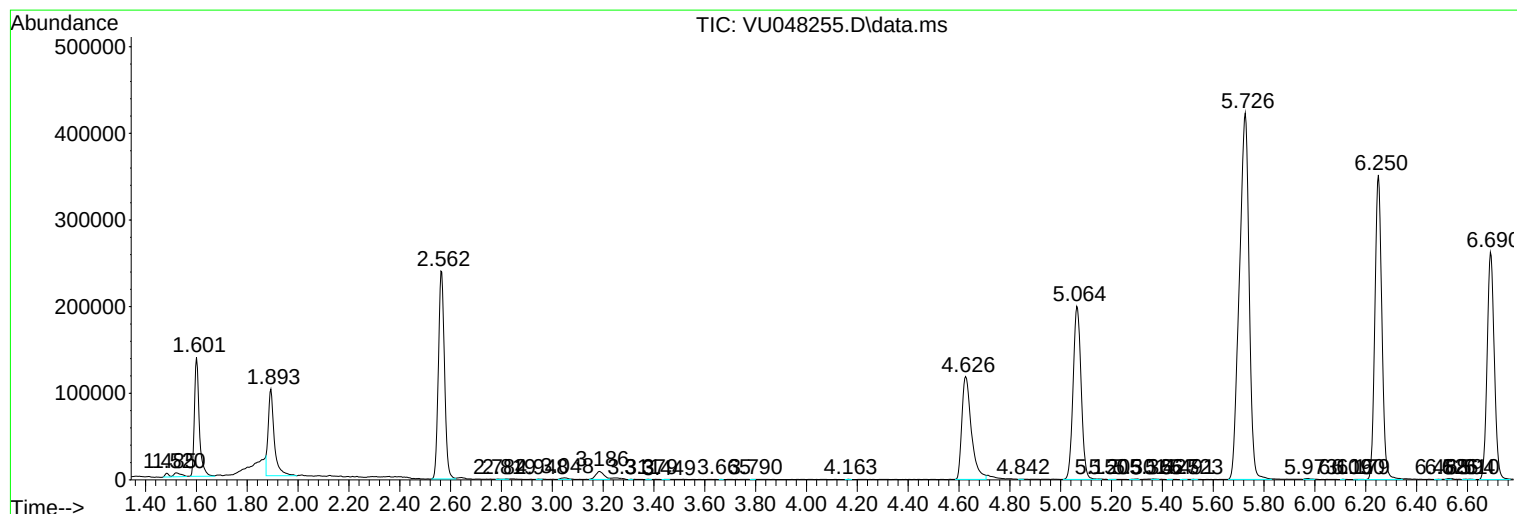

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048255.D
Acq On : 23 Apr 2022 18:48
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
Data File : VU048255.D
Acq On : 23 Apr 2022 18:48
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------