


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042322\
 Data File : VU048239.D
 Acq On : 23 Apr 2022 11:19
 Operator : SY/MD
 Sample : BFB071
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB071

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 25 01:24:32 2022

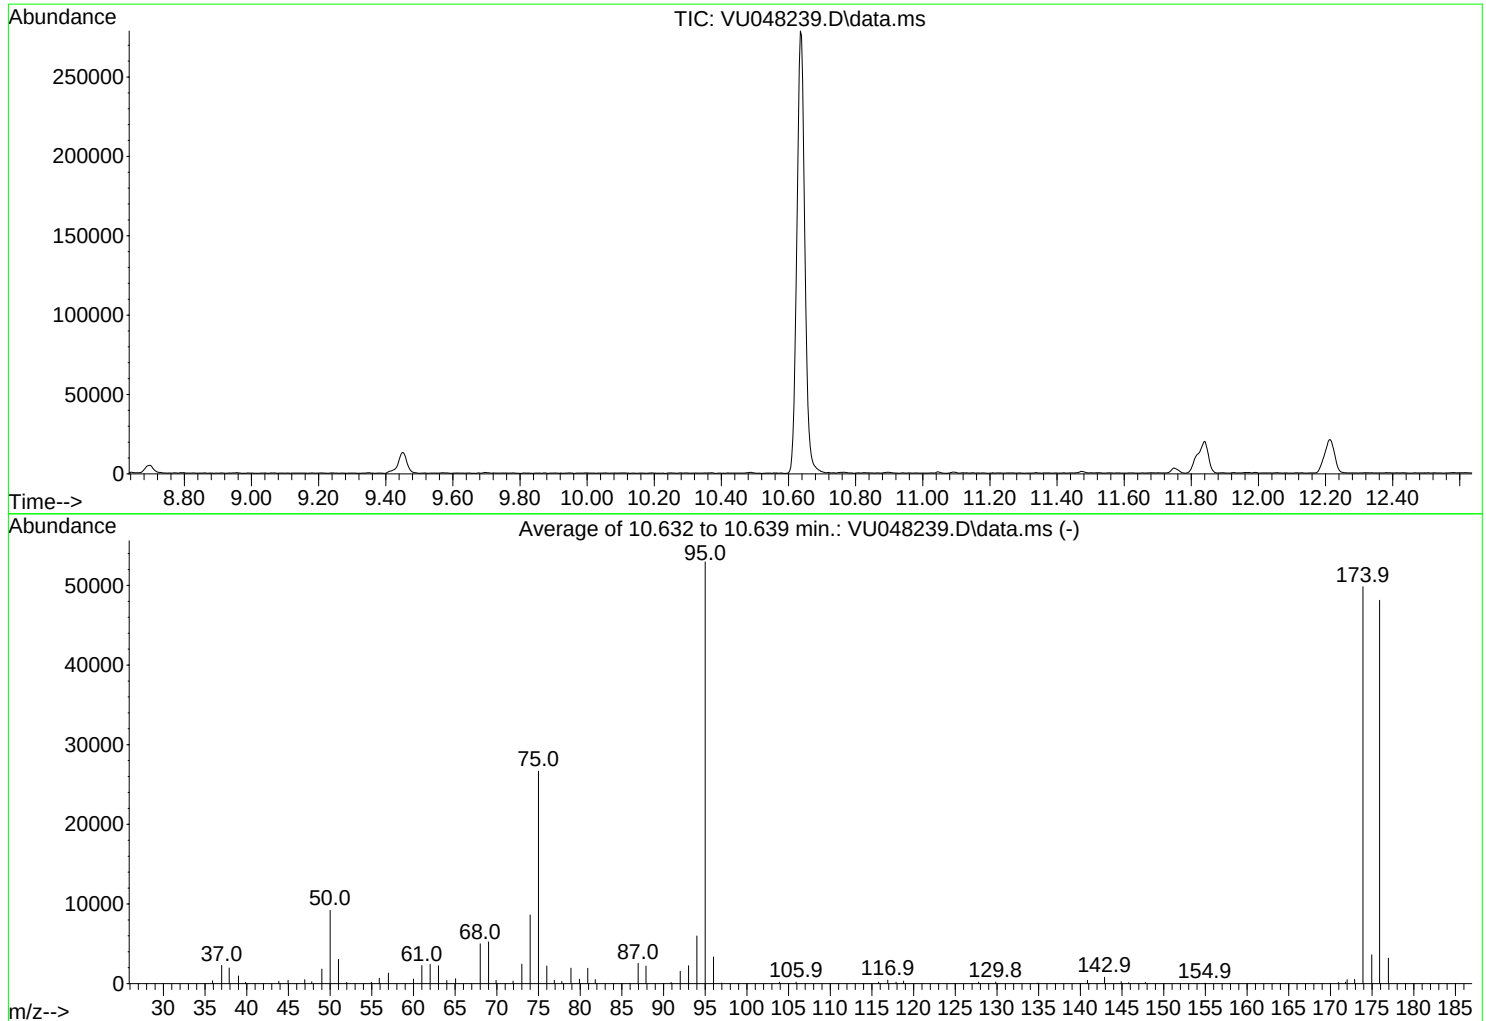

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	9202	PASS
75	95	30	80	50.4	26677	PASS
95	95	100	100	100.0	52960	PASS
96	95	5	9	6.3	3357	PASS
173	174	0.00	2	1.1	536	PASS
174	95	50	120	94.1	49835	PASS
175	174	5	9	7.2	3608	PASS
176	174	95	101	96.6	48136	PASS
177	176	5	9	6.6	3192	PASS

m/z	Abundance
43.80	399.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	411.0
37.00	2182.0
37.90	1911.0
39.00	996.0
39.90	138.0
43.90	608.0
44.90	388.0
46.90	503.0
47.80	224.0
49.00	1843.0
50.00	8789.0
51.00	2989.0
52.00	202.0
54.90	167.0
55.90	611.0
57.00	1298.0
60.00	592.0
61.00	2268.0
62.00	2301.0
63.00	2325.0
64.00	364.0
65.00	580.0
66.90	124.0
68.00	4737.0
69.00	4944.0
69.90	430.0
71.90	305.0
73.00	2280.0
74.00	8072.0
75.00	25264.0
76.00	2072.0
76.90	408.0
77.80	222.0
78.90	1971.0
79.90	531.0
80.90	1900.0
81.80	526.0
87.00	2586.0
87.90	2081.0
90.90	155.0
92.00	1493.0
93.00	2069.0
94.00	5958.0
95.00	50928.0
96.00	3334.0
97.00	110.0
103.90	164.0
105.90	214.0
115.80	210.0
116.90	402.0
117.90	161.0
118.80	322.0
127.80	195.0
129.80	168.0
140.90	364.0
142.90	738.0
144.90	274.0
145.80	135.0
147.80	133.0
171.00	126.0
171.80	604.0
172.90	486.0
173.90	46104.0
174.90	3363.0
175.90	44736.0
176.90	3129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	376.0
37.00	2384.0
37.90	2017.0
39.00	1024.0
39.80	159.0
43.90	717.0
44.90	435.0
47.00	553.0
47.80	246.0
49.00	1872.0
50.00	9506.0
51.00	3153.0
52.00	170.0
54.90	197.0
55.90	694.0
57.00	1355.0
60.00	633.0
61.00	2309.0
62.00	2421.0
63.00	2328.0
64.00	418.0
65.10	614.0
68.00	5167.0
69.00	5419.0
69.90	423.0
71.90	302.0
73.00	2532.0
74.00	8923.0
75.00	27664.0
76.00	2301.0
76.90	453.0
77.80	306.0
78.90	2035.0
79.90	569.0
80.90	2011.0
81.80	529.0
86.90	2632.0
87.90	2237.0
90.90	177.0
92.00	1584.0
93.00	2331.0
94.00	6161.0
95.00	54544.0
96.00	3382.0
97.00	113.0
103.90	176.0
105.90	203.0
115.80	201.0
116.90	463.0
117.90	212.0
118.80	333.0
127.80	214.0
129.90	201.0
134.90	119.0
140.90	428.0
142.90	832.0
144.90	261.0
145.80	130.0
147.80	154.0
154.90	106.0
171.00	152.0
172.00	702.0
172.90	548.0
173.90	51456.0
175.00	3686.0
175.90	49696.0
176.90	3296.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	331.0
37.00	2291.0
37.90	1986.0
39.00	906.0
39.80	186.0
43.90	751.0
45.00	426.0
46.90	469.0
47.80	261.0
49.00	1770.0
50.00	9311.0
51.00	3052.0
51.90	120.0
55.00	200.0
55.90	741.0
57.00	1301.0
60.00	553.0
61.00	2232.0
62.00	2483.0
63.00	2100.0
64.00	413.0
65.10	668.0
68.00	5091.0
69.00	5355.0
69.90	421.0
72.00	351.0
73.00	2520.0
74.00	8874.0
75.00	27104.0
76.00	2281.0
76.90	397.0
77.80	303.0
78.90	1819.0
79.90	591.0
80.90	1899.0
81.80	459.0
86.00	107.0
86.90	2409.0
87.90	2306.0
90.90	182.0
92.00	1545.0
93.00	2330.0
94.00	5839.0
95.00	53408.0
96.00	3356.0
103.90	191.0
105.90	210.0
115.80	176.0
116.90	460.0
117.90	228.0
118.80	321.0
127.80	181.0
129.80	233.0
134.90	104.0
140.80	471.0
142.90	824.0
144.90	260.0
145.80	107.0
147.80	177.0
155.00	108.0
170.90	174.0
172.00	809.0
172.90	573.0
173.90	51944.0
175.00	3775.0
175.90	49976.0
177.00	3150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071