


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071420\
 Data File : VU039475.D
 Acq On : 14 Jul 2020 08:31
 Operator : SY/MD
 Sample : BFB01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 15 06:21:40 2020

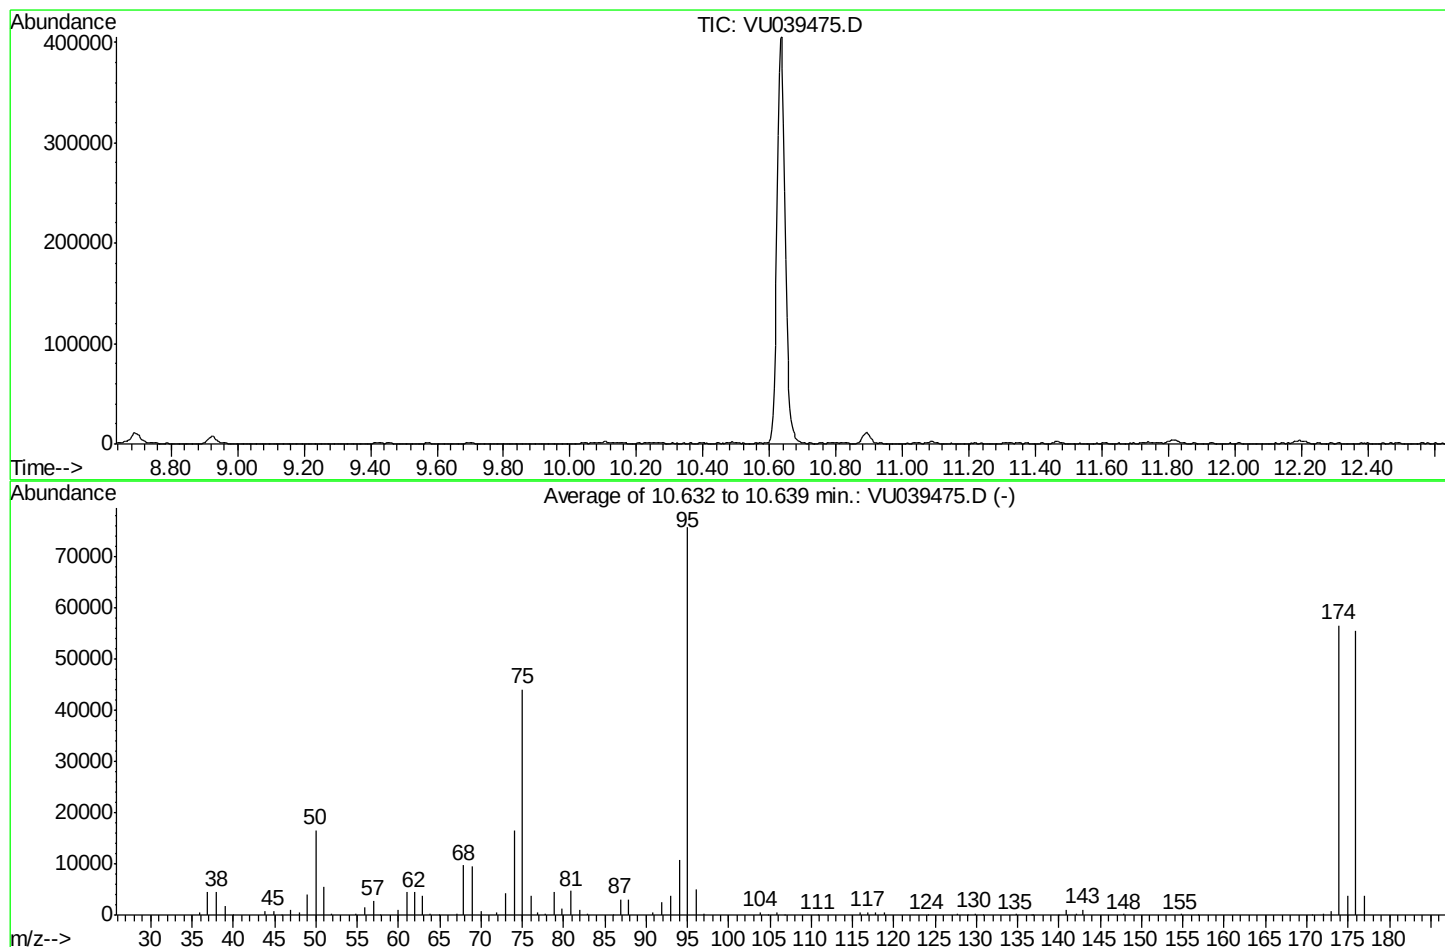

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	16544	PASS
75	95	30	80	58.3	44064	PASS
95	95	100	100	100.0	75613	PASS
96	95	5	9	6.6	5007	PASS
173	174	0.00	2	1.2	656	PASS
174	95	50	120	74.6	56432	PASS
175	174	5	9	6.8	3815	PASS
176	174	95	101	98.4	55504	PASS
177	176	5	9	6.8	3780	PASS

m/z	Abundance
35.90	938.0
36.90	4542.0
38.00	4638.0
39.00	1908.0
40.00	161.0
43.90	969.0
44.90	895.0
45.80	130.0
47.00	884.0
47.90	476.0
48.90	4310.0
50.00	17792.0
50.90	5488.0
51.90	358.0
54.90	209.0
55.90	1561.0
57.00	2895.0
57.80	102.0
59.90	864.0
61.00	4522.0
61.90	4469.0
62.90	3866.0
63.80	212.0
67.10	234.0
67.90	10112.0
69.00	10049.0
69.90	888.0
71.90	512.0
72.90	4462.0
74.00	17072.0
75.00	45616.0
76.00	4055.0
76.90	437.0
77.70	379.0
78.90	4792.0
79.80	1341.0
80.90	4781.0
81.90	1051.0
82.90	145.0
86.90	3109.0
87.90	3140.0
90.80	493.0
91.90	2563.0
93.00	3973.0
94.00	10780.0
95.00	77544.0
96.00	5286.0
97.10	159.0
103.90	615.0
104.80	114.0
105.80	574.0
110.80	110.0
115.90	385.0
116.80	609.0
117.80	450.0
118.90	633.0
124.10	115.0
127.80	269.0
128.80	116.0
129.80	268.0
130.80	147.0
134.80	121.0
136.70	122.0
136.90	123.0
140.80	966.0
142.00	145.0
142.90	1165.0
147.80	134.0
154.80	154.0
156.80	194.0
170.70	131.0
172.00	338.0
172.90	627.0
173.90	56632.0
174.90	3936.0
175.90	56080.0
176.90	3757.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
35.90	952.0
36.90	4590.0
38.00	4641.0
39.00	1809.0
40.00	172.0
43.90	1006.0
44.90	912.0
47.00	917.0
48.00	523.0
48.90	4038.0
50.00	16864.0
50.90	5615.0
51.90	339.0
54.80	221.0
55.90	1515.0
57.00	2822.0
57.80	137.0
59.90	932.0
61.00	4528.0
62.00	4589.0
62.90	3887.0
63.90	258.0
65.00	114.0
67.10	271.0
67.90	9939.0
69.00	9996.0
69.90	864.0
71.90	526.0
72.90	4389.0
74.00	16968.0
75.00	45248.0
76.00	3924.0
76.90	531.0
77.70	376.0
78.90	4741.0
79.80	1251.0
80.90	4732.0
81.90	1009.0
82.80	150.0
86.00	126.0
86.90	3157.0
87.90	3012.0
90.80	448.0
91.90	2598.0
93.00	3976.0
94.00	11099.0
95.00	77960.0
96.00	5185.0
97.00	200.0
103.90	670.0
104.70	106.0
105.80	542.0
106.70	110.0
110.80	122.0
115.90	413.0
116.90	545.0
117.80	441.0
118.80	581.0
127.70	261.0
128.80	134.0
129.80	291.0
130.80	112.0
134.80	163.0
136.90	135.0
139.90	107.0
140.80	964.0
142.10	156.0
142.90	1129.0
147.90	171.0
154.80	136.0
156.80	135.0
170.60	130.0
172.00	351.0
172.90	689.0
173.90	57912.0
174.90	3884.0
175.90	56784.0
176.90	3927.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
35.90	908.0
36.90	4370.0
37.90	4353.0
38.90	1604.0
40.00	195.0
43.90	945.0
44.90	782.0
47.00	916.0
48.00	528.0
48.90	3419.0
50.00	14976.0
50.90	5196.0
51.90	264.0
54.80	249.0
56.00	1453.0
57.00	2587.0
57.80	128.0
59.90	914.0
61.00	4323.0
61.90	4323.0
62.90	3723.0
63.90	262.0
64.90	135.0
67.10	268.0
67.90	8859.0
68.90	8777.0
70.00	749.0
71.90	464.0
72.90	3920.0
74.00	15134.0
75.00	41328.0
76.00	3528.0
76.90	502.0
77.80	341.0
78.90	4275.0
79.80	999.0
80.90	4490.0
81.90	937.0
82.80	175.0
85.90	159.0
86.90	2861.0
87.90	2609.0
90.90	398.0
91.90	2470.0
93.00	3613.0
94.00	10572.0
95.00	71336.0
96.00	4551.0
97.00	178.0
103.80	592.0
104.70	123.0
105.80	475.0
106.70	110.0
110.80	101.0
115.90	378.0
116.90	555.0
117.80	415.0
118.80	450.0
127.70	278.0
128.90	119.0
129.80	297.0
134.80	174.0
136.70	114.0
140.00	114.0
140.80	862.0
142.00	178.0
142.90	1011.0
147.90	182.0
154.80	125.0
170.60	120.0
171.90	332.0
172.90	654.0
173.90	54752.0
174.90	3627.0
175.90	53648.0
176.90	3656.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
35.90	312.0
39.90	127.0
44.00	337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01