

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
Data File : VU039599.D
Acq On : 21 Jul 2020 16:10
Operator : SY/MD
Sample : L3348-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAXZ0

Manual Integrations
APPROVED

MMDadoda
7/27/2020 8:10:09 AM

Quant Time: Jul 22 02:05:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 22 02:01:33 2020
Response via : Initial Calibration

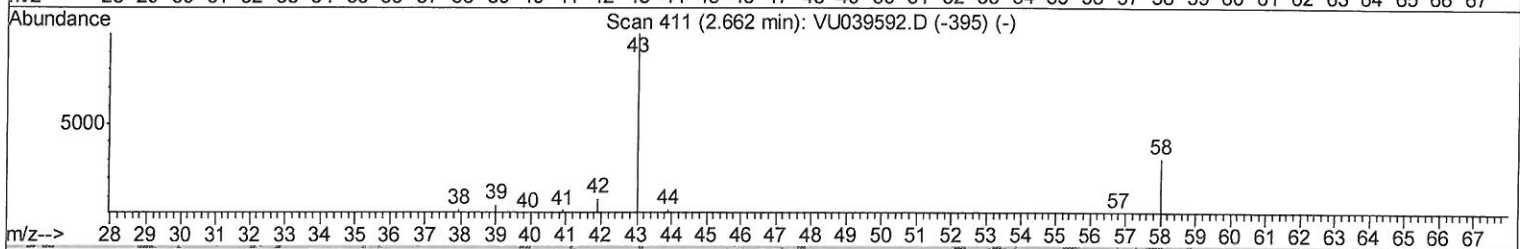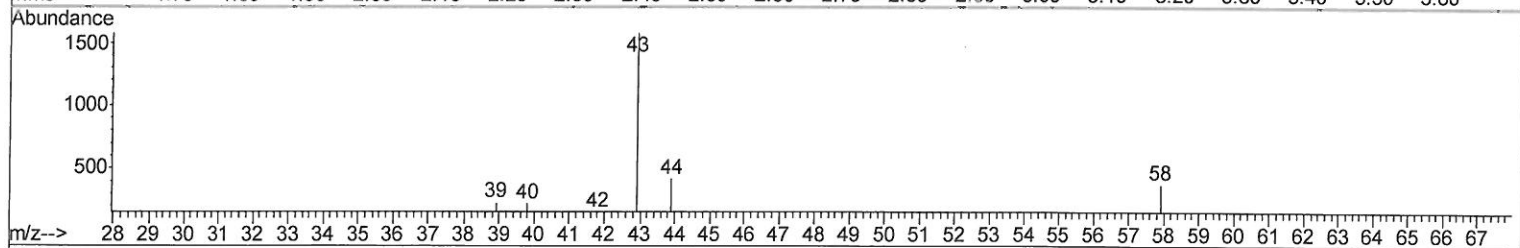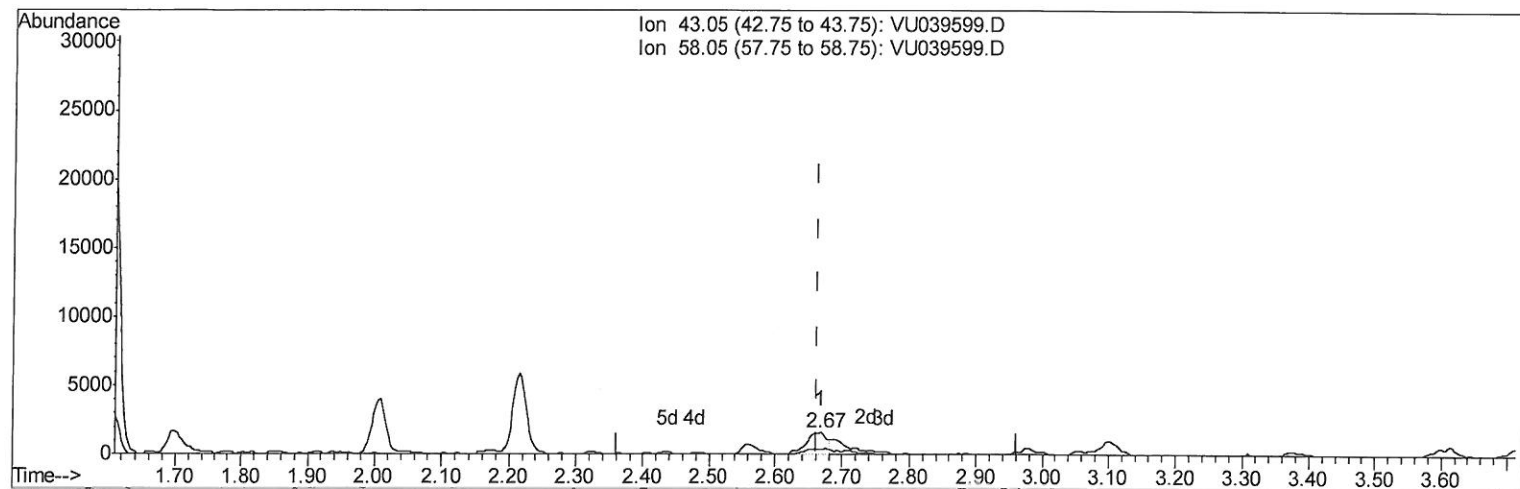

TIC: VU039599.D

(13) Acetone (T)

2.668min (+0.006) 2.43ug/L

response 3362

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	11.18
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
Data File : VU039599.D
Acq On : 21 Jul 2020 16:10
Operator : SY/MD
Sample : L3348-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAXZ0

Manual Integrations
APPROVED

MMDadoda
7/27/2020 8:10:09 AM

Quant Time: Jul 22 02:05:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 22 02:01:33 2020
Response via : Initial Calibration

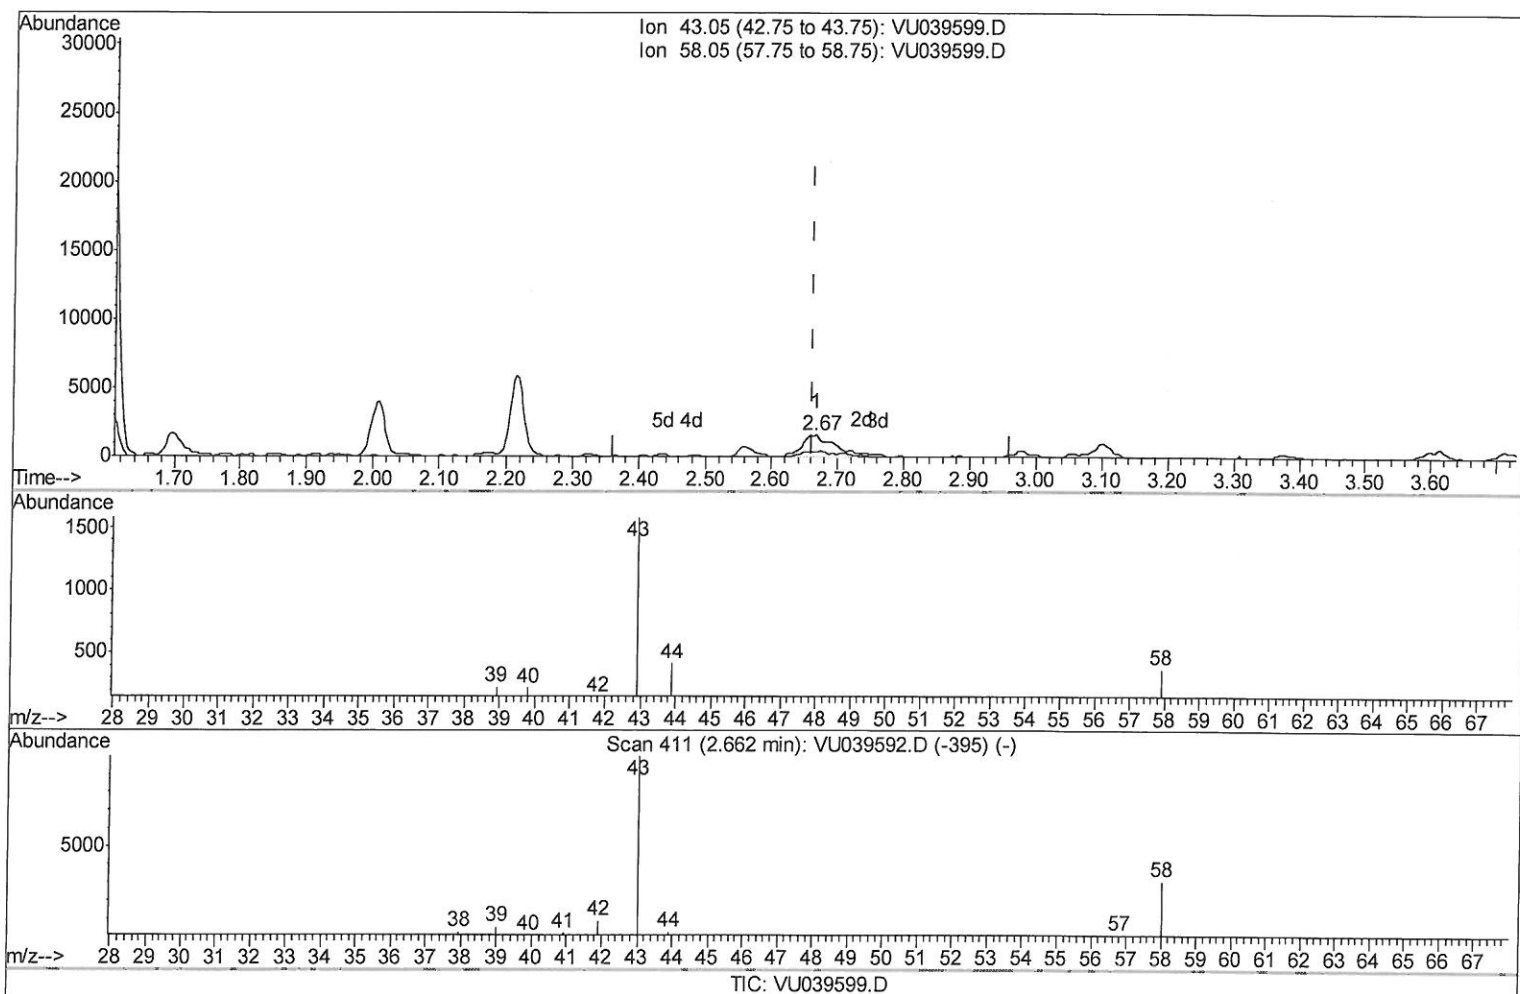

(13) Acetone (T)

2.668min (+0.006) 3.78ug/L m

> 0.7/28/2024

response 5227

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	7.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
 Data File : VU039599.D
 Acq On : 21 Jul 2020 16:10
 Operator : SY/MD
 Sample : L3348-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAXZ0

Manual Integrations
 APPROVED

MMDadoda
 7/27/2020 8:10:09 AM

Quant Time: Jul 22 02:53:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 22 02:01:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	118806	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	113230	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	52864	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	35722	6.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 129.60%	
7) Chloroethane-d5	1.93	69	34789	5.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 115.60%	
11) 1,1-Dichloroethene-d2	2.58	63	58390	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 94.20%	
20) 2-Butanone-d5	4.66	46	133147	53.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	= 107.06%	
24) Chloroform-d	5.09	84	73893	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 105.60%	
26) 1,2-Dichloroethane-d4	5.72	65	48120	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 104.20%	
32) Benzene-d6	5.75	84	147737	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 108.60%	
36) 1,2-Dichloropropane-d6	6.70	67	47774	5.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 106.60%	
41) Toluene-d8	7.91	98	133010	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 103.20%	
43) trans-1,3-Dichloropropene-	8.19	79	18740	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 96.20%	
46) 2-Hexanone-d5	8.64	63	97750	51.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 102.64%	
57) 1,1,2,2-Tetrachloroethane-	10.76	84	40329	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 97.00%	
64) 1,2-Dichlorobenzene-d4	12.19	152	49067	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 103.20%	

Target Compounds

					Ovalue
13) Acetone	2.67	43	5227m	3.776	ug/L
14) Carbon disulfide	2.81	76	5865	0.347	ug/L
42) Toluene	7.98	91	7300	0.245	ug/L
52) Ethylbenzene	9.57	91	2394	0.071	ug/L
53) m,p-Xylene	9.69	106	1854	0.147	ug/L
54) o-Xylene	10.10	106	768	0.062	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
Data File : VU039599.D
Acq On : 21 Jul 2020 16:10
Operator : SY/MD
Sample : L3348-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAXZ0

Manual Integrations
APPROVED

MMDadoda
7/27/2020 8:10:09 AM

Quant Time: Jul 22 02:53:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 22 02:01:33 2020
Response via : Initial Calibration

