

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
Data File : VU039612.D
Acq On : 21 Jul 2020 21:10
Operator : SY/MD
Sample : L3347-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAY00

Manual Integrations
APPROVED

MMDadoda
7/27/2020 8:10:14 AM

Quant Time: Jul 22 02:08:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 22 02:01:33 2020
Response via : Initial Calibration

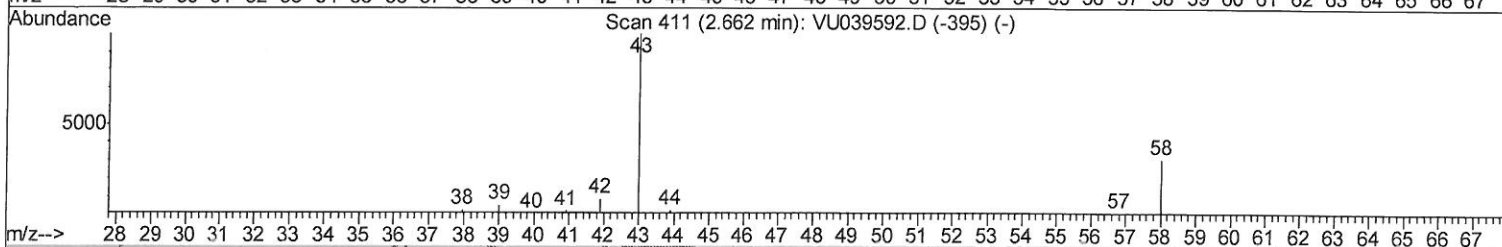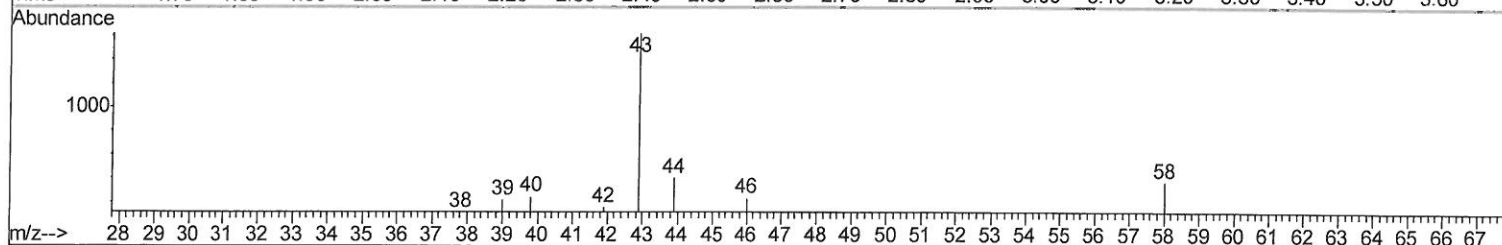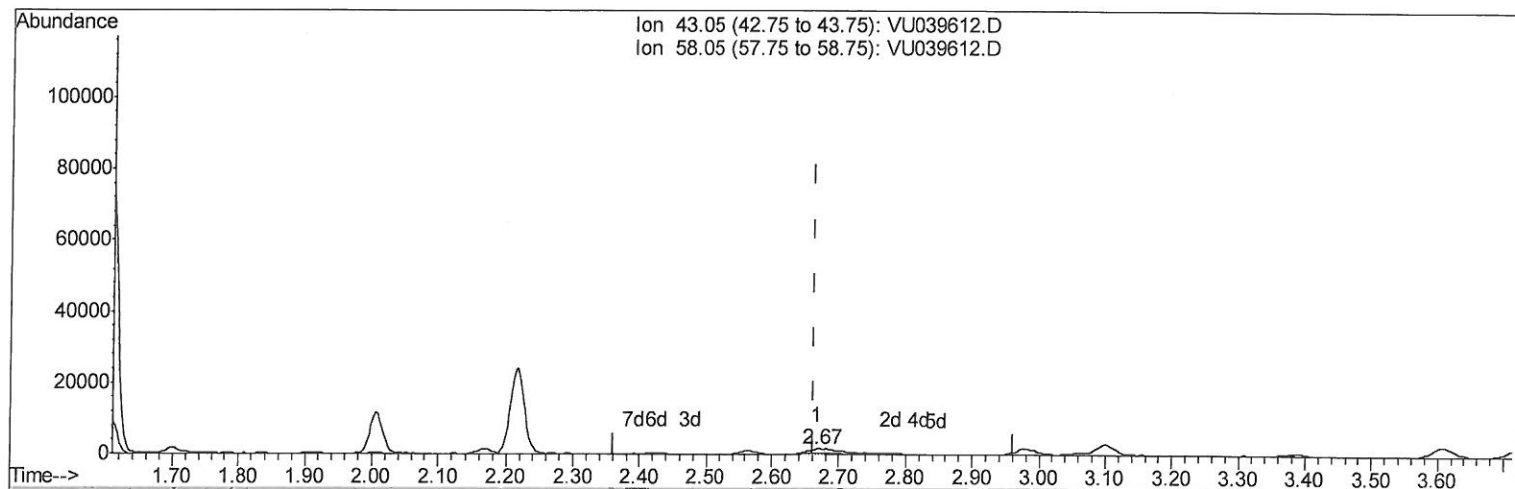

TIC: VU039612.D

(13) Acetone (T)

2.668min (+0.006) 2.08ug/L

response 2763

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	17.77
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
 Data File : VU039612.D
 Acq On : 21 Jul 2020 21:10
 Operator : SY/MD
 Sample : L3347-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAY00

Manual Integrations
 APPROVED

MMDadoda
 7/27/2020 8:10:14 AM

Quant Time: Jul 22 02:08:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 22 02:01:33 2020
 Response via : Initial Calibration

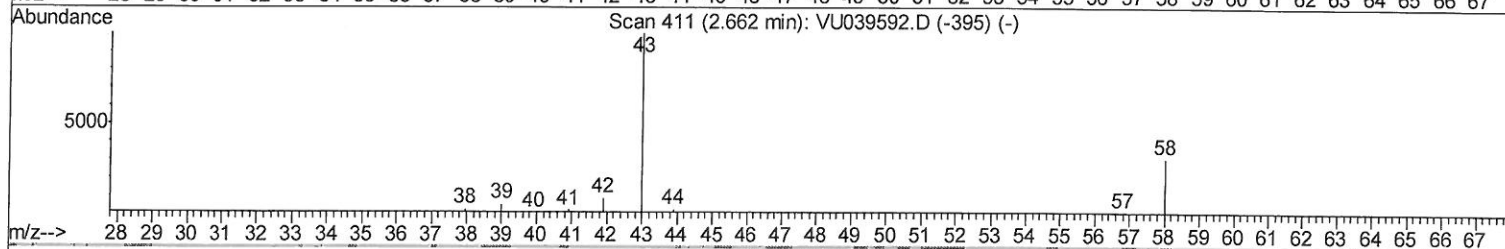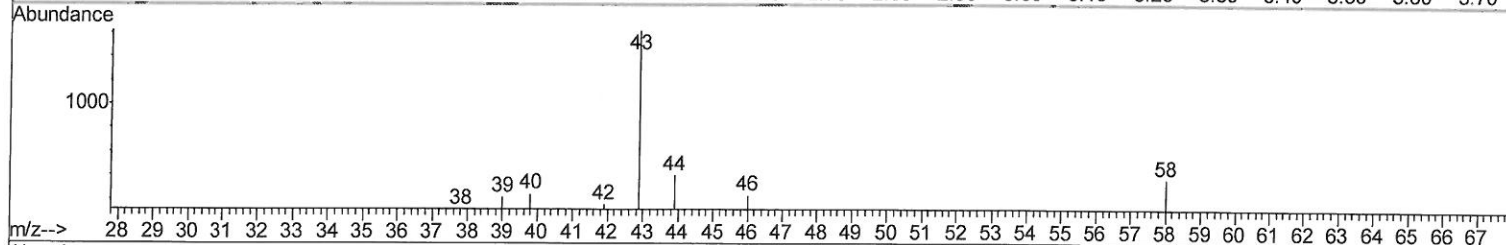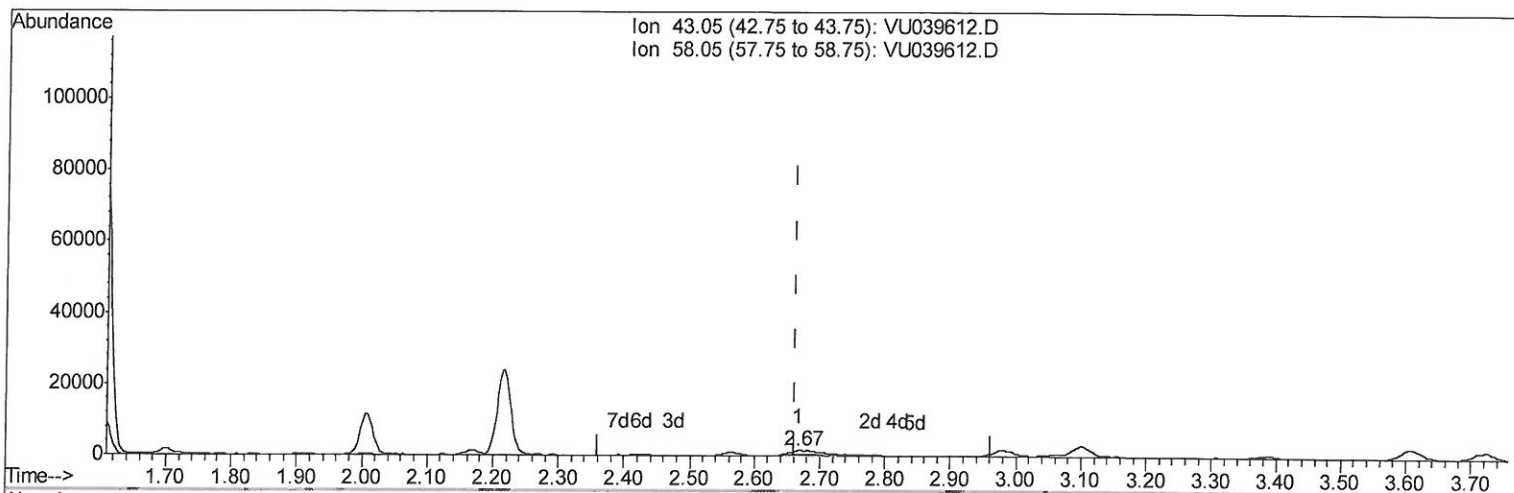

TIC: VU039612.D

(13) Acetone (T)

2.668min (+0.006) 4.98ug/L m

207/28/20 by

response 6602

Ion	Exp%	Act%
43.05	100	100
58.05	29.50	7.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
 Data File : VU039612.D
 Acq On : 21 Jul 2020 21:10
 Operator : SY/MD
 Sample : L3347-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 GAY00

Manual Integrations
 APPROVED

MMDadoda
 7/27/2020 8:10:14 AM

Quant Time: Jul 22 03:46:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 22 02:01:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	113826	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	106427	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47254	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.61	65	31583	5.98	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 119.60%			
7) Chloroethane-d5	1.93	69	27807	4.82	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 96.40%			
11) 1,1-Dichloroethene-d2	2.58	63	47886	4.03	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 80.60%			
20) 2-Butanone-d5	4.66	46	117284	49.21	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 98.42%			
24) Chloroform-d	5.09	84	63493	4.74	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 94.80%			
26) 1,2-Dichloroethane-d4	5.72	65	42174	4.77	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 95.40%			
32) Benzene-d6	5.75	84	125751	4.91	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 98.20%			
36) 1,2-Dichloropropane-d6	6.71	67	40925	4.86	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 97.20%			
41) Toluene-d8	7.91	98	111511	4.60	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 92.00%			
43) trans-1,3-Dichloropropene-	8.19	79	15551	4.25	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 85.00%			
46) 2-Hexanone-d5	8.64	63	82528	46.10	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 92.20%			
57) 1,1,2,2-Tetrachloroethane-	10.76	84	34473	4.41	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 88.20%			
64) 1,2-Dichlorobenzene-d4	12.19	152	41482	4.88	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 97.60%			
Target Compounds						
13) Acetone	2.67	43	6602m	4.978	ug/L	Ovalue 97
14) Carbon disulfide	2.81	76	3945	0.244	ug/L	97
16) Methylene chloride	3.06	84	1360	0.175	ug/L	93
25) Chloroform	5.11	83	3980	0.285	ug/L	83
33) Benzene	5.79	78	6054	0.237	ug/L	100
35) Methylcyclohexane	6.78	83	1541	0.149	ug/L	# 85
42) Toluene	7.98	91	11833	0.423	ug/L	99
52) Ethylbenzene	9.57	91	3814	0.120	ug/L	88
53) m,p-Xylene	9.70	106	2205	0.186	ug/L	91
54) o-Xylene	10.10	106	1735	0.150	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072120\
Data File : VU039612.D
Acq On : 21 Jul 2020 21:10
Operator : SY/MD
Sample : L3347-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAY00

Manual Integrations
APPROVED

MMDadoda
7/27/2020 8:10:14 AM

Quant Time: Jul 22 03:46:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 22 02:01:33 2020
Response via : Initial Calibration

