




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050684.D
Acq On : 08 Sep 2022 14:37
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Manual IntegrationsAPPROVED

Quant Time: Sep 08 22:55:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 08 22:51:50 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/09/2022
Supervised By :Mahesh Dadoda 09/09/2022

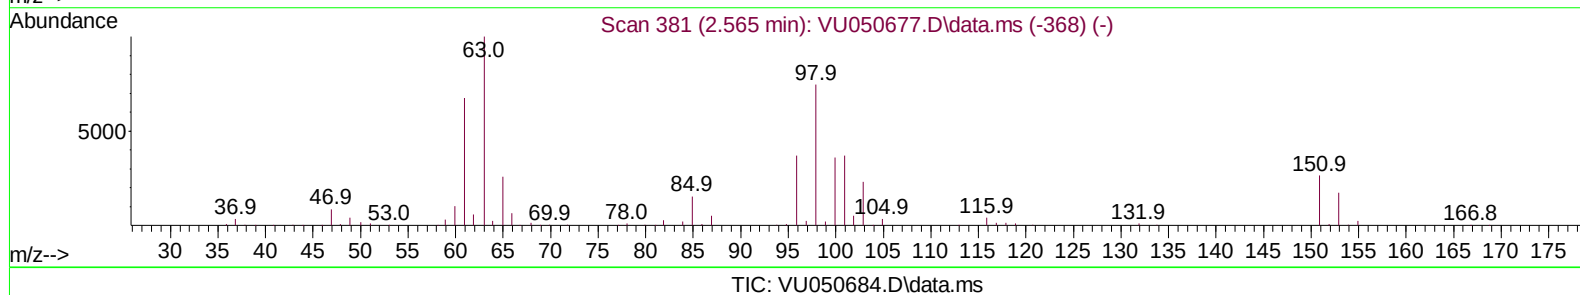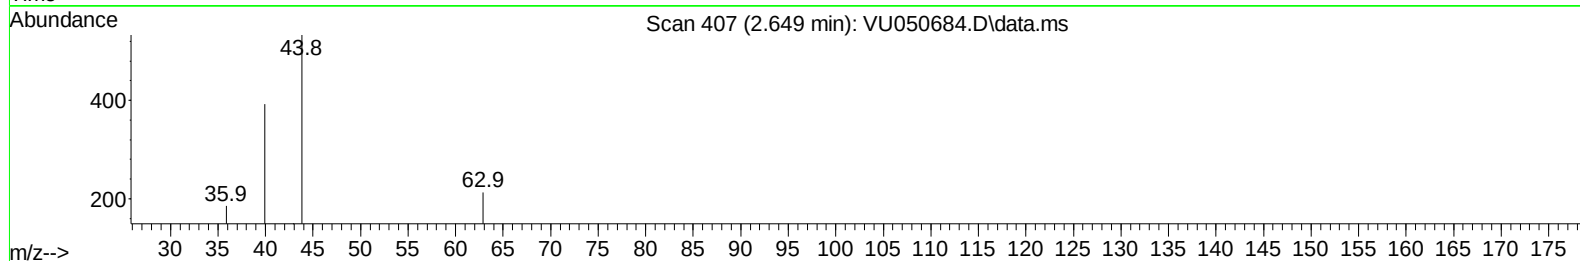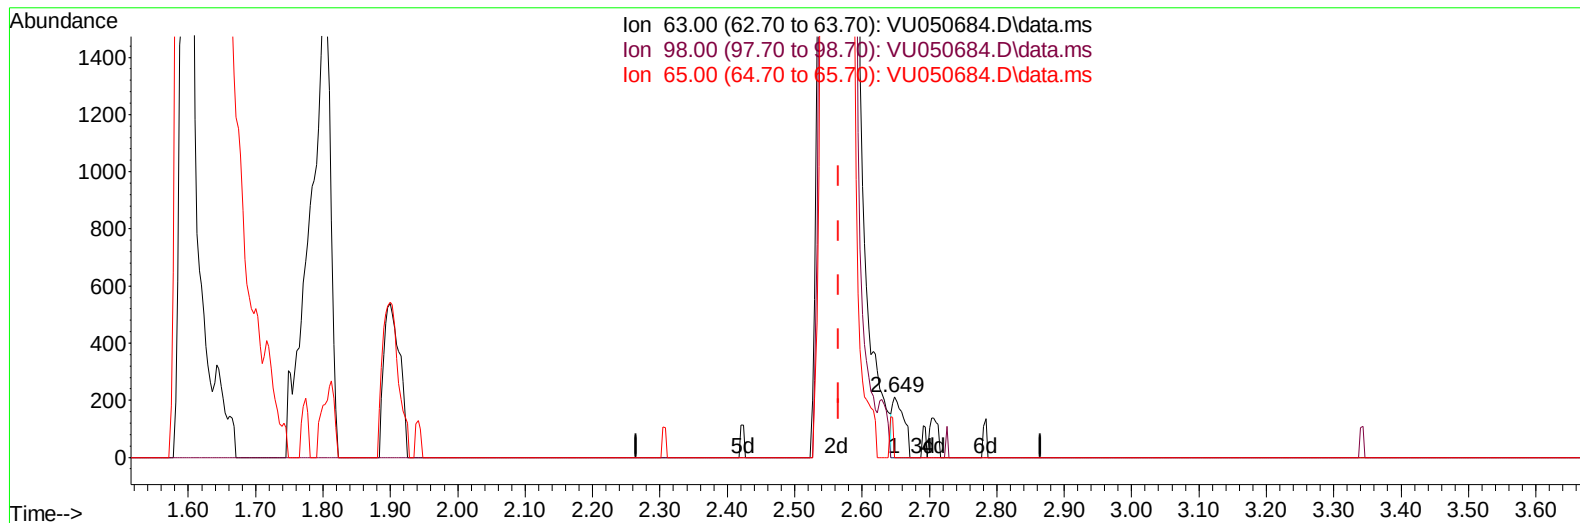

(11) 1,1-Dichloroethene-d2 (S)

2.649min (+ 0.084) 0.06 ug/L

response 250

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.80	67.20
65.00	23.80	21.60
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050684.D
 Acq On : 08 Sep 2022 14:37
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Manual IntegrationsAPPROVED

Quant Time: Sep 08 22:55:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 08 22:51:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/09/2022
 Supervised By :Mahesh Dadoda 09/09/2022

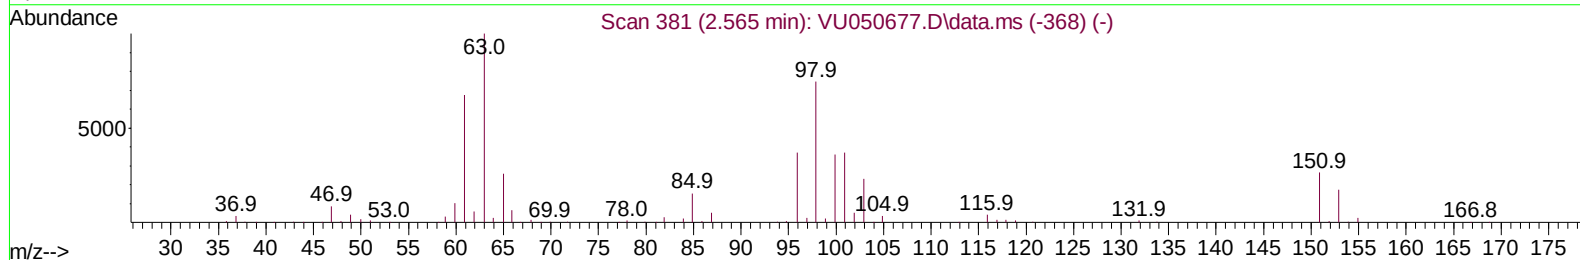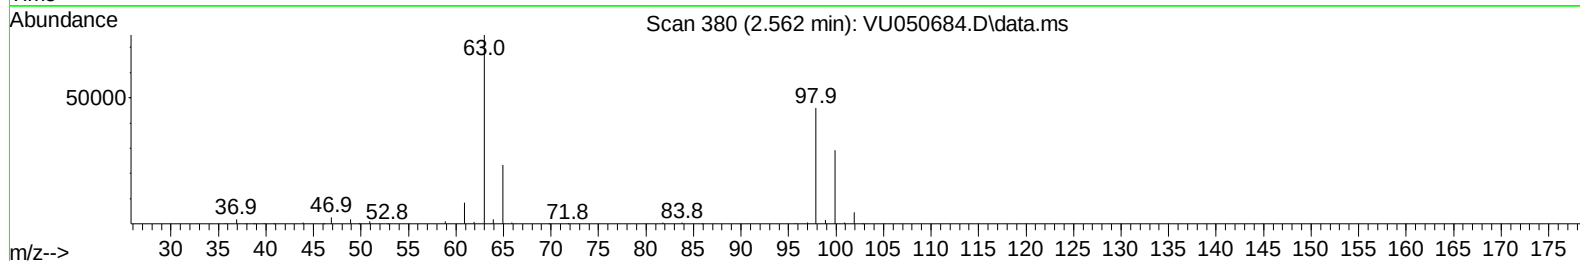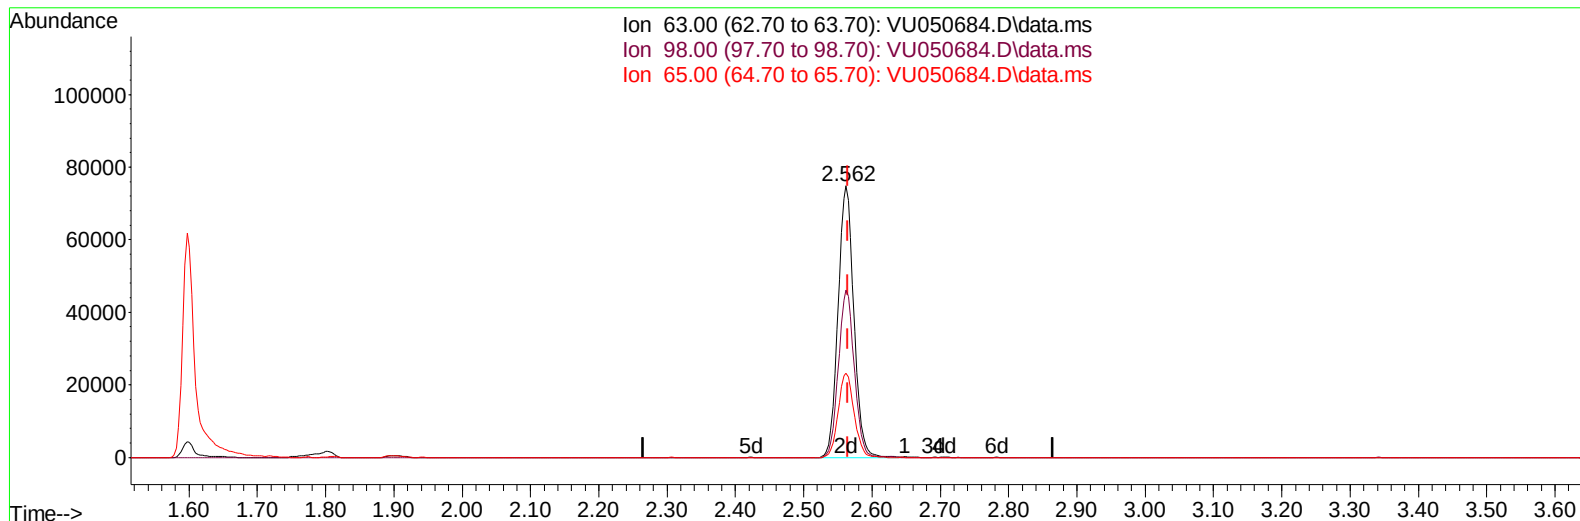

TIC: VU050684.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.562min (-0.003) 28.68 ug/L m

response 119914

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.80	0.14#
65.00	23.80	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050684.D
 Acq On : 08 Sep 2022 14:37
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Manual IntegrationsAPPROVED

Quant Time: Sep 08 22:55:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 08 22:51:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/09/2022
 Supervised By :Mahesh Dadoda 09/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	276611	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	278414	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	105907	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	81617	34.497	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	69.000%	
7) Chloroethane-d5	1.900	69	68122	42.579	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	85.160%	
11) 1,1-Dichloroethene-d2	2.562	63	119914m	28.682	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	57.360%#	
21) 2-Butanone-d5	4.620	46	180872	104.493	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	104.490%	
24) Chloroform-d	5.063	84	222696	49.665	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.320%	
26) 1,2-Dichloroethane-d4	5.700	65	146865	53.599	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.200%	
32) Benzene-d6	5.726	84	431303	46.877	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.760%	
36) 1,2-Dichloropropane-d6	6.690	67	144709	47.905	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	95.800%	
41) Toluene-d8	7.899	98	342854	43.576	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.160%	
43) trans-1,3-Dichloroprop...	8.179	79	61548	49.244	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	98.480%	
47) 2-Hexanone-d5	8.632	63	75615	99.515	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	99.510%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	236233	51.678	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	103.360%	
66) 1,2-Dichlorobenzene-d4	12.192	152	127268	51.334	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	102.660%	
Target Compounds						
16) Methylene chloride	3.041	84	3371	1.223	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050684.D
Acq On : 08 Sep 2022 14:37
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Manual IntegrationsAPPROVED

Quant Time: Sep 08 22:55:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 08 22:51:50 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/09/2022
Supervised By :Mahesh Dadoda 09/09/2022

