

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050679.D
 Acq On : 08 Sep 2022 12:07
 Operator : SY/MD
 Sample : VU0908WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	108	rBV	127026	166125	12.45%	1.769%
2	1.800	126	143	150	rVB9	8930	16495	1.24%	0.176%
3	1.906	166	176	200	rVB	100996	142586	10.69%	1.518%
4	2.144	248	250	256	rBV4	532	371	0.03%	0.004%
5	2.192	260	265	269	rBV2	723	755	0.06%	0.008%
6	2.257	281	285	287	rVB2	518	302	0.02%	0.003%
7	2.276	289	291	295	rVB2	413	279	0.02%	0.003%
8	2.295	295	297	303	rVB4	437	441	0.03%	0.005%
9	2.363	314	318	319	rBV2	415	301	0.02%	0.003%
10	2.565	365	381	398	rBV	263523	432503	32.42%	4.605%
11	2.691	416	420	421	rBV2	449	312	0.02%	0.003%
12	2.784	444	449	451	rBV	729	640	0.05%	0.007%
13	2.941	495	498	506	rBV	275	246	0.02%	0.003%
14	3.044	521	530	539	rVB3	2700	4811	0.36%	0.051%
15	3.121	549	554	558	rBV	418	472	0.04%	0.005%
16	3.179	563	572	573	rBV2	1307	1360	0.10%	0.014%
17	3.250	590	594	598	rBV2	311	339	0.03%	0.004%
18	3.388	632	637	640	rBV2	310	286	0.02%	0.003%
19	3.536	681	683	689	rVB2	436	298	0.02%	0.003%
20	3.662	716	722	727	rBV2	244	333	0.02%	0.004%
21	3.687	727	730	737	rVB2	232	232	0.02%	0.002%
22	3.748	746	749	757	rVV2	334	333	0.02%	0.004%
23	3.877	786	789	793	rBV	268	232	0.02%	0.002%
24	3.916	794	801	805	rBV2	207	296	0.02%	0.003%
25	4.160	874	877	881	rVB	317	237	0.02%	0.003%
26	4.199	885	889	896	rVB2	265	325	0.02%	0.003%
27	4.250	896	905	908	rBV2	240	300	0.02%	0.003%
28	4.398	946	951	956	rBV2	306	352	0.03%	0.004%
29	4.620	1004	1020	1054	rBV	116920	329152	24.68%	3.504%
30	4.800	1073	1076	1081	rVB4	603	458	0.03%	0.005%
31	5.060	1140	1157	1182	rBV	247391	552014	41.38%	5.877%
32	5.292	1221	1229	1234	rBV5	864	1395	0.10%	0.015%
33	5.375	1250	1255	1259	rVB3	704	753	0.06%	0.008%
34	5.514	1293	1298	1300	rBV2	489	351	0.03%	0.004%
35	5.723	1341	1363	1394	rBV2	486882	1333888	100.00%	14.201%
36	5.925	1420	1426	1431	rBV3	613	648	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050679.D
 Acq On : 08 Sep 2022 12:07
 Operator : SY/MD
 Sample : VU0908WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.018	1449	1455	1459	rBV3	360	513	0.04%	0.005%
38	6.109	1480	1483	1489	rVB3	516	535	0.04%	0.006%
39	6.247	1512	1526	1561	rBV	379561	744308	55.80%	7.924%
40	6.533	1604	1615	1624	rBV3	2566	4324	0.32%	0.046%
41	6.600	1633	1636	1642	rVB4	645	579	0.04%	0.006%
42	6.690	1650	1664	1692	rBV	312801	613425	45.99%	6.531%
43	7.044	1769	1774	1780	rBV2	267	282	0.02%	0.003%
44	7.179	1809	1816	1818	rBV4	652	639	0.05%	0.007%
45	7.382	1874	1879	1882	rBV	362	299	0.02%	0.003%
46	7.565	1922	1936	1965	rBV	153318	274948	20.61%	2.927%
47	7.697	1973	1977	1983	rVV3	721	746	0.06%	0.008%
48	7.723	1983	1985	1988	rVB2	486	255	0.02%	0.003%
49	7.797	2001	2008	2013	rBV3	931	1152	0.09%	0.012%
50	7.896	2025	2039	2063	rBV	546854	986277	73.94%	10.501%
51	8.179	2114	2127	2150	rBV	106977	181887	13.64%	1.936%
52	8.526	2232	2235	2239	rVV2	415	253	0.02%	0.003%
53	8.636	2256	2269	2278	rBV3	204968	452673	33.94%	4.819%
54	8.825	2325	2328	2333	rVB5	711	525	0.04%	0.006%
55	8.909	2350	2354	2357	rBV3	289	232	0.02%	0.002%
56	9.121	2417	2420	2424	rVB	517	294	0.02%	0.003%
57	9.221	2446	2451	2455	rBV2	261	300	0.02%	0.003%
58	9.346	2486	2490	2493	rBV2	291	271	0.02%	0.003%
59	9.417	2499	2512	2540	rBV	530040	897528	67.29%	9.556%
60	9.604	2567	2570	2574	rVB3	309	251	0.02%	0.003%
61	9.687	2590	2596	2597	rBV	454	371	0.03%	0.004%
62	10.112	2721	2728	2729	rBV3	470	492	0.04%	0.005%
63	10.224	2758	2763	2769	rBV2	217	276	0.02%	0.003%
64	10.485	2839	2844	2846	rBV2	558	452	0.03%	0.005%
65	10.642	2890	2893	2897	rVB3	503	333	0.02%	0.004%
66	10.755	2916	2928	2949	rBV	459655	758300	56.85%	8.073%
67	10.848	2954	2957	2960	rVV	384	297	0.02%	0.003%
68	10.915	2974	2978	2981	rVB2	381	264	0.02%	0.003%
69	11.012	3005	3008	3012	rVB	495	367	0.03%	0.004%
70	11.034	3012	3015	3018	rBV2	475	342	0.03%	0.004%
71	11.092	3028	3033	3036	rBV2	478	509	0.04%	0.005%
72	11.163	3051	3055	3061	rBV2	314	400	0.03%	0.004%
73	11.298	3095	3097	3105	rVB	301	313	0.02%	0.003%
74	11.472	3148	3151	3153	rBV2	313	252	0.02%	0.003%
75	11.748	3232	3237	3244	rVB2	1036	964	0.07%	0.010%
76	11.812	3244	3257	3280	rBV	397725	665853	49.92%	7.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050679.D
 Acq On : 08 Sep 2022 12:07
 Operator : SY/MD
 Sample : VU0908WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.957	3300	3302	3304	rVB2	584	256	0.02%	0.003%
78	11.973	3304	3307	3310	rBV2	359	232	0.02%	0.002%
79	12.028	3319	3324	3327	rBV	246	264	0.02%	0.003%
80	12.192	3362	3375	3398	rBV	474284	786647	58.97%	8.375%
81	12.308	3409	3411	3415	rVB3	685	444	0.03%	0.005%
82	12.356	3422	3426	3430	rVB5	671	621	0.05%	0.007%
83	12.452	3451	3456	3459	rBV3	410	321	0.02%	0.003%
84	12.478	3461	3464	3467	rVB2	371	247	0.02%	0.003%
85	12.668	3520	3523	3528	rBV2	395	407	0.03%	0.004%
86	12.722	3538	3540	3544	rVB2	408	277	0.02%	0.003%
87	13.015	3629	3631	3641	rBV2	384	532	0.04%	0.006%
88	13.160	3673	3676	3678	rBV2	342	249	0.02%	0.003%
89	13.224	3690	3696	3699	rBV4	1228	1349	0.10%	0.014%
90	13.716	3845	3849	3853	rBV3	605	653	0.05%	0.007%
91	13.764	3860	3864	3867	rVV3	303	228	0.02%	0.002%
92	13.800	3871	3875	3877	rBV3	335	277	0.02%	0.003%
93	13.845	3883	3889	3891	rBV3	2354	2425	0.18%	0.026%
94	14.095	3961	3967	3978	rBV4	4310	7590	0.57%	0.081%
95	14.333	4034	4041	4054	rBV6	3007	5178	0.39%	0.055%
96	14.777	4177	4179	4181	rVB	530	242	0.02%	0.003%
97	14.909	4217	4220	4221	rBV2	499	304	0.02%	0.003%
98	14.980	4238	4242	4245	rVB4	598	494	0.04%	0.005%
99	15.410	4373	4376	4379	rBV3	777	458	0.03%	0.005%
100	15.854	4512	4514	4516	rBV2	784	421	0.03%	0.004%




Sum of corrected areas: 9392618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050679.D
Acq On : 08 Sep 2022 12:07
Operator : SY/MD
Sample : VU0908WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

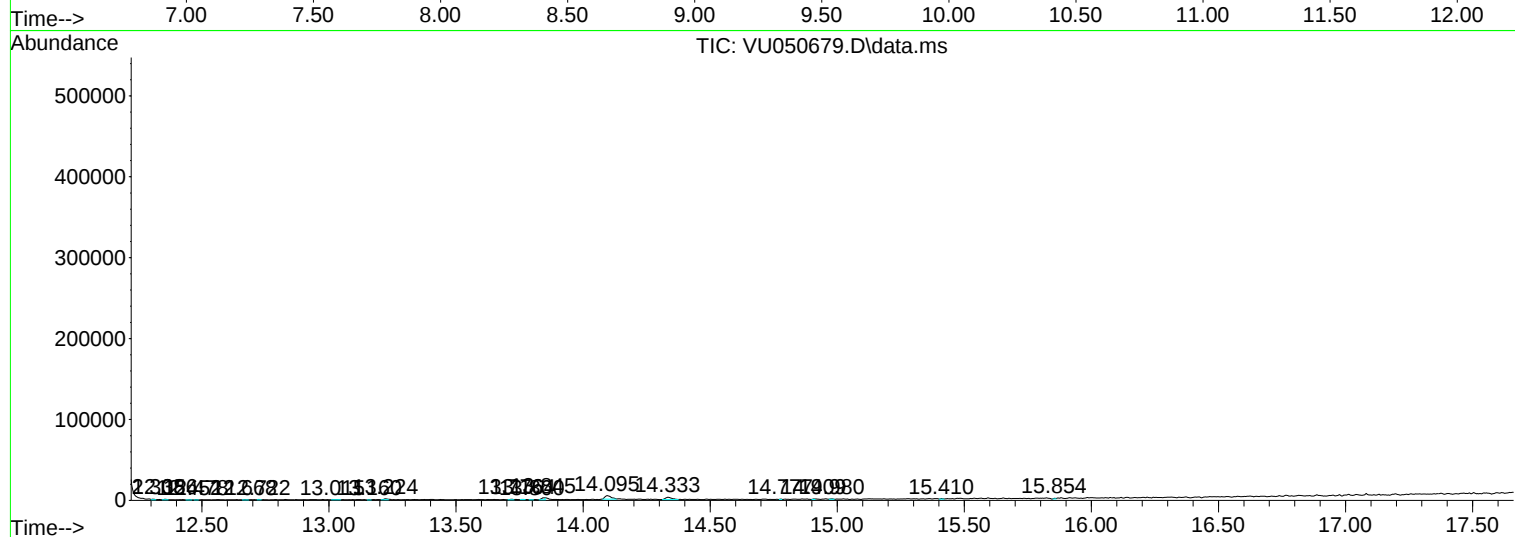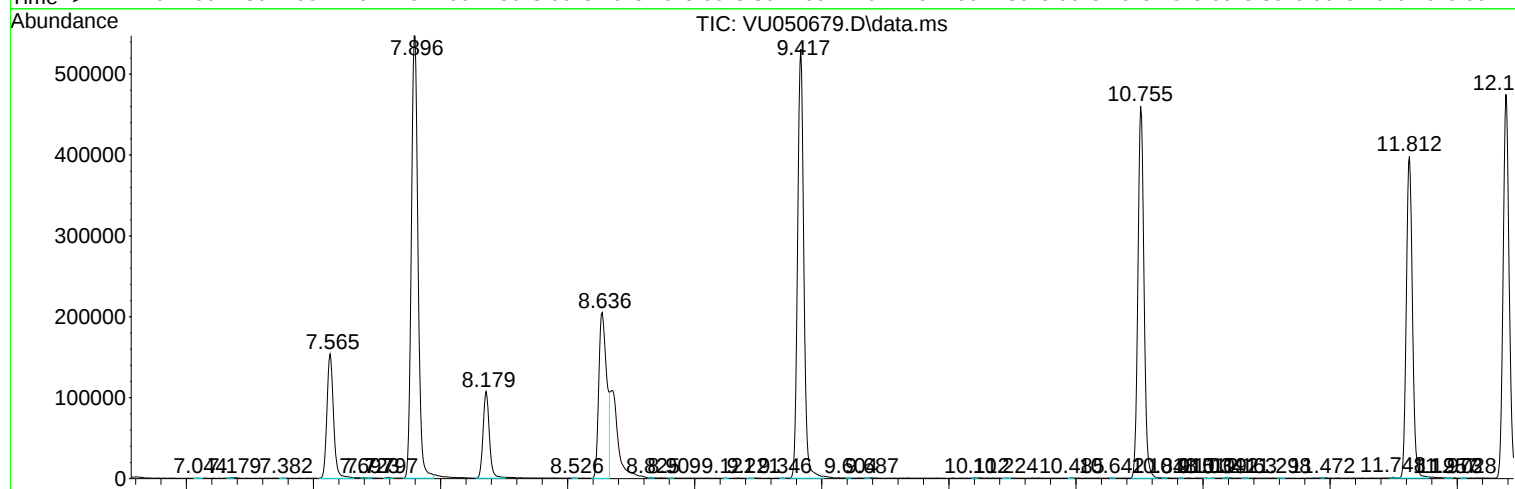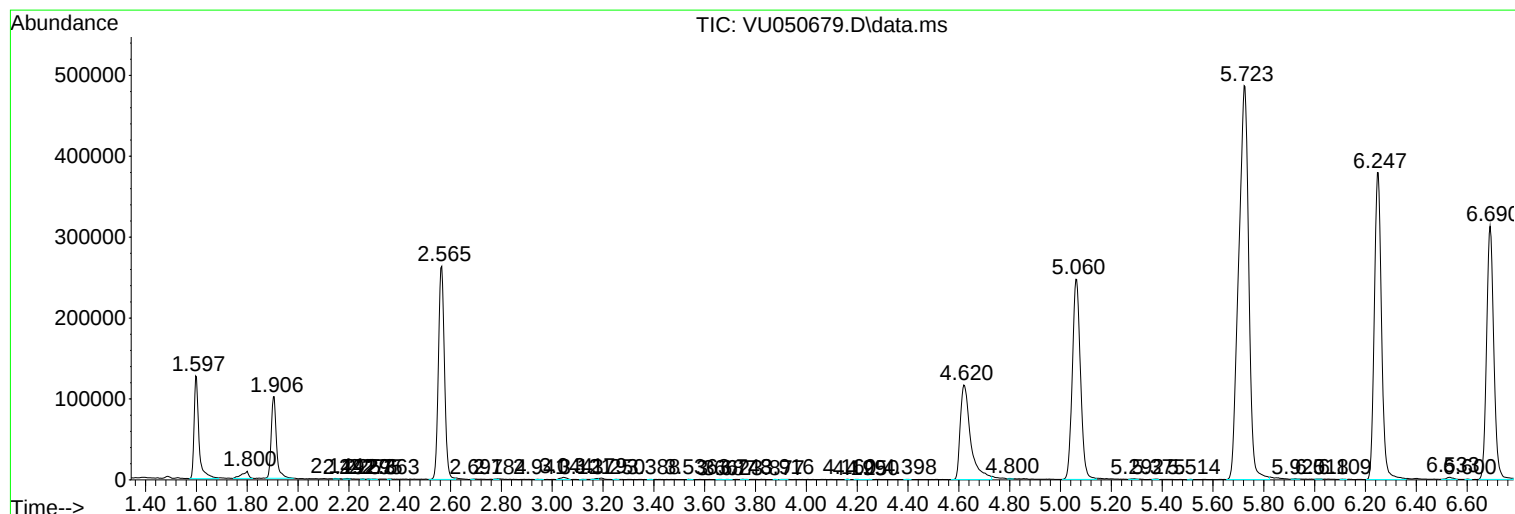

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050679.D
Acq On : 08 Sep 2022 12:07
Operator : SY/MD
Sample : VU0908WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050679.D
Acq On : 08 Sep 2022 12:07
Operator : SY/MD
Sample : VU0908WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------