

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050681.D
 Acq On : 08 Sep 2022 13:01
 Operator : SY/MD
 Sample : N4475-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rBV	100118	130067	10.34%	1.354%
2	1.903	167	175	192	rBV	82184	112066	8.91%	1.167%
3	2.565	368	381	395	rBV	208211	339830	27.03%	3.539%
4	2.713	425	427	431	rVB	544	265	0.02%	0.003%
5	2.970	504	507	510	rVB2	519	344	0.03%	0.004%
6	3.153	561	564	566	rBV	136	73	0.01%	0.001%
7	3.169	566	569	570	rBV2	381	243	0.02%	0.003%
8	3.321	614	616	618	rBV2	282	170	0.01%	0.002%
9	3.343	621	623	624	rBV2	352	163	0.01%	0.002%
10	3.462	658	660	663	rVB	170	96	0.01%	0.001%
11	3.494	663	670	672	rBV2	199	208	0.02%	0.002%
12	3.510	672	675	678	rVB2	236	129	0.01%	0.001%
13	3.555	686	689	691	rBV2	169	106	0.01%	0.001%
14	3.739	744	746	750	rBV2	98	83	0.01%	0.001%
15	3.784	758	760	766	rBV	477	424	0.03%	0.004%
16	3.854	778	782	785	rBV2	194	166	0.01%	0.002%
17	3.899	793	796	798	rBV2	231	118	0.01%	0.001%
18	4.067	846	848	851	rBV	140	74	0.01%	0.001%
19	4.198	887	889	891	rVB	298	90	0.01%	0.001%
20	4.234	896	900	903	rBV	138	109	0.01%	0.001%
21	4.263	903	909	916	rBV2	244	365	0.03%	0.004%
22	4.321	924	927	929	rBV2	103	70	0.01%	0.001%
23	4.353	936	937	938	rBV	151	31	0.00%	0.000%
24	4.366	938	941	946	rVV2	105	79	0.01%	0.001%
25	4.449	964	967	970	rVB2	238	147	0.01%	0.002%
26	4.468	970	973	979	rBV2	283	293	0.02%	0.003%
27	4.620	1008	1020	1061	rBV	106361	322764	25.67%	3.361%
28	5.063	1141	1158	1181	rBV	211326	470021	37.38%	4.894%
29	5.275	1222	1224	1225	rBV	705	317	0.03%	0.003%
30	5.337	1239	1243	1249	rVB3	381	382	0.03%	0.004%
31	5.382	1249	1257	1260	rBV3	1009	1363	0.11%	0.014%
32	5.423	1267	1270	1273	rBV2	149	109	0.01%	0.001%
33	5.478	1285	1287	1290	rBV2	231	136	0.01%	0.001%
34	5.510	1294	1297	1301	rVB2	334	251	0.02%	0.003%
35	5.533	1301	1304	1305	rBV	183	95	0.01%	0.001%
36	5.549	1305	1309	1314	rBV2	243	275	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050681.D
 Acq On : 08 Sep 2022 13:01
 Operator : SY/MD
 Sample : N4475-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.629	1329	1334	1336	rBV2	252	194	0.02%	0.002%
38	5.722	1342	1363	1397	rBV2	412301	1159815	92.24%	12.077%
39	6.195	1508	1510	1512	rVB2	153	64	0.01%	0.001%
40	6.250	1512	1527	1554	rBV	322470	637719	50.72%	6.641%
41	6.542	1606	1618	1635	rBV2	77627	147127	11.70%	1.532%
42	6.690	1649	1664	1684	rBV	272692	536260	42.65%	5.584%
43	7.034	1767	1771	1773	rBV	178	134	0.01%	0.001%
44	7.169	1808	1813	1814	rBV3	489	371	0.03%	0.004%
45	7.308	1854	1856	1857	rBV3	258	119	0.01%	0.001%
46	7.375	1872	1877	1880	rVB2	290	255	0.02%	0.003%
47	7.465	1902	1905	1907	rBV	217	141	0.01%	0.001%
48	7.565	1924	1936	1956	rBV	129725	228935	18.21%	2.384%
49	7.681	1970	1972	1975	rBV3	753	452	0.04%	0.005%
50	7.899	2026	2040	2070	rBV	471950	833557	66.29%	8.680%
51	8.179	2115	2127	2148	rBV	90162	153893	12.24%	1.602%
52	8.475	2215	2219	2224	rBV2	260	291	0.02%	0.003%
53	8.552	2229	2243	2258	rBV	744709	1257415	100.00%	13.093%
54	8.635	2259	2269	2279	rBV4	193252	431015	34.28%	4.488%
55	9.076	2403	2406	2408	rBV	203	119	0.01%	0.001%
56	9.127	2418	2422	2424	rBV2	169	144	0.01%	0.001%
57	9.163	2431	2433	2439	rVB2	297	217	0.02%	0.002%
58	9.230	2452	2454	2463	rBV2	343	374	0.03%	0.004%
59	9.279	2467	2469	2472	rVB	262	130	0.01%	0.001%
60	9.417	2499	2512	2531	rBV	467333	800177	63.64%	8.332%
61	9.565	2552	2558	2561	rBV4	560	596	0.05%	0.006%
62	9.600	2567	2569	2571	rBV3	237	129	0.01%	0.001%
63	9.758	2613	2618	2622	rBV2	348	407	0.03%	0.004%
64	9.819	2634	2637	2640	rBV2	229	137	0.01%	0.001%
65	9.951	2675	2678	2679	rBV2	118	69	0.01%	0.001%
66	10.031	2699	2703	2706	rBV2	263	245	0.02%	0.003%
67	10.246	2768	2770	2776	rVB	346	258	0.02%	0.003%
68	10.288	2778	2783	2784	rBV	421	283	0.02%	0.003%
69	10.346	2797	2801	2804	rBV2	478	363	0.03%	0.004%
70	10.536	2856	2860	2862	rBV2	241	217	0.02%	0.002%
71	10.549	2862	2864	2866	rVB	339	146	0.01%	0.002%
72	10.754	2916	2928	2953	rBV	420622	698173	55.52%	7.270%
73	10.893	2969	2971	2975	rVB2	475	294	0.02%	0.003%
74	11.693	3213	3220	3229	rVB5	3970	6866	0.55%	0.071%
75	11.812	3245	3257	3276	rBV	374010	609893	48.50%	6.351%
76	11.967	3303	3305	3310	rBV	354	325	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050681.D
Acq On : 08 Sep 2022 13:01
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

77	12.073	3331	3338	3348	rVB6	2277	4071	0.32%	0.042%
78	12.192	3362	3375	3395	rBV	418687	700783	55.73%	7.297%
79	12.378	3427	3433	3440	rVB4	578	790	0.06%	0.008%
80	12.651	3515	3518	3520	rBV	357	235	0.02%	0.002%
81	12.893	3587	3593	3604	rVB6	4972	7170	0.57%	0.075%
82	13.227	3690	3697	3703	rBV5	1195	1555	0.12%	0.016%




Sum of corrected areas: 9603445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050681.D
Acq On : 08 Sep 2022 13:01
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

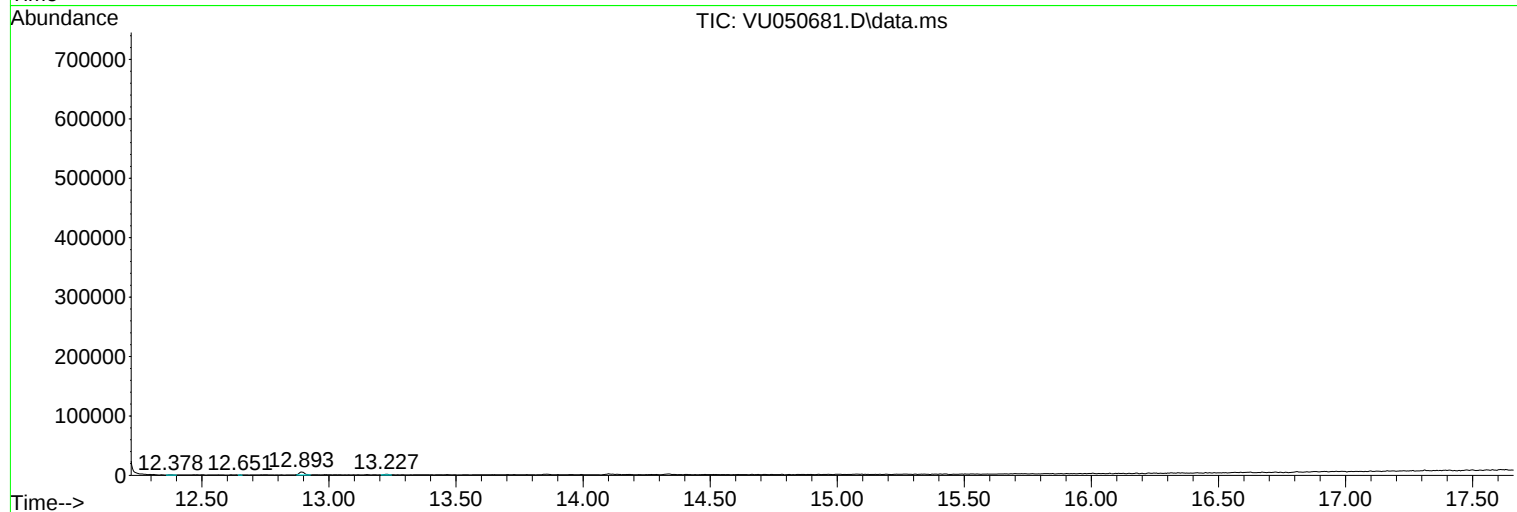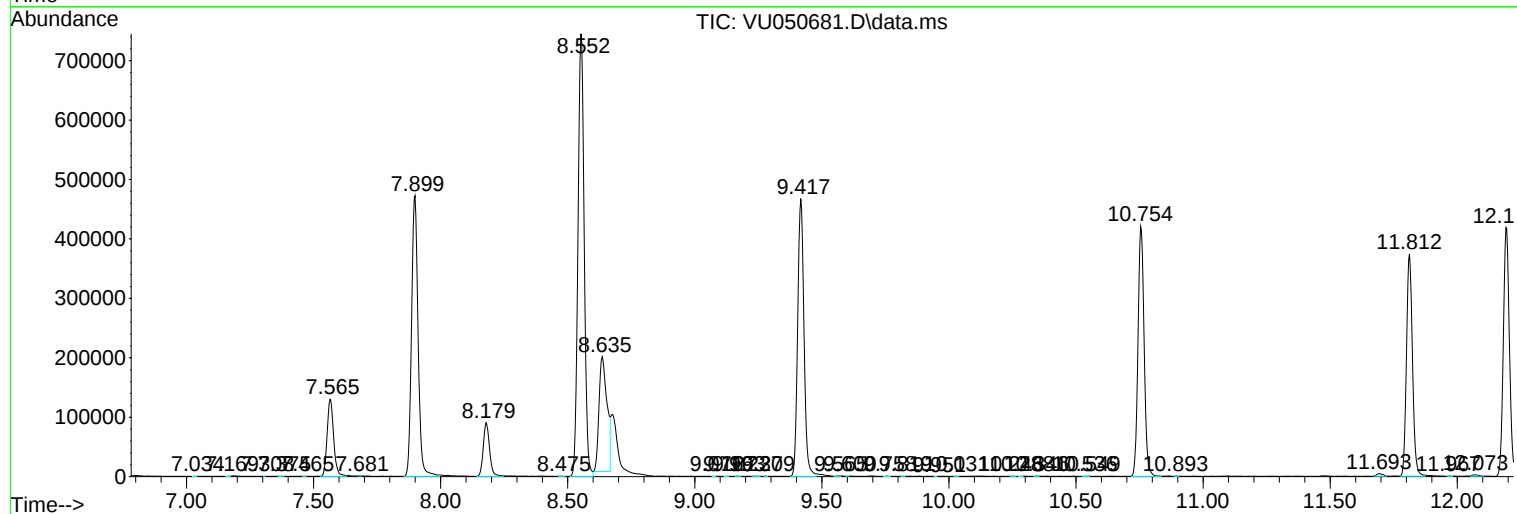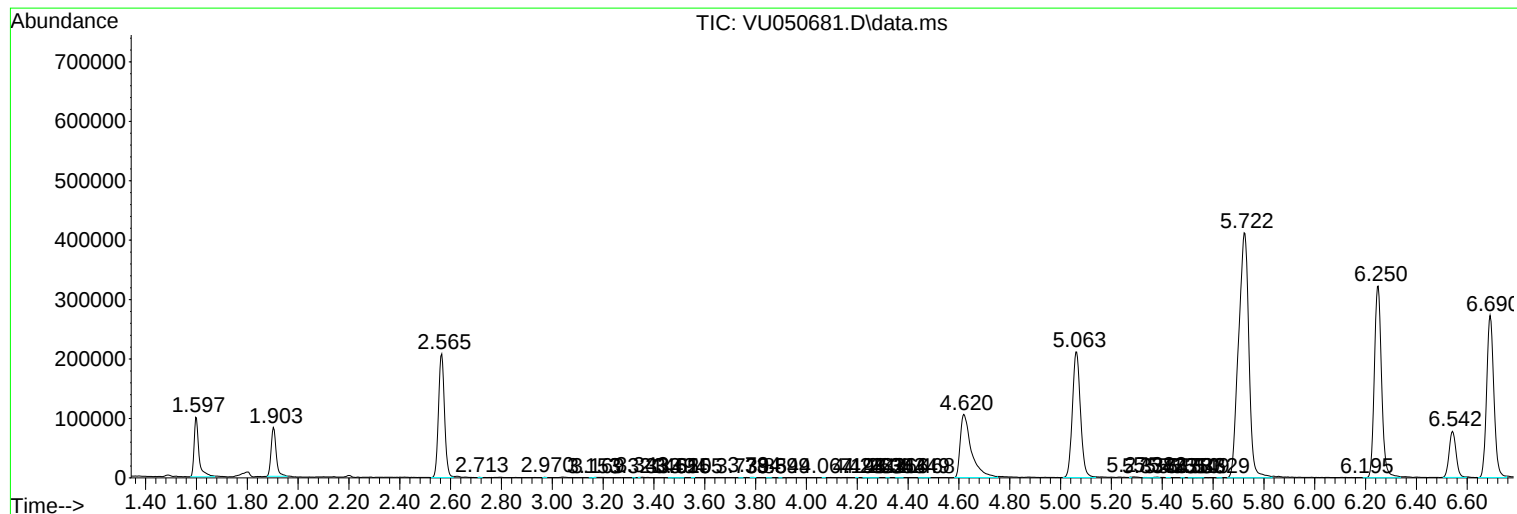

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050681.D
Acq On : 08 Sep 2022 13:01
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050681.D
Acq On : 08 Sep 2022 13:01
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------