

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050684.D
 Acq On : 08 Sep 2022 14:37
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

Signal : TIC: VU050684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rBV	100836	128286	10.28%	1.419%
2	1.900	167	174	195	rVB	82361	115014	9.22%	1.272%
3	2.382	318	324	329	rBV4	685	1066	0.09%	0.012%
4	2.424	334	337	343	rVB3	759	669	0.05%	0.007%
5	2.562	368	380	400	rBV	204758	330634	26.49%	3.656%
6	2.726	429	431	434	rBV	420	309	0.02%	0.003%
7	2.871	473	476	479	rBV2	230	202	0.02%	0.002%
8	3.044	520	530	541	rBV3	6202	11632	0.93%	0.129%
9	3.112	547	551	553	rBV2	309	237	0.02%	0.003%
10	3.182	559	573	592	rVB	13290	29562	2.37%	0.327%
11	3.761	750	753	755	rBV2	237	150	0.01%	0.002%
12	3.851	778	781	783	rBV2	125	72	0.01%	0.001%
13	3.887	790	792	794	rBV	130	75	0.01%	0.001%
14	3.912	798	800	802	rBV	141	76	0.01%	0.001%
15	3.922	802	803	804	rBV	199	45	0.00%	0.000%
16	3.964	814	816	817	rBV	207	59	0.00%	0.001%
17	4.025	832	835	837	rBV	193	108	0.01%	0.001%
18	4.060	843	846	851	rVB2	236	181	0.01%	0.002%
19	4.086	851	854	856	rBV	152	93	0.01%	0.001%
20	4.121	864	865	869	rBV	202	84	0.01%	0.001%
21	4.269	907	911	913	rBV	244	180	0.01%	0.002%
22	4.311	922	924	928	rVB	212	133	0.01%	0.001%
23	4.334	928	931	935	rBV2	209	225	0.02%	0.002%
24	4.382	943	946	948	rBV2	180	116	0.01%	0.001%
25	4.436	959	963	964	rBV2	254	168	0.01%	0.002%
26	4.526	988	991	993	rVB	115	60	0.00%	0.001%
27	4.552	993	999	1002	rBV2	298	352	0.03%	0.004%
28	4.620	1008	1020	1054	rBV	131036	347259	27.83%	3.840%
29	5.063	1141	1158	1180	rBV	225573	504961	40.46%	5.584%
30	5.288	1222	1228	1236	rVB4	1317	1815	0.15%	0.020%
31	5.379	1251	1256	1259	rBV2	740	670	0.05%	0.007%
32	5.417	1267	1268	1269	rBV2	105	32	0.00%	0.000%
33	5.459	1278	1281	1282	rBV	106	58	0.00%	0.001%
34	5.578	1316	1318	1322	rBV	208	141	0.01%	0.002%
35	5.723	1342	1363	1397	rBV2	443886	1247978	100.00%	13.800%
36	5.993	1445	1447	1451	rVB2	416	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050684.D
 Acq On : 08 Sep 2022 14:37
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.063	1468	1469	1471	rBV	220	63	0.01%	0.001%
38	6.247	1513	1526	1550	rBV	331054	640122	51.29%	7.078%
39	6.536	1606	1616	1618	rBV6	2699	4090	0.33%	0.045%
40	6.623	1639	1643	1648	rBV3	290	300	0.02%	0.003%
41	6.690	1648	1664	1682	rBV	289678	575035	46.08%	6.359%
42	6.883	1721	1724	1725	rBV	389	205	0.02%	0.002%
43	6.951	1744	1745	1748	rBV	177	95	0.01%	0.001%
44	6.970	1748	1751	1756	rVB3	376	317	0.03%	0.004%
45	7.012	1762	1764	1767	rVB2	170	89	0.01%	0.001%
46	7.034	1767	1771	1778	rVB2	330	391	0.03%	0.004%
47	7.067	1778	1781	1784	rBV2	222	171	0.01%	0.002%
48	7.095	1787	1790	1794	rVB	344	193	0.02%	0.002%
49	7.121	1794	1798	1802	rBV2	273	253	0.02%	0.003%
50	7.141	1802	1804	1806	rBV	217	106	0.01%	0.001%
51	7.404	1883	1886	1889	rBV2	240	157	0.01%	0.002%
52	7.510	1916	1919	1921	rBV2	148	73	0.01%	0.001%
53	7.565	1923	1936	1964	rBV	148618	263142	21.09%	2.910%
54	7.755	1993	1995	1997	rBV2	146	78	0.01%	0.001%
55	7.835	2018	2020	2021	rBV2	184	56	0.00%	0.001%
56	7.851	2021	2025	2026	rBV2	377	250	0.02%	0.003%
57	7.896	2026	2039	2060	rBV	493976	872304	69.90%	9.646%
58	8.179	2115	2127	2143	rBV	103606	176854	14.17%	1.956%
59	8.382	2187	2190	2195	rVB2	645	455	0.04%	0.005%
60	8.407	2195	2198	2203	rBV3	399	430	0.03%	0.005%
61	8.452	2208	2212	2214	rBV	488	371	0.03%	0.004%
62	8.478	2218	2220	2221	rBV	120	38	0.00%	0.000%
63	8.549	2234	2242	2253	rBV4	5455	9187	0.74%	0.102%
64	8.636	2257	2269	2299	rBV6	252611	718747	57.59%	7.948%
65	8.899	2348	2351	2353	rBV2	404	214	0.02%	0.002%
66	8.915	2353	2356	2357	rBV	318	198	0.02%	0.002%
67	9.054	2396	2399	2403	rVB	361	248	0.02%	0.003%
68	9.137	2423	2425	2428	rVV	228	93	0.01%	0.001%
69	9.160	2428	2432	2436	rVB2	524	425	0.03%	0.005%
70	9.185	2436	2440	2445	rBV2	317	359	0.03%	0.004%
71	9.320	2480	2482	2483	rBV	285	108	0.01%	0.001%
72	9.356	2490	2493	2496	rVB	252	134	0.01%	0.001%
73	9.417	2499	2512	2553	rBV	466508	812504	65.11%	8.984%
74	9.751	2613	2616	2619	rBV	161	125	0.01%	0.001%
75	10.018	2697	2699	2702	rVB	220	126	0.01%	0.001%
76	10.176	2746	2748	2753	rBV2	267	222	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050684.D
 Acq On : 08 Sep 2022 14:37
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

77	10.755	2915	2928	2948	rBV	466997	763785	61.20%	8.446%
78	11.089	3024	3032	3040	rBV3	1723	2931	0.23%	0.032%
79	11.472	3144	3151	3157	rBV4	2423	2934	0.24%	0.032%
80	11.748	3229	3237	3244	rVB4	3385	4908	0.39%	0.054%
81	11.812	3244	3257	3282	rBV	373004	627160	50.25%	6.935%
82	12.192	3363	3375	3394	rBV	457004	767900	61.53%	8.491%
83	12.394	3436	3438	3440	rBV	353	142	0.01%	0.002%
84	13.227	3688	3697	3705	rBV3	4792	7760	0.62%	0.086%
85	13.848	3883	3890	3905	rVB2	8564	12609	1.01%	0.139%
86	14.092	3957	3966	3986	rBV2	17898	34676	2.78%	0.383%
87	14.333	4033	4041	4058	rVB3	10809	17495	1.40%	0.193%




Sum of corrected areas: 9043533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050684.D
Acq On : 08 Sep 2022 14:37
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

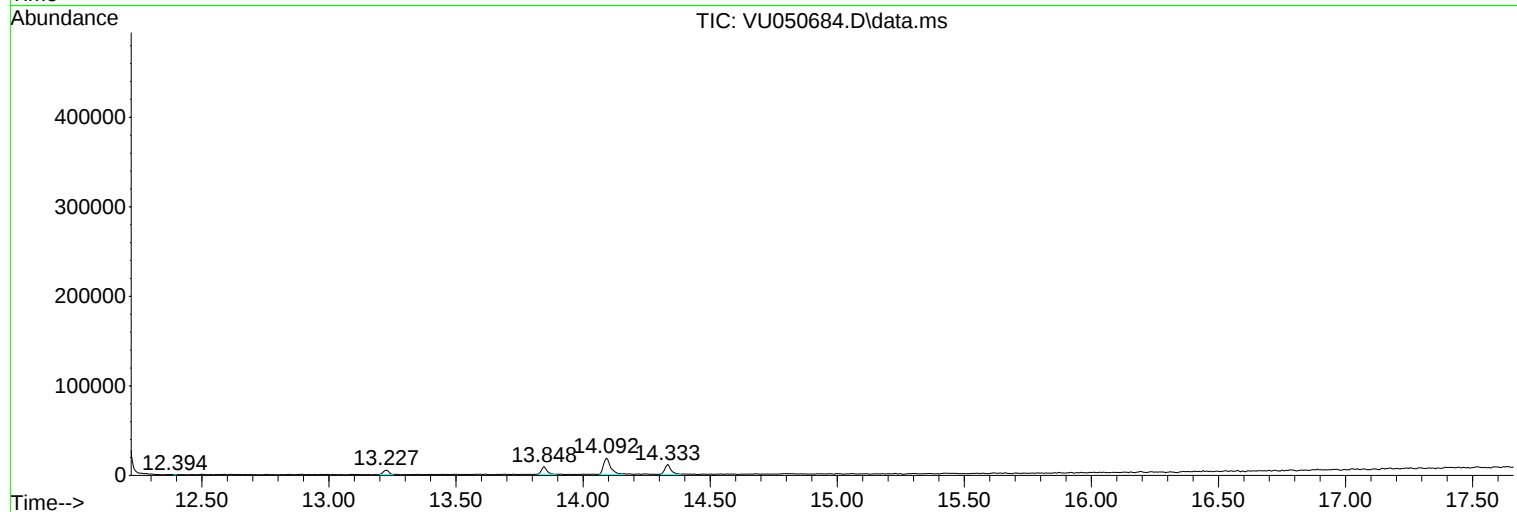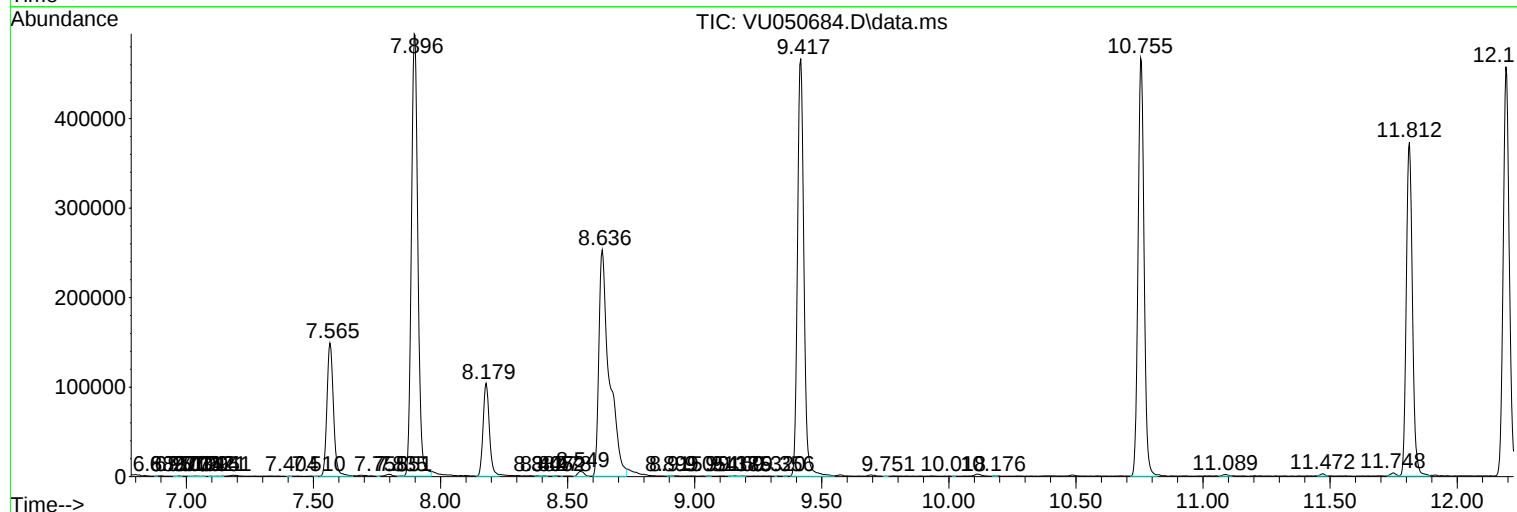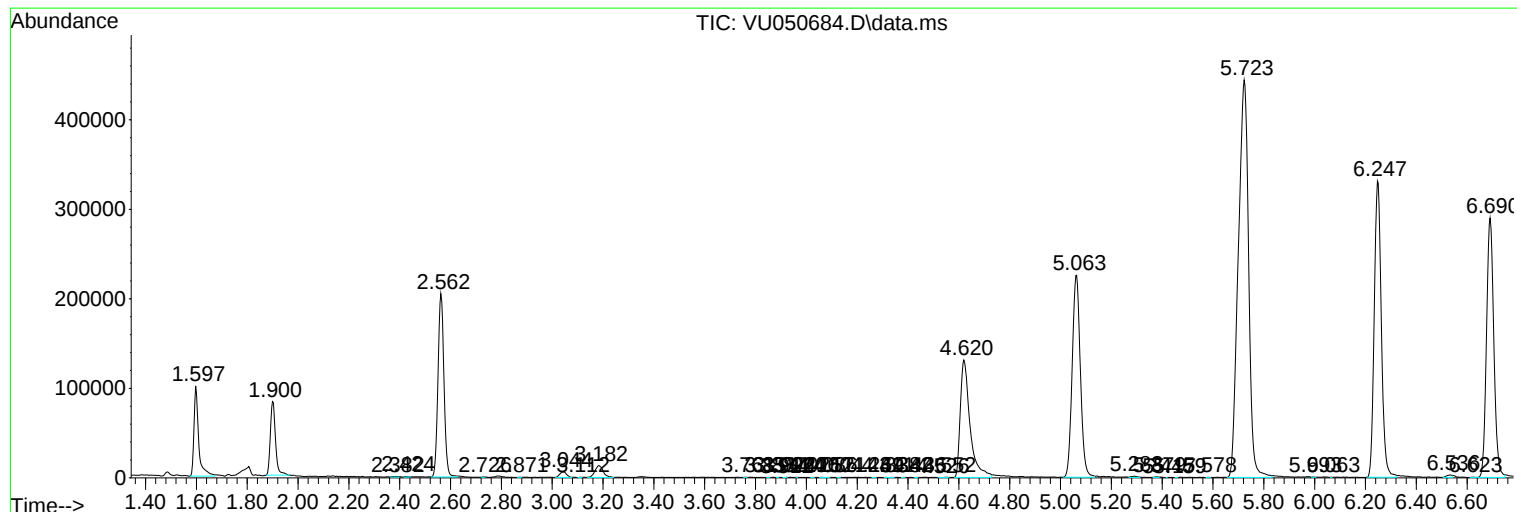

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050684.D
Acq On : 08 Sep 2022 14:37
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050684.D
Acq On : 08 Sep 2022 14:37
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------