

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050686.D
 Acq On : 08 Sep 2022 15:26
 Operator : SY/MD
 Sample : N4475-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	72601	94691	8.74%	1.082%
2	1.903	167	175	193	rBV	66443	91952	8.49%	1.051%
3	2.279	288	292	295	rBV3	697	661	0.06%	0.008%
4	2.321	302	305	308	rBV2	638	488	0.05%	0.006%
5	2.562	368	380	396	rBV	153341	253811	23.43%	2.901%
6	2.774	444	446	449	rBV2	508	440	0.04%	0.005%
7	2.855	467	471	477	rBV2	290	388	0.04%	0.004%
8	3.086	538	543	546	rBV2	278	280	0.03%	0.003%
9	3.166	565	568	569	rBV	587	361	0.03%	0.004%
10	3.353	620	626	629	rBV2	818	869	0.08%	0.010%
11	3.459	656	659	662	rBV	183	107	0.01%	0.001%
12	3.478	662	665	670	rVV2	207	196	0.02%	0.002%
13	3.549	684	687	691	rVB	343	240	0.02%	0.003%
14	3.581	691	697	700	rBV2	319	384	0.04%	0.004%
15	3.636	707	714	716	rBV2	226	295	0.03%	0.003%
16	3.784	757	760	762	rBV	82	48	0.00%	0.001%
17	3.810	764	768	769	rBV2	192	102	0.01%	0.001%
18	3.896	792	795	797	rBV	167	104	0.01%	0.001%
19	3.909	797	799	800	rBV	262	71	0.01%	0.001%
20	4.009	826	830	834	rVB2	283	252	0.02%	0.003%
21	4.031	834	837	843	rBV2	216	223	0.02%	0.003%
22	4.247	901	904	907	rVB2	205	129	0.01%	0.001%
23	4.266	907	910	914	rBV	187	155	0.01%	0.002%
24	4.372	940	943	947	rBV2	185	158	0.01%	0.002%
25	4.472	971	974	977	rVB2	289	198	0.02%	0.002%
26	4.494	977	981	985	rVB2	174	129	0.01%	0.001%
27	4.523	985	990	994	rBV2	298	324	0.03%	0.004%
28	4.562	998	1002	1006	rBV2	293	240	0.02%	0.003%
29	4.620	1008	1020	1057	rBV	121200	337820	31.18%	3.861%
30	5.064	1141	1158	1186	rBV	183591	414288	38.24%	4.735%
31	5.260	1217	1219	1220	rBV	170	67	0.01%	0.001%
32	5.356	1245	1249	1251	rBV2	526	416	0.04%	0.005%
33	5.475	1281	1286	1289	rBV	293	258	0.02%	0.003%
34	5.527	1297	1302	1304	rBV	199	226	0.02%	0.003%
35	5.539	1304	1306	1309	rVV	265	145	0.01%	0.002%
36	5.568	1313	1315	1318	rBV	161	89	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050686.D
 Acq On : 08 Sep 2022 15:26
 Operator : SY/MD
 Sample : N4475-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.652	1337	1341	1342	rBV2	287	179	0.02%	0.002%
38	5.723	1342	1363	1391	rBV2	366091	1016827	93.85%	11.623%
39	6.063	1467	1469	1472	rVB2	338	201	0.02%	0.002%
40	6.080	1472	1474	1475	rBV	168	89	0.01%	0.001%
41	6.105	1480	1482	1483	rBV	240	104	0.01%	0.001%
42	6.186	1504	1507	1512	rBV3	269	266	0.02%	0.003%
43	6.250	1512	1527	1547	rBV	280286	547184	50.50%	6.254%
44	6.543	1606	1618	1636	rBV2	65691	127378	11.76%	1.456%
45	6.690	1650	1664	1682	rBV	242966	476619	43.99%	5.448%
46	6.973	1750	1752	1753	rBV	154	68	0.01%	0.001%
47	7.047	1773	1775	1777	rBV2	236	100	0.01%	0.001%
48	7.086	1784	1787	1789	rBV	222	148	0.01%	0.002%
49	7.221	1827	1829	1830	rBV	112	57	0.01%	0.001%
50	7.282	1846	1848	1851	rBV	91	62	0.01%	0.001%
51	7.343	1862	1867	1870	rBV2	230	196	0.02%	0.002%
52	7.362	1870	1873	1876	rVB2	196	145	0.01%	0.002%
53	7.388	1876	1881	1883	rBV2	156	140	0.01%	0.002%
54	7.481	1906	1910	1914	rBV2	214	210	0.02%	0.002%
55	7.517	1918	1921	1924	rBV	282	224	0.02%	0.003%
56	7.565	1924	1936	1960	rBV2	121970	217015	20.03%	2.481%
57	7.774	1998	2001	2002	rBV	344	208	0.02%	0.002%
58	7.793	2005	2007	2011	rVB3	506	289	0.03%	0.003%
59	7.848	2021	2024	2026	rBV	277	183	0.02%	0.002%
60	7.899	2026	2040	2063	rBV	395035	696985	64.33%	7.967%
61	8.179	2115	2127	2144	rBV	85749	149141	13.77%	1.705%
62	8.446	2206	2210	2212	rBV2	386	324	0.03%	0.004%
63	8.552	2230	2243	2258	rBV	642126	1083434	100.00%	12.384%
64	8.636	2259	2269	2310	rVB6	230250	665932	61.46%	7.612%
65	8.883	2343	2346	2349	rVB3	473	303	0.03%	0.003%
66	8.896	2349	2350	2353	rVV	193	61	0.01%	0.001%
67	8.909	2353	2354	2359	rVB2	301	217	0.02%	0.002%
68	8.983	2374	2377	2379	rBV	386	213	0.02%	0.002%
69	8.999	2379	2382	2384	rBV2	217	148	0.01%	0.002%
70	9.067	2400	2403	2408	rVB2	460	321	0.03%	0.004%
71	9.092	2408	2411	2415	rVB	365	265	0.02%	0.003%
72	9.121	2415	2420	2423	rBV2	343	338	0.03%	0.004%
73	9.157	2428	2431	2433	rBV2	507	310	0.03%	0.004%
74	9.263	2459	2464	2467	rBV2	465	371	0.03%	0.004%
75	9.298	2472	2475	2478	rVB3	367	244	0.02%	0.003%
76	9.417	2495	2512	2533	rBV	420283	712393	65.75%	8.143%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050686.D
 Acq On : 08 Sep 2022 15:26
 Operator : SY/MD
 Sample : N4475-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	9.771	2617	2622	2625	rBV2	247	226	0.02%	0.003%
78	9.787	2625	2627	2629	rVV	220	106	0.01%	0.001%
79	9.803	2629	2632	2638	rVV	352	217	0.02%	0.002%
80	9.841	2641	2644	2649	rVB2	244	251	0.02%	0.003%
81	9.893	2656	2660	2664	rBV2	208	159	0.01%	0.002%
82	9.928	2668	2671	2675	rBV2	224	199	0.02%	0.002%
83	10.102	2723	2725	2727	rBV	442	213	0.02%	0.002%
84	10.616	2882	2885	2888	rBV	337	260	0.02%	0.003%
85	10.652	2893	2896	2900	rBV2	348	333	0.03%	0.004%
86	10.755	2915	2928	2948	rBV	399565	661270	61.03%	7.558%
87	10.874	2962	2965	2966	rBV2	248	127	0.01%	0.001%
88	11.468	3146	3150	3159	rVB2	1127	1453	0.13%	0.017%
89	11.745	3231	3236	3244	rVB4	1385	1878	0.17%	0.021%
90	11.812	3244	3257	3274	rBV	329532	544498	50.26%	6.224%
91	12.002	3313	3316	3321	rBV3	424	318	0.03%	0.004%
92	12.192	3363	3375	3406	rBV	373281	637201	58.81%	7.283%
93	12.378	3429	3433	3438	rVB3	549	528	0.05%	0.006%




Sum of corrected areas: 8748734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050686.D
Acq On : 08 Sep 2022 15:26
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

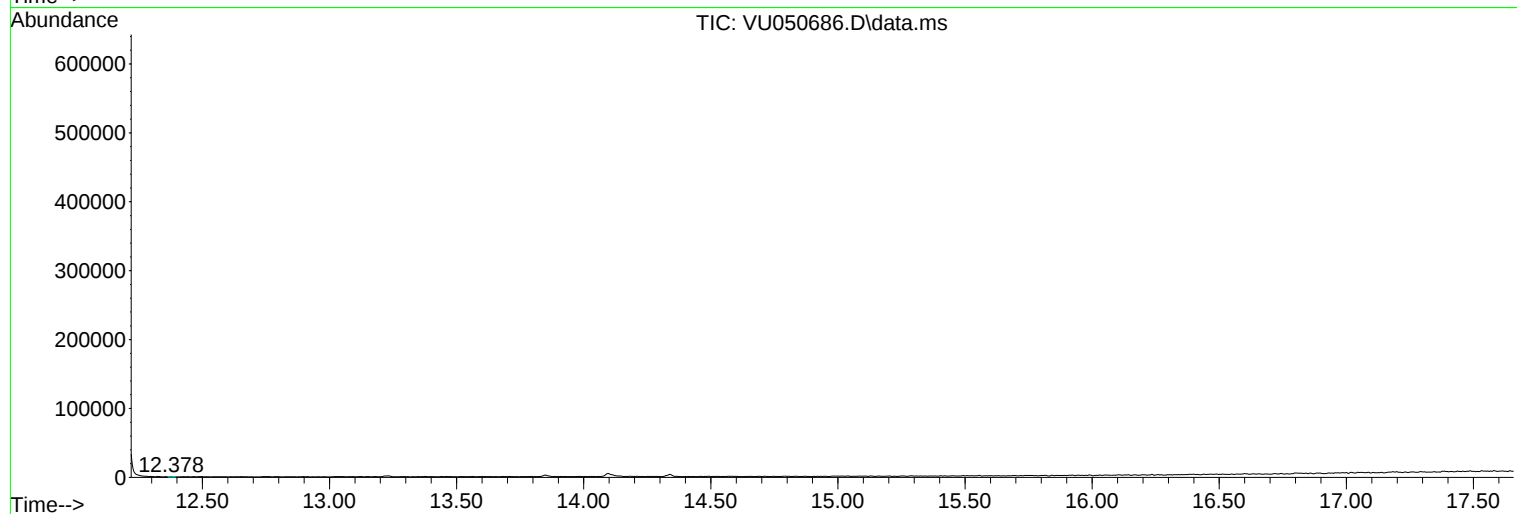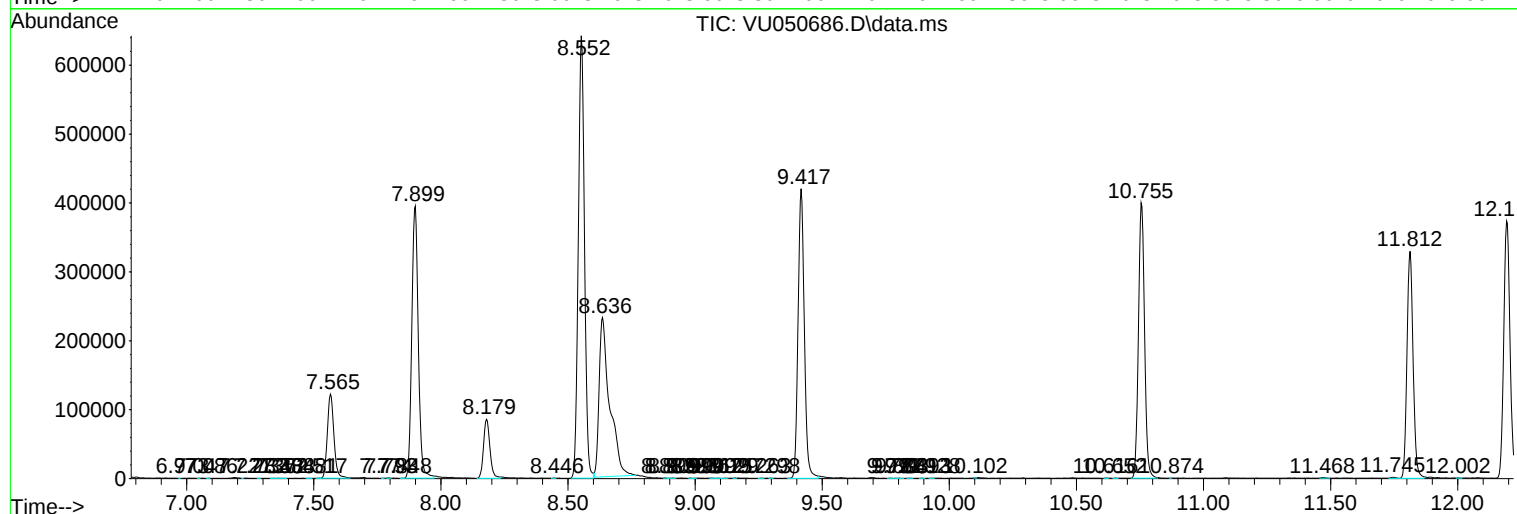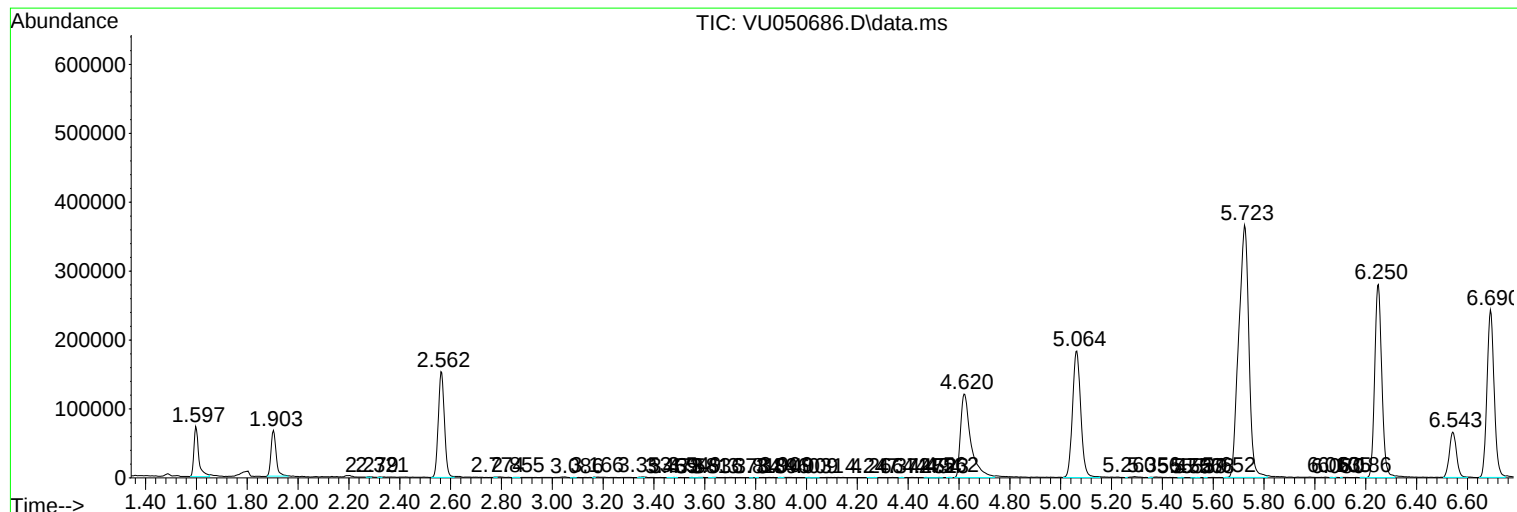

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050686.D
Acq On : 08 Sep 2022 15:26
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050686.D
Acq On : 08 Sep 2022 15:26
Operator : SY/MD
Sample : N4475-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------