

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050687.D
 Acq On : 08 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4475-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	53	rBV5	3132	3976	0.32%	0.043%
2	1.597	73	80	114	rBV	102577	133916	10.65%	1.464%
3	1.797	127	142	150	rVB6	9070	15663	1.25%	0.171%
4	1.903	167	175	196	rVB	87763	122213	9.72%	1.336%
5	2.054	220	222	225	rBV3	526	290	0.02%	0.003%
6	2.211	266	271	273	rBV3	470	465	0.04%	0.005%
7	2.327	304	307	308	rBV3	450	281	0.02%	0.003%
8	2.388	323	326	330	rVB2	793	465	0.04%	0.005%
9	2.514	362	365	368	rVB3	374	252	0.02%	0.003%
10	2.562	368	380	406	rBV	218783	362527	28.82%	3.963%
11	2.665	410	412	415	rVB3	477	222	0.02%	0.002%
12	2.755	436	440	441	rBV2	320	221	0.02%	0.002%
13	2.810	455	457	462	rVB2	809	542	0.04%	0.006%
14	2.842	462	467	471	rBV2	352	332	0.03%	0.004%
15	2.871	471	476	480	rBV2	408	349	0.03%	0.004%
16	3.044	519	530	542	rBV2	7534	13625	1.08%	0.149%
17	3.186	559	574	591	rVV2	16521	38860	3.09%	0.425%
18	3.324	615	617	623	rVV2	348	309	0.02%	0.003%
19	3.408	638	643	648	rBV	238	229	0.02%	0.003%
20	3.623	707	710	717	rVB2	315	257	0.02%	0.003%
21	3.867	781	786	790	rVB2	250	252	0.02%	0.003%
22	3.935	805	807	815	rVB	253	307	0.02%	0.003%
23	3.980	815	821	827	rBV2	293	411	0.03%	0.004%
24	4.083	850	853	857	rBV2	269	223	0.02%	0.002%
25	4.575	998	1006	1008	rBV2	342	400	0.03%	0.004%
26	4.620	1008	1020	1058	rBV	130610	360085	28.63%	3.937%
27	4.986	1129	1134	1137	rVB2	476	350	0.03%	0.004%
28	5.060	1142	1157	1181	rBV	231323	515703	41.00%	5.638%
29	5.289	1224	1228	1229	rBV3	566	437	0.03%	0.005%
30	5.369	1250	1253	1255	rVV	707	412	0.03%	0.005%
31	5.388	1257	1259	1261	rVV	534	267	0.02%	0.003%
32	5.539	1301	1306	1311	rVB2	236	268	0.02%	0.003%
33	5.584	1317	1320	1325	rBV2	256	270	0.02%	0.003%
34	5.726	1341	1364	1388	rBV3	446193	1257824	100.00%	13.752%
35	6.089	1474	1477	1480	rBV2	255	237	0.02%	0.003%
36	6.147	1491	1495	1501	rVB3	472	480	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050687.D
 Acq On : 08 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4475-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1557	rBV	339892	668535	53.15%	7.309%
38	6.430	1580	1583	1588	rVB4	510	335	0.03%	0.004%
39	6.536	1606	1616	1625	rVB7	2717	5131	0.41%	0.056%
40	6.575	1625	1628	1630	rBV	473	287	0.02%	0.003%
41	6.690	1649	1664	1688	rBV	298498	587919	46.74%	6.428%
42	6.851	1711	1714	1717	rVV3	570	340	0.03%	0.004%
43	6.883	1721	1724	1727	rVB4	525	228	0.02%	0.002%
44	7.022	1761	1767	1771	rBV2	254	373	0.03%	0.004%
45	7.070	1780	1782	1787	rVB2	269	235	0.02%	0.003%
46	7.182	1811	1817	1819	rBV4	956	966	0.08%	0.011%
47	7.263	1838	1842	1846	rBV2	269	223	0.02%	0.002%
48	7.292	1846	1851	1855	rVB2	299	306	0.02%	0.003%
49	7.565	1922	1936	1962	rBV	146042	262966	20.91%	2.875%
50	7.838	2015	2021	2025	rBV2	259	291	0.02%	0.003%
51	7.899	2025	2040	2070	rBV	506457	897469	71.35%	9.812%
52	8.179	2113	2127	2146	rBV	103955	178463	14.19%	1.951%
53	8.330	2172	2174	2178	rVB3	544	294	0.02%	0.003%
54	8.407	2193	2198	2201	rVB3	503	460	0.04%	0.005%
55	8.427	2201	2204	2206	rBV2	391	278	0.02%	0.003%
56	8.497	2219	2226	2230	rBV2	240	317	0.03%	0.003%
57	8.555	2236	2244	2253	rVB5	6059	9908	0.79%	0.108%
58	8.636	2256	2269	2317	rBV5	239002	727987	57.88%	7.959%
59	8.832	2328	2330	2335	rVB2	449	294	0.02%	0.003%
60	8.861	2336	2339	2343	rVV2	376	260	0.02%	0.003%
61	8.948	2361	2366	2371	rBV	472	432	0.03%	0.005%
62	9.105	2413	2415	2422	rVB2	452	300	0.02%	0.003%
63	9.247	2453	2459	2462	rBV2	263	241	0.02%	0.003%
64	9.417	2499	2512	2551	rBV	478914	823611	65.48%	9.004%
65	9.620	2568	2575	2577	rBV	322	398	0.03%	0.004%
66	9.690	2594	2597	2602	rVB2	275	237	0.02%	0.003%
67	10.012	2695	2697	2703	rVV2	301	279	0.02%	0.003%
68	10.115	2721	2729	2737	rBV3	559	868	0.07%	0.009%
69	10.459	2832	2836	2841	rBV2	371	399	0.03%	0.004%
70	10.755	2916	2928	2951	rBV	455881	756499	60.14%	8.271%
71	10.909	2973	2976	2983	rVB3	389	401	0.03%	0.004%
72	11.124	3038	3043	3046	rBV	298	275	0.02%	0.003%
73	11.343	3108	3111	3116	rVB2	305	291	0.02%	0.003%
74	11.375	3116	3121	3124	rBV2	313	326	0.03%	0.004%
75	11.745	3234	3236	3243	rVB3	835	718	0.06%	0.008%
76	11.812	3243	3257	3277	rBV	380200	620278	49.31%	6.781%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050687.D
 Acq On : 08 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4475-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	12.195	3363	3376	3399	rBV	444143	749782	59.61%	8.197%
78	12.394	3435	3438	3442	rVV2	358	294	0.02%	0.003%
79	12.433	3448	3450	3454	rVV2	309	231	0.02%	0.003%
80	12.459	3454	3458	3461	rVB3	556	420	0.03%	0.005%
81	12.607	3500	3504	3506	rBV2	387	264	0.02%	0.003%
82	12.674	3521	3525	3528	rVB3	267	230	0.02%	0.003%
83	12.693	3528	3531	3540	rBV3	395	477	0.04%	0.005%
84	12.970	3613	3617	3622	rBV2	551	572	0.05%	0.006%
85	13.037	3635	3638	3641	rBV	353	263	0.02%	0.003%
86	13.082	3649	3652	3655	rVB3	458	343	0.03%	0.004%
87	13.237	3693	3700	3706	rBV6	972	1652	0.13%	0.018%
88	13.449	3762	3766	3771	rBV3	506	575	0.05%	0.006%
89	13.526	3786	3790	3793	rBV2	402	395	0.03%	0.004%
90	13.590	3807	3810	3817	rBV3	388	494	0.04%	0.005%
91	13.838	3884	3887	3889	rBV3	436	340	0.03%	0.004%
92	13.851	3889	3891	3898	rVB3	1106	1077	0.09%	0.012%
93	13.931	3913	3916	3921	rBV2	344	419	0.03%	0.005%
94	14.024	3941	3945	3946	rBV	482	276	0.02%	0.003%
95	14.111	3962	3972	3977	rBV5	1657	3465	0.28%	0.038%
96	14.217	4002	4005	4009	rVB	686	450	0.04%	0.005%
97	14.336	4039	4042	4046	rBV2	962	814	0.06%	0.009%
98	14.385	4054	4057	4059	rBV2	442	271	0.02%	0.003%
99	15.655	4450	4452	4454	rBV2	787	330	0.03%	0.004%
100	16.327	4658	4661	4663	rBV4	1230	902	0.07%	0.010%




Sum of corrected areas: 9146674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050687.D
Acq On : 08 Sep 2022 15:49
Operator : SY/MD
Sample : N4475-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

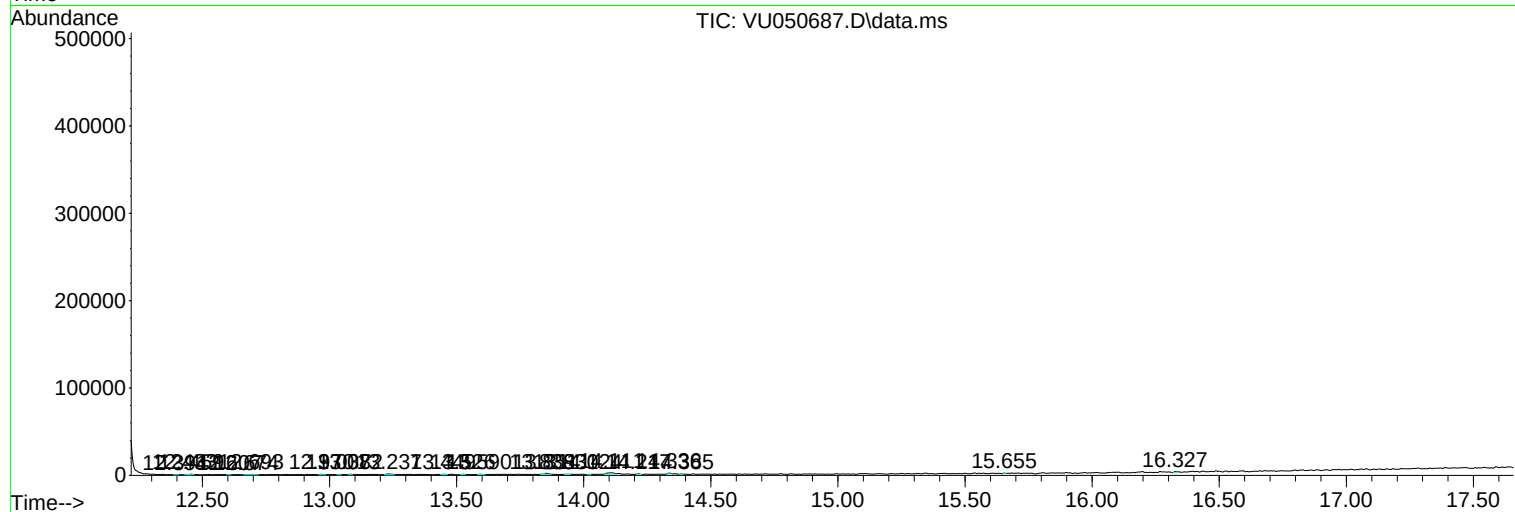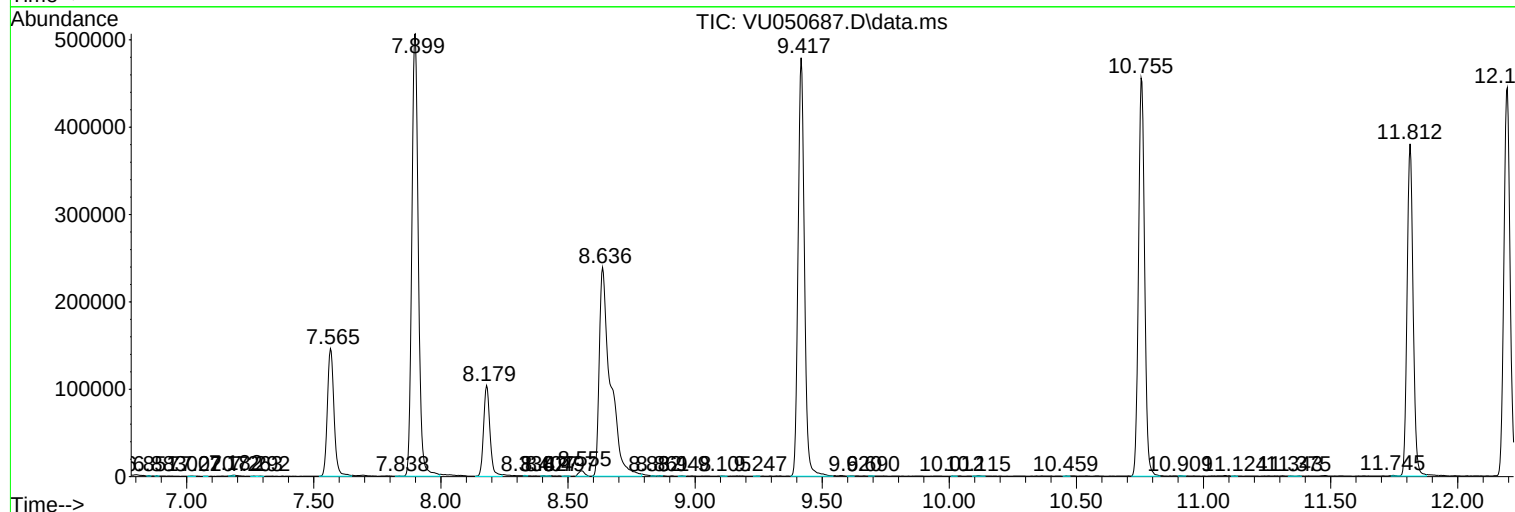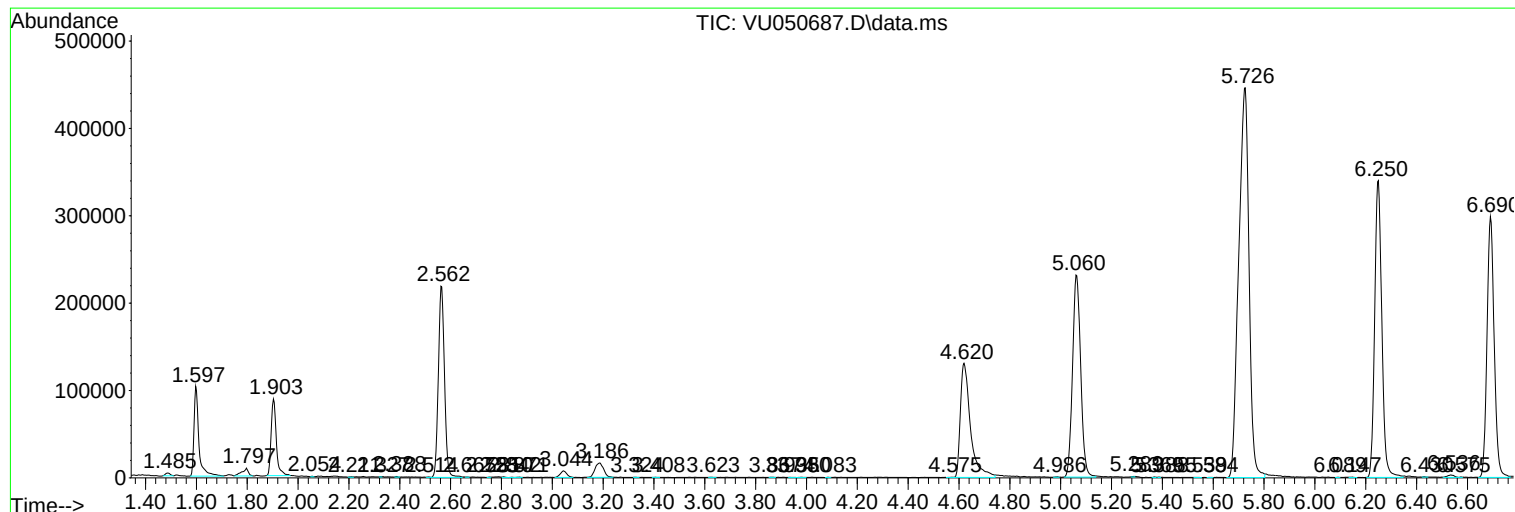

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050687.D
Acq On : 08 Sep 2022 15:49
Operator : SY/MD
Sample : N4475-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050687.D
Acq On : 08 Sep 2022 15:49
Operator : SY/MD
Sample : N4475-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------