

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050689.D
 Acq On : 08 Sep 2022 16:50
 Operator : SY/MD
 Sample : N4482-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	99	rBV	114114	144663	11.19%	1.526%
2	1.910	169	177	199	rVB	96962	135972	10.52%	1.435%
3	2.482	353	355	362	rVB2	501	402	0.03%	0.004%
4	2.566	368	381	398	rBV	236115	388204	30.04%	4.096%
5	2.762	437	442	443	rBV3	389	274	0.02%	0.003%
6	2.948	498	500	506	rVB2	275	197	0.02%	0.002%
7	3.045	517	530	542	rBV5	4068	7678	0.59%	0.081%
8	3.119	550	553	557	rBV2	399	341	0.03%	0.004%
9	3.353	623	626	630	rBV2	198	146	0.01%	0.002%
10	3.424	646	648	652	rVB2	342	227	0.02%	0.002%
11	3.498	666	671	675	rBV	300	256	0.02%	0.003%
12	3.524	676	679	680	rBV2	136	82	0.01%	0.001%
13	3.678	724	727	729	rBV2	166	88	0.01%	0.001%
14	3.739	743	746	749	rBV	196	155	0.01%	0.002%
15	3.868	783	786	788	rBV	290	214	0.02%	0.002%
16	4.019	830	833	834	rBV	264	128	0.01%	0.001%
17	4.045	839	841	843	rVV	102	49	0.00%	0.001%
18	4.077	847	851	853	rBV	119	94	0.01%	0.001%
19	4.138	867	870	873	rBV2	256	164	0.01%	0.002%
20	4.160	873	877	880	rBV2	206	168	0.01%	0.002%
21	4.176	880	882	883	rBV	199	89	0.01%	0.001%
22	4.212	891	893	895	rVB	362	115	0.01%	0.001%
23	4.228	895	898	902	rBV2	253	193	0.01%	0.002%
24	4.250	902	905	907	rBV	177	90	0.01%	0.001%
25	4.356	936	938	942	rBV	214	121	0.01%	0.001%
26	4.398	948	951	957	rBV2	208	192	0.01%	0.002%
27	4.446	963	966	968	rBV2	184	114	0.01%	0.001%
28	4.527	987	991	996	rBV2	287	243	0.02%	0.003%
29	4.620	1008	1020	1048	rBV	131672	344483	26.66%	3.634%
30	5.064	1143	1158	1183	rBV	238915	528295	40.88%	5.574%
31	5.279	1222	1225	1226	rBV	570	365	0.03%	0.004%
32	5.344	1243	1245	1248	rBV	355	247	0.02%	0.003%
33	5.421	1267	1269	1276	rVB2	200	147	0.01%	0.002%
34	5.459	1278	1281	1283	rVB2	158	94	0.01%	0.001%
35	5.479	1283	1287	1290	rBV2	237	196	0.02%	0.002%
36	5.501	1291	1294	1297	rVV2	289	155	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
 Data File : VU050689.D
 Acq On : 08 Sep 2022 16:50
 Operator : SY/MD
 Sample : N4482-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.546	1305	1308	1310	rBV2	225	156	0.01%	0.002%
38	5.610	1326	1328	1332	rBV2	150	143	0.01%	0.002%
39	5.726	1342	1364	1398	rBV2	460041	1292230	100.00%	13.634%
40	6.250	1512	1527	1558	rBV	374906	735439	56.91%	7.759%
41	6.691	1649	1664	1685	rBV	304597	597774	46.26%	6.307%
42	6.929	1735	1738	1741	rBV	374	210	0.02%	0.002%
43	6.951	1743	1745	1752	rVB2	466	351	0.03%	0.004%
44	7.006	1760	1762	1764	rVB2	250	103	0.01%	0.001%
45	7.022	1764	1767	1768	rBV	141	86	0.01%	0.001%
46	7.073	1780	1783	1787	rVB2	248	133	0.01%	0.001%
47	7.179	1808	1816	1817	rBV2	858	713	0.06%	0.008%
48	7.308	1853	1856	1859	rBV2	279	200	0.02%	0.002%
49	7.469	1902	1906	1910	rBV2	261	252	0.02%	0.003%
50	7.524	1919	1923	1924	rBV	359	234	0.02%	0.002%
51	7.565	1924	1936	1968	rVV2	148282	271090	20.98%	2.860%
52	7.900	2026	2040	2068	rBV	528847	942252	72.92%	9.941%
53	8.179	2116	2127	2142	rBV	104364	180625	13.98%	1.906%
54	8.478	2217	2220	2223	rBV	198	112	0.01%	0.001%
55	8.533	2236	2237	2238	rBV	166	59	0.00%	0.001%
56	8.559	2239	2245	2248	rVB4	942	968	0.07%	0.010%
57	8.636	2256	2269	2315	rBV5	252643	722571	55.92%	7.623%
58	8.941	2361	2364	2368	rVB3	388	241	0.02%	0.003%
59	8.970	2368	2373	2374	rBV	303	194	0.02%	0.002%
60	9.048	2395	2397	2398	rBV	356	99	0.01%	0.001%
61	9.131	2422	2423	2424	rBV	246	58	0.00%	0.001%
62	9.141	2424	2426	2429	rVV2	326	208	0.02%	0.002%
63	9.417	2498	2512	2553	rBV	521951	906665	70.16%	9.566%
64	9.723	2603	2607	2610	rBV	248	193	0.01%	0.002%
65	9.819	2634	2637	2639	rBV	192	120	0.01%	0.001%
66	10.089	2718	2721	2723	rBV	231	159	0.01%	0.002%
67	10.125	2729	2732	2735	rBV	264	184	0.01%	0.002%
68	10.166	2742	2745	2747	rBV	204	154	0.01%	0.002%
69	10.260	2772	2774	2778	rVB	288	163	0.01%	0.002%
70	10.427	2824	2826	2827	rBV2	247	88	0.01%	0.001%
71	10.758	2916	2929	2954	rBV	471349	765738	59.26%	8.079%
72	11.215	3068	3071	3076	rBV2	362	357	0.03%	0.004%
73	11.404	3128	3130	3133	rBV2	342	161	0.01%	0.002%
74	11.813	3244	3257	3278	rBV	426968	703488	54.44%	7.422%
75	12.195	3363	3376	3398	rBV	474496	798334	61.78%	8.423%
76	13.330	3726	3729	3735	rBV	545	484	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050689.D
Acq On : 08 Sep 2022 16:50
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis

77	13.854	3888	3892	3897	rVB4	768	826	0.06%	0.009%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 9478256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050689.D
Acq On : 08 Sep 2022 16:50
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

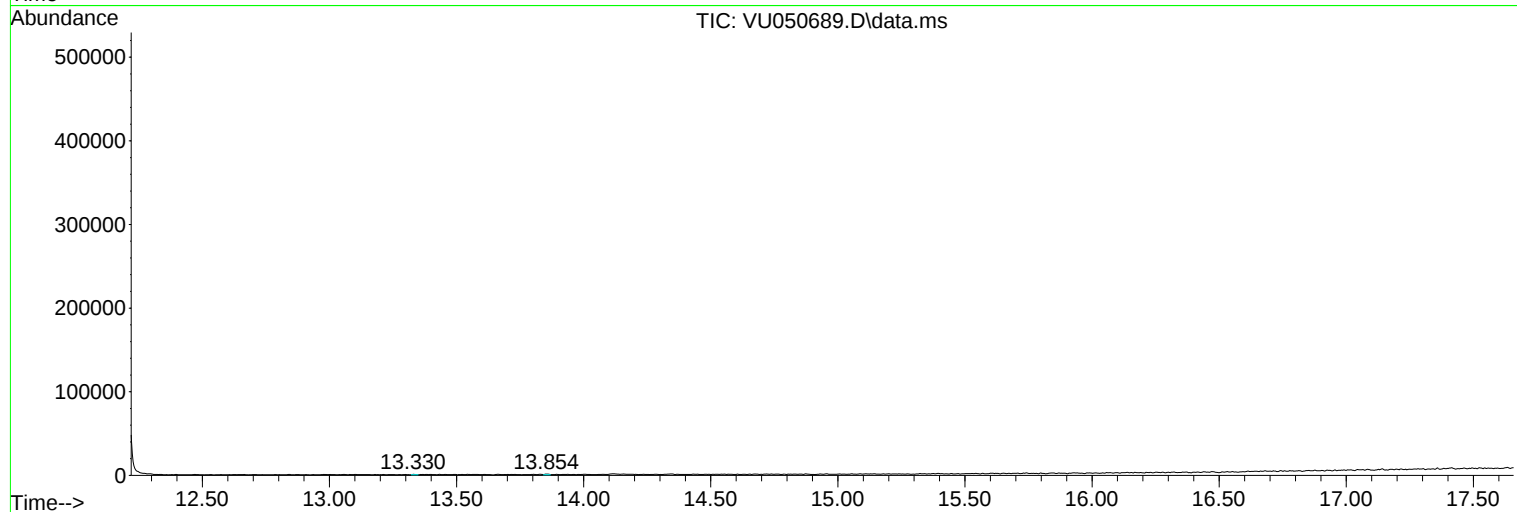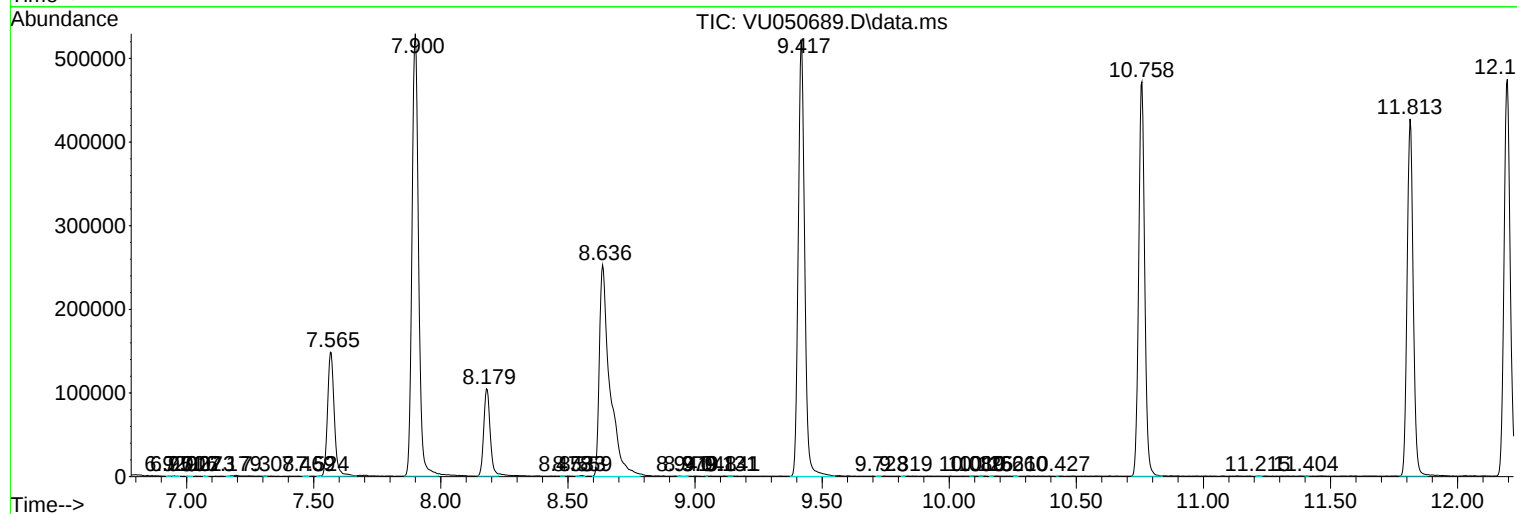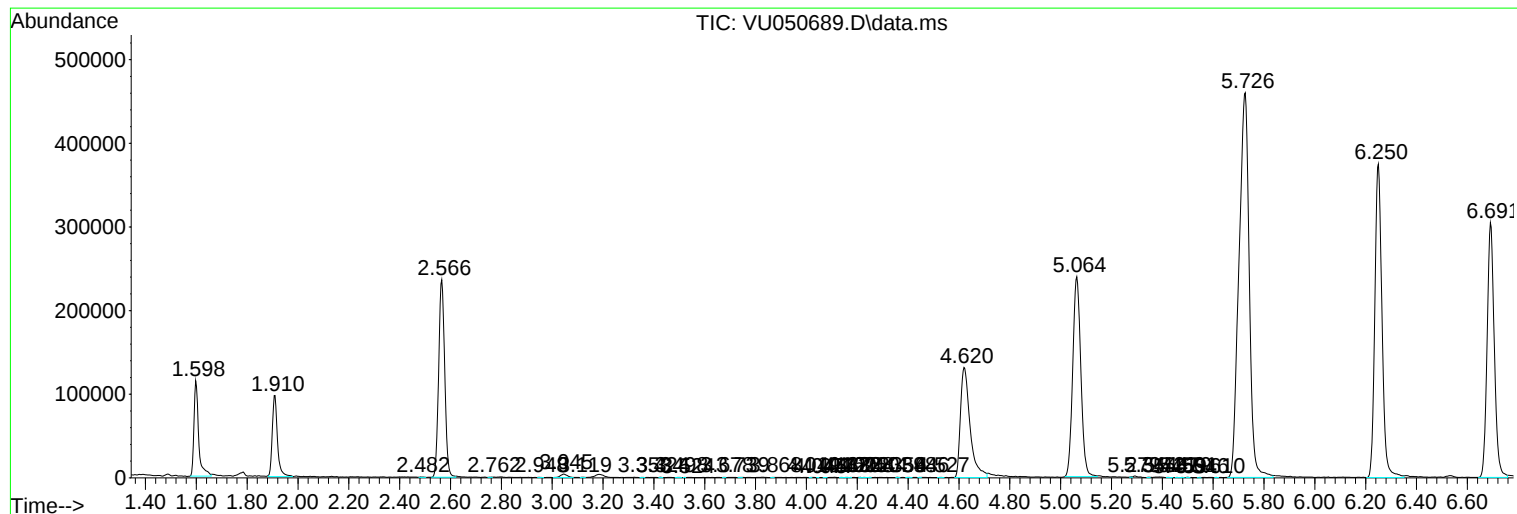

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050689.D
Acq On : 08 Sep 2022 16:50
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050689.D
Acq On : 08 Sep 2022 16:50
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------