


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090822\
Data File : VU050676.D
Acq On : 08 Sep 2022 10:26
Operator : SY/MD
Sample : BFB122
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB122

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis
Last Update : Thu Sep 08 22:51:50 2022

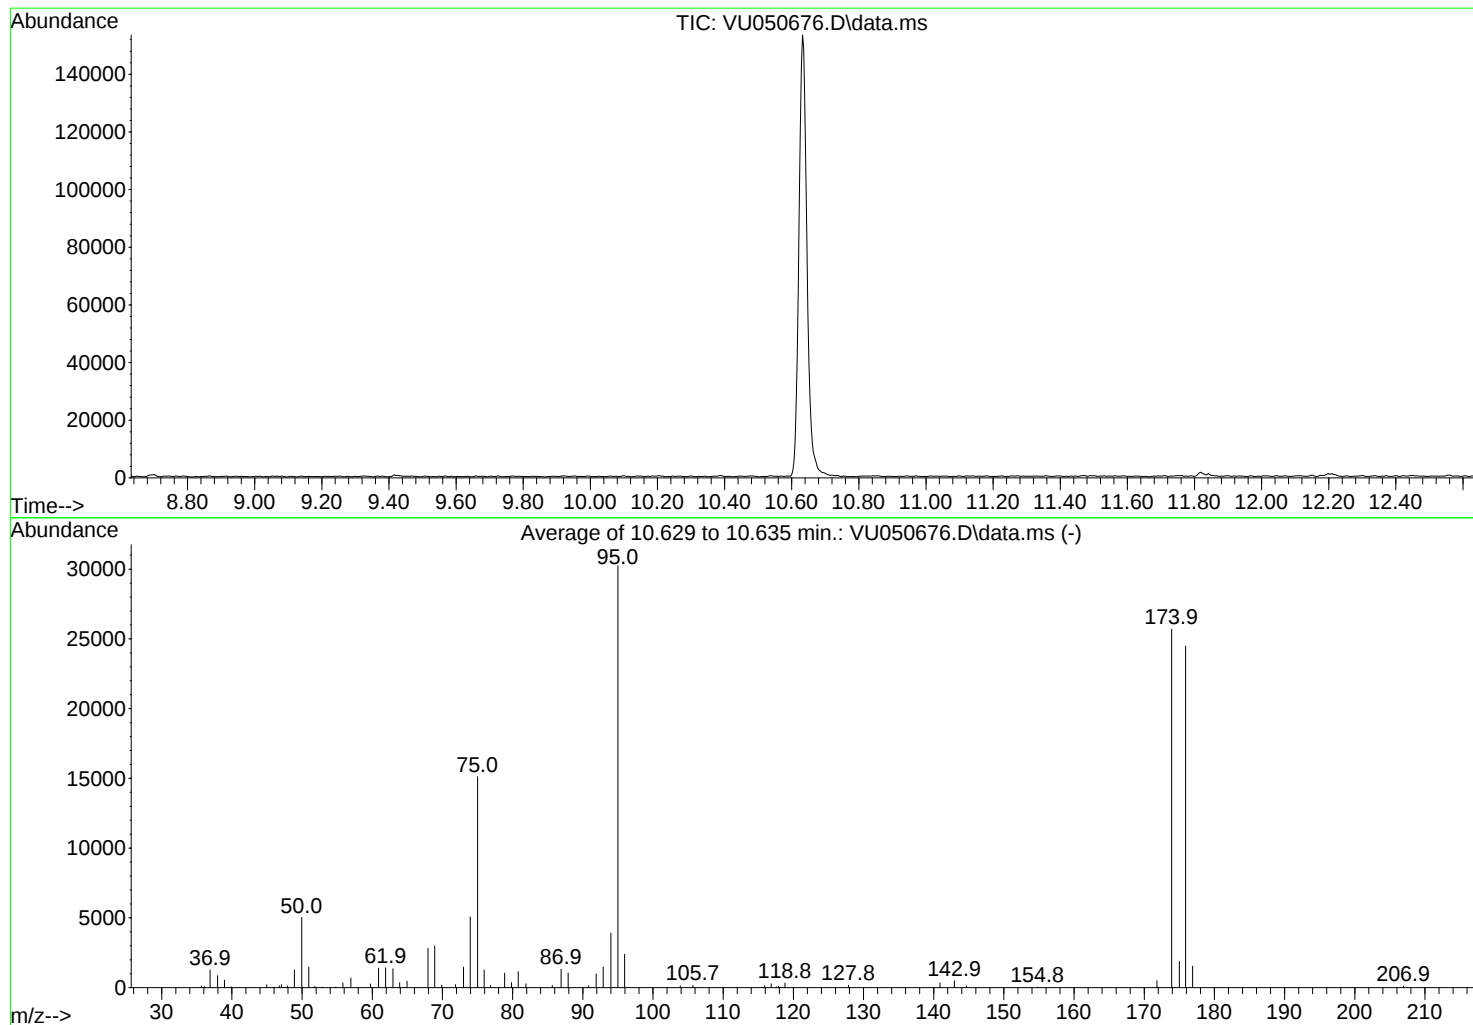

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5031	PASS
75	95	30	80	50.0	15120	PASS
95	95	100	100	100.0	30237	PASS
96	95	5	9	7.9	2393	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.0	25707	PASS
175	174	5	9	7.3	1884	PASS
176	174	95	101	95.2	24480	PASS
177	176	5	9	6.3	1537	PASS

m/z	Abundance
39.90	204.0
44.00	409.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.70	114.0
36.10	104.0
36.90	1270.0
37.90	882.0
38.90	608.0
39.90	274.0
43.90	406.0
44.90	200.0
46.70	173.0
47.10	138.0
47.90	110.0
48.90	1076.0
50.00	5048.0
51.00	1417.0
51.80	117.0
54.80	122.0
55.80	387.0
57.00	633.0
59.70	294.0
60.90	1417.0
61.90	1385.0
62.90	1332.0
63.90	326.0
65.00	451.0
68.00	2662.0
68.90	3075.0
69.90	189.0
71.80	213.0
73.00	1462.0
73.90	4909.0
75.00	14251.0
75.90	1323.0
76.80	134.0
78.80	948.0
79.80	302.0
80.80	1054.0
81.90	303.0
85.60	113.0
86.90	1200.0
87.90	994.0
90.80	134.0
91.90	1050.0
92.90	1527.0
94.00	3560.0
95.00	29384.0
95.90	2413.0
103.90	121.0
105.70	187.0
115.90	134.0
116.80	278.0
117.60	123.0
118.80	346.0
127.80	156.0
140.90	327.0
142.90	492.0
144.60	102.0
171.90	378.0
173.90	24592.0
175.00	1874.0
175.90	23160.0
176.90	1603.0
207.00	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.60	111.0
36.10	111.0
36.90	1288.0
38.00	886.0
38.90	563.0
39.90	262.0
43.90	400.0
45.00	220.0
46.80	193.0
47.00	196.0
47.90	145.0
48.90	1333.0
50.00	5223.0
50.90	1544.0
51.80	107.0
52.90	105.0
55.80	344.0
57.00	706.0
59.70	270.0
60.90	1468.0
61.90	1476.0
62.90	1368.0
63.90	386.0
64.90	472.0
67.90	2853.0
68.90	3086.0
69.90	188.0
71.80	229.0
73.00	1517.0
73.90	5287.0
75.00	15630.0
75.90	1310.0
76.80	151.0
78.90	1045.0
79.90	360.0
80.80	1190.0
81.90	289.0
85.60	164.0
86.90	1373.0
87.90	1099.0
90.90	125.0
91.90	1035.0
92.90	1532.0
94.00	4116.0
95.00	31248.0
95.90	2467.0
103.90	142.0
105.70	189.0
115.90	114.0
116.90	257.0
117.90	116.0
118.80	351.0
127.80	183.0
140.90	306.0
143.00	492.0
144.60	118.0
171.80	521.0
173.90	26616.0
175.00	1932.0
175.90	25096.0
176.90	1587.0
207.00	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.70	108.0
36.90	1251.0
37.90	807.0
39.00	458.0
39.90	235.0
43.90	388.0
45.00	190.0
47.00	314.0
47.90	137.0
48.90	1383.0
49.90	4821.0
51.00	1462.0
55.80	284.0
56.90	737.0
59.80	228.0
60.90	1297.0
61.90	1400.0
63.00	1367.0
63.90	364.0
64.90	464.0
67.90	2944.0
68.90	2815.0
69.90	167.0
71.90	222.0
73.00	1412.0
74.00	5005.0
75.00	15480.0
76.00	1179.0
76.90	167.0
78.90	1154.0
79.90	429.0
80.80	1189.0
81.90	249.0
85.70	165.0
86.90	1395.0
87.90	1076.0
90.90	118.0
91.90	882.0
92.90	1375.0
94.00	4054.0
95.00	30080.0
96.00	2299.0
103.90	163.0
105.70	119.0
115.90	130.0
116.90	290.0
117.90	150.0
118.80	296.0
127.90	169.0
140.90	378.0
143.00	497.0
144.70	126.0
154.80	119.0
171.70	613.0
173.90	25912.0
175.00	1847.0
175.90	25184.0
176.90	1421.0
206.90	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122