

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
 Data File : VU051438.D
 Acq On : 18 Oct 2022 13:17
 Operator : JC/MD
 Sample : VU1018WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1018WBL01

Quant Time: Oct 19 02:47:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Oct 18 04:53:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	49002	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.635	95	13258	0.771	ug/l	0.00
Spiked Amount 1.000			Recovery	=	77.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	13822	0.720	ug/l	0.00
Spiked Amount 1.000			Recovery	=	72.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
Data File : VU051438.D
Acq On : 18 Oct 2022 13:17
Operator : JC/MD
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Time: Oct 19 02:47:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Oct 18 04:53:19 2022
Response via : Initial Calibration




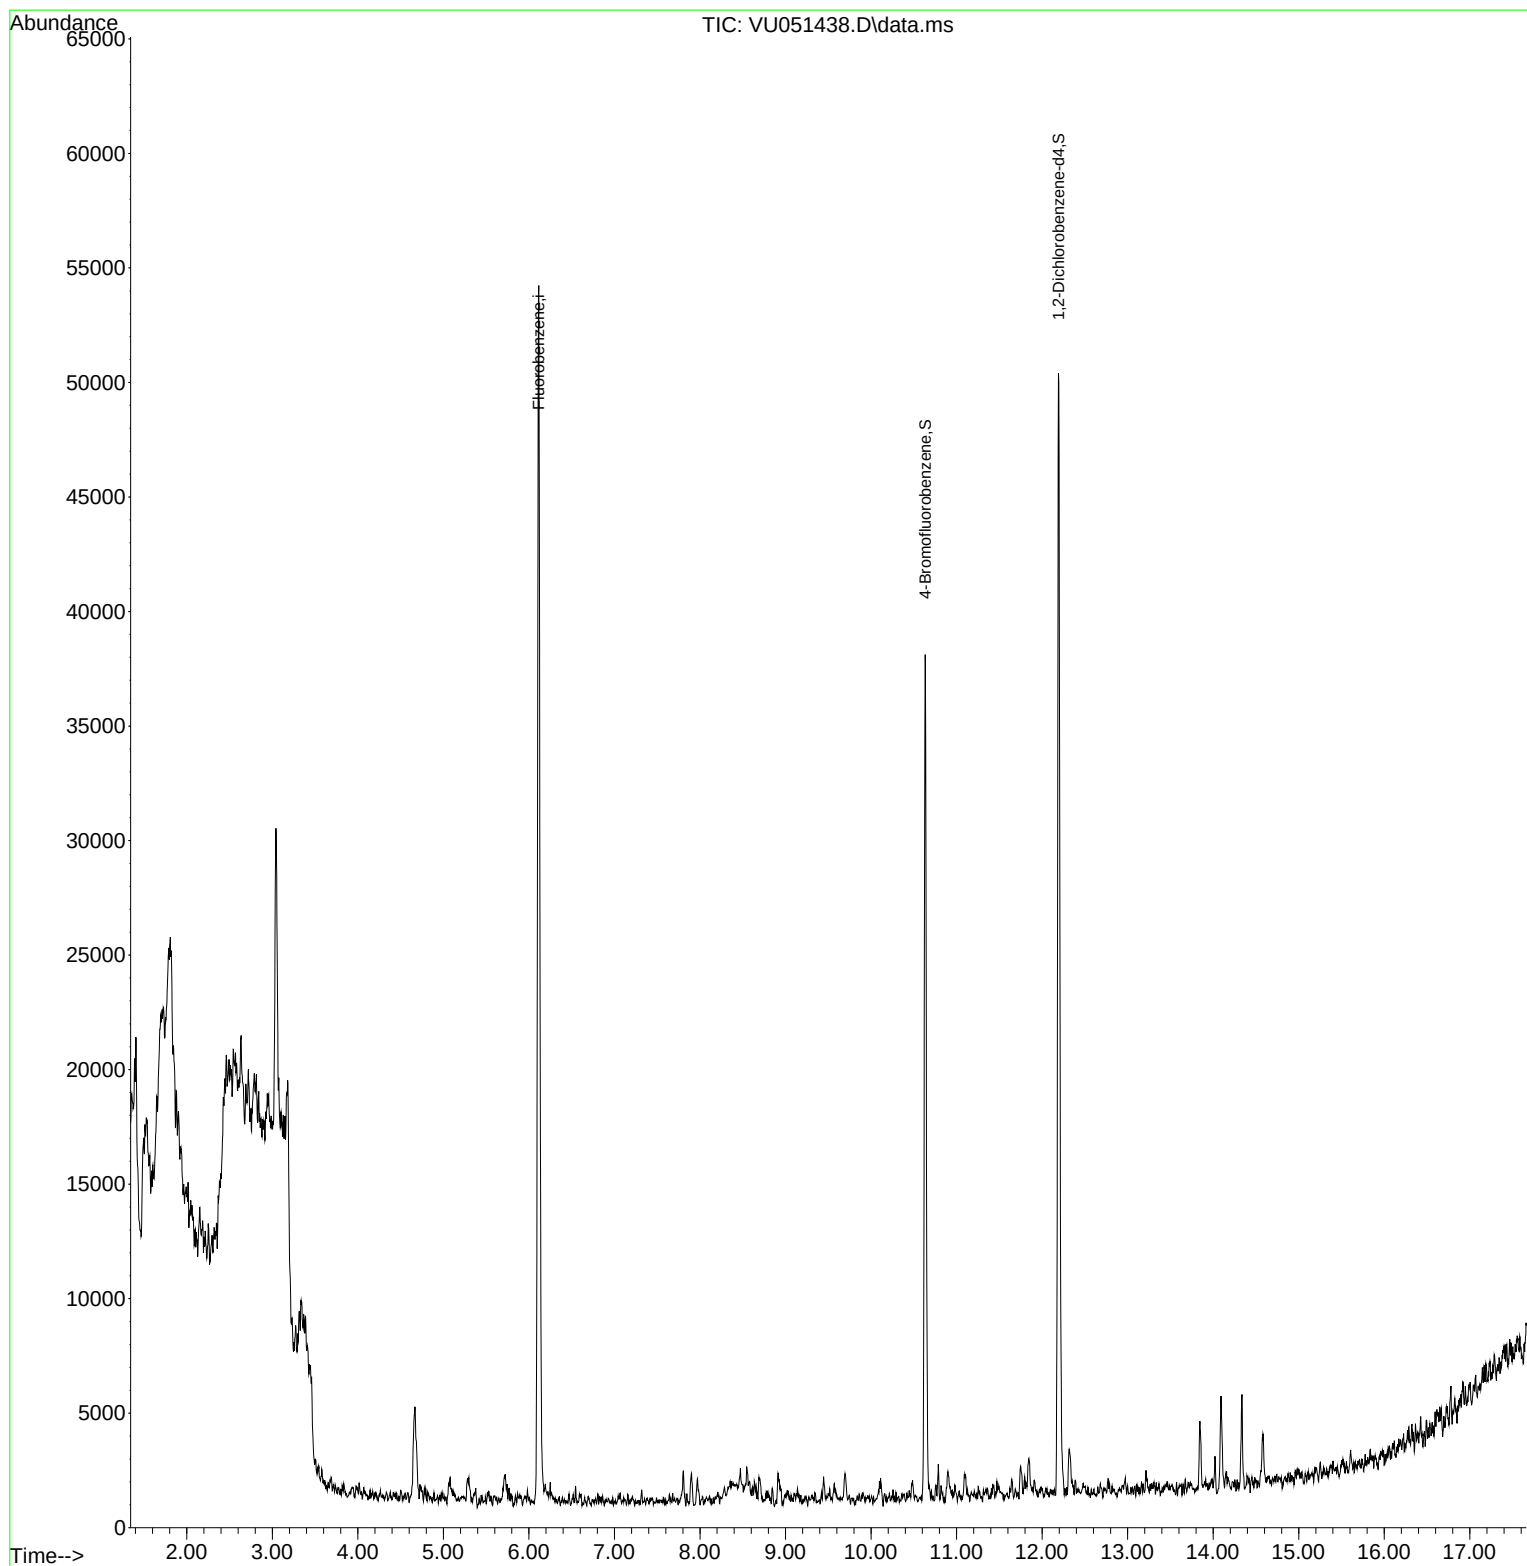


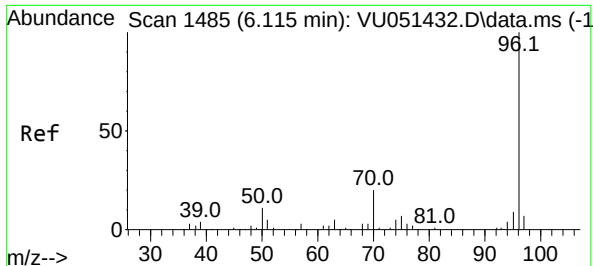

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU051438.D
Acq: 18 Oct 2022 13:17




Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01


Tgt Ion: 96	Resp: 49002
Ion Ratio	Lower Upper
96 100	
70 20.0	16.7 25.1
95 9.1	7.5 11.3
97 5.9	0.0 0.0#

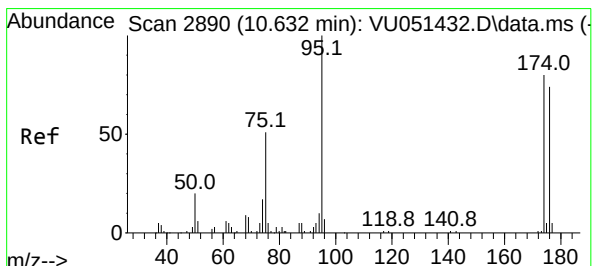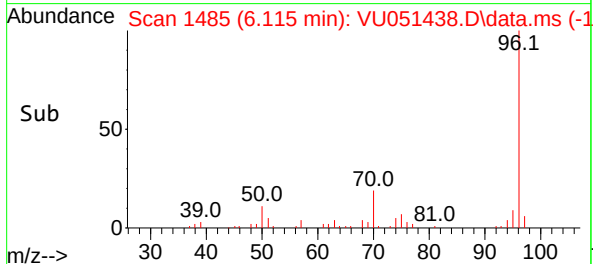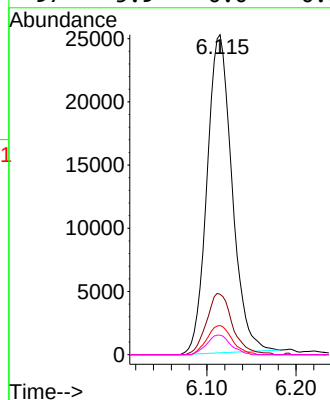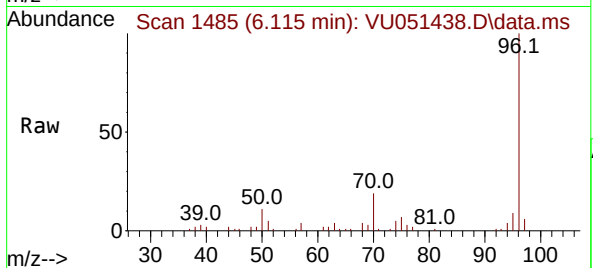

#57
4-Bromofluorobenzene
Concen: 0.771 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU051438.D
Acq: 18 Oct 2022 13:17

Tgt Ion: 95	Resp: 13258
Ion Ratio	Lower Upper
95 100	
174 77.0	63.0 94.6
176 73.6	59.8 89.6

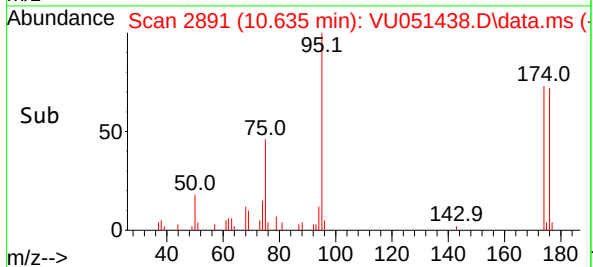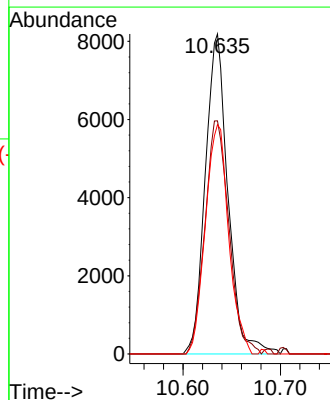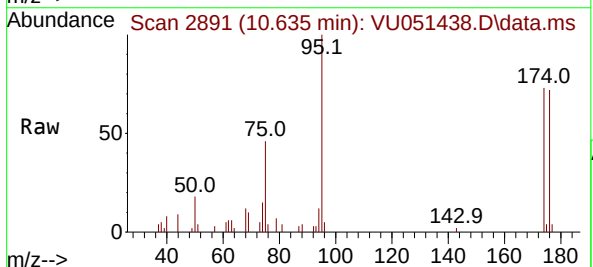

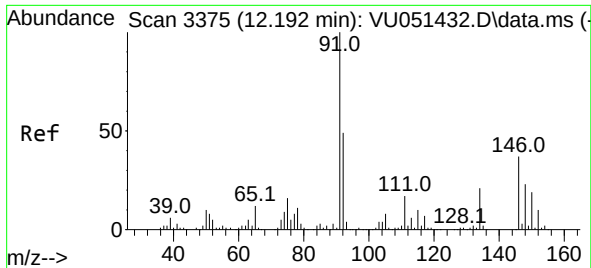

#68

1,2-Dichlorobenzene-d4

Concen: 0.720 ug/l

RT: 12.195 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU051438.D


Acq: 18 Oct 2022 13:17

Instrument :

MSVOA_U

ClientSampleId :

VU1018WBL01

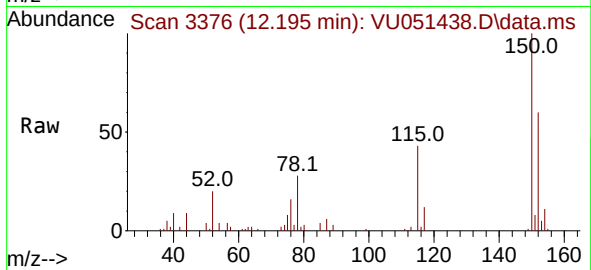

Tgt Ion:152 Resp: 13822

Ion Ratio Lower Upper

152 100

115 68.6 0.0 333.0

150 166.2 0.0 662.0

