

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
 Data File : VU051438.D
 Acq On : 18 Oct 2022 13:17
 Operator : JC/MD
 Sample : VU1018WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1018WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU051438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	525	529	538	rVB5	11433	17125	16.42%	5.190%
2	4.668	1022	1035	1050	rVB2	4034	10326	9.90%	3.129%
3	5.063	1151	1158	1160	rBV4	934	1051	1.01%	0.319%
4	5.282	1220	1226	1229	rBV4	1009	1200	1.15%	0.364%
5	5.298	1229	1231	1239	rVB3	1046	1090	1.05%	0.330%
6	5.713	1350	1360	1362	rBV4	1009	1308	1.25%	0.396%
7	6.115	1468	1485	1504	rBV	53194	104274	100.00%	31.601%
8	7.899	2033	2040	2048	rVB4	1404	2134	2.05%	0.647%
9	7.970	2052	2062	2065	rBV2	1163	1458	1.40%	0.442%
10	8.912	2350	2355	2357	rBV4	1349	1235	1.18%	0.374%
11	9.446	2516	2521	2527	rBV5	999	1111	1.07%	0.337%
12	9.697	2588	2599	2608	rBV5	1158	2002	1.92%	0.607%
13	10.111	2726	2728	2737	rVB3	1246	1388	1.33%	0.421%
14	10.632	2878	2890	2904	rBV2	36943	60083	57.62%	18.209%
15	10.786	2933	2938	2944	rVB3	1548	1410	1.35%	0.427%
16	11.095	3026	3034	3035	rBV2	1117	1154	1.11%	0.350%
17	11.748	3231	3237	3245	rBV6	1449	2482	2.38%	0.752%
18	11.844	3260	3267	3274	rBV5	1241	1918	1.84%	0.581%
19	12.192	3365	3375	3396	rVB3	48972	88538	84.91%	26.832%
20	12.317	3407	3414	3422	rBV5	2003	3762	3.61%	1.140%
21	13.844	3882	3889	3898	rBV6	2973	4316	4.14%	1.308%
22	14.021	3937	3944	3950	rVB5	1646	1811	1.74%	0.549%
23	14.092	3953	3966	3978	rBV2	4227	7382	7.08%	2.237%
24	14.336	4033	4042	4052	rVB4	4133	5386	5.17%	1.632%
25	14.581	4111	4118	4128	rVB4	2093	3347	3.21%	1.014%
26	15.253	4321	4327	4332	rBV4	840	1043	1.00%	0.316%
27	16.780	4796	4802	4806	rVB8	1671	1635	1.57%	0.496%




Sum of corrected areas: 329969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
Data File : VU051438.D
Acq On : 18 Oct 2022 13:17
Operator : JC/MD
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

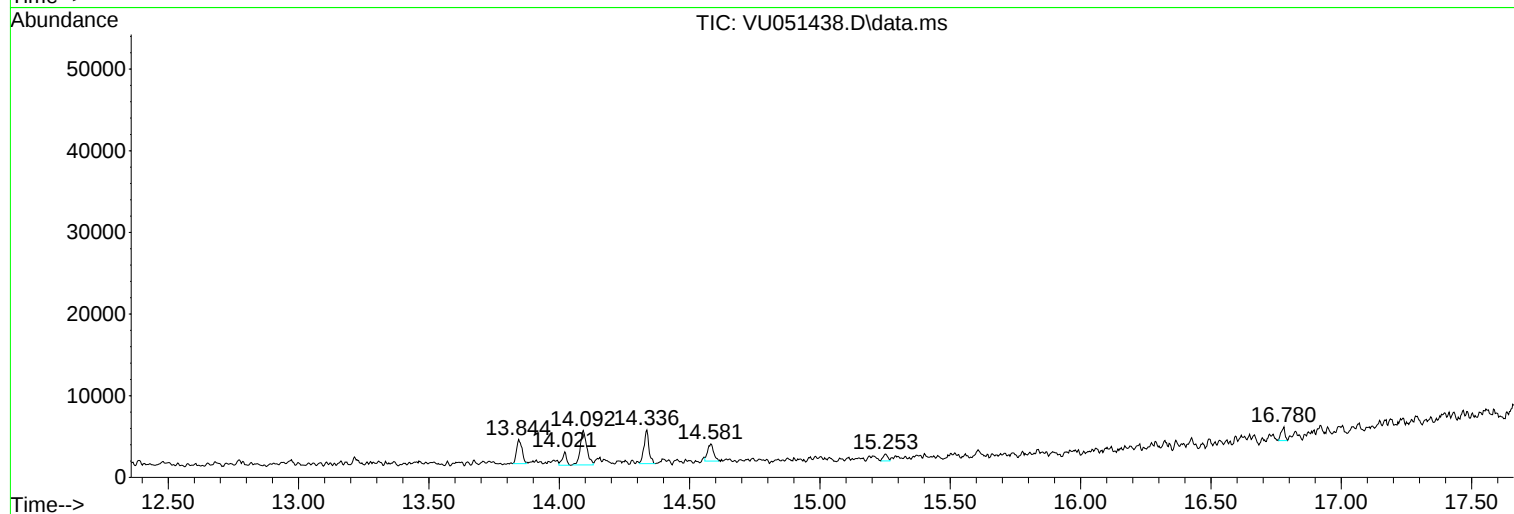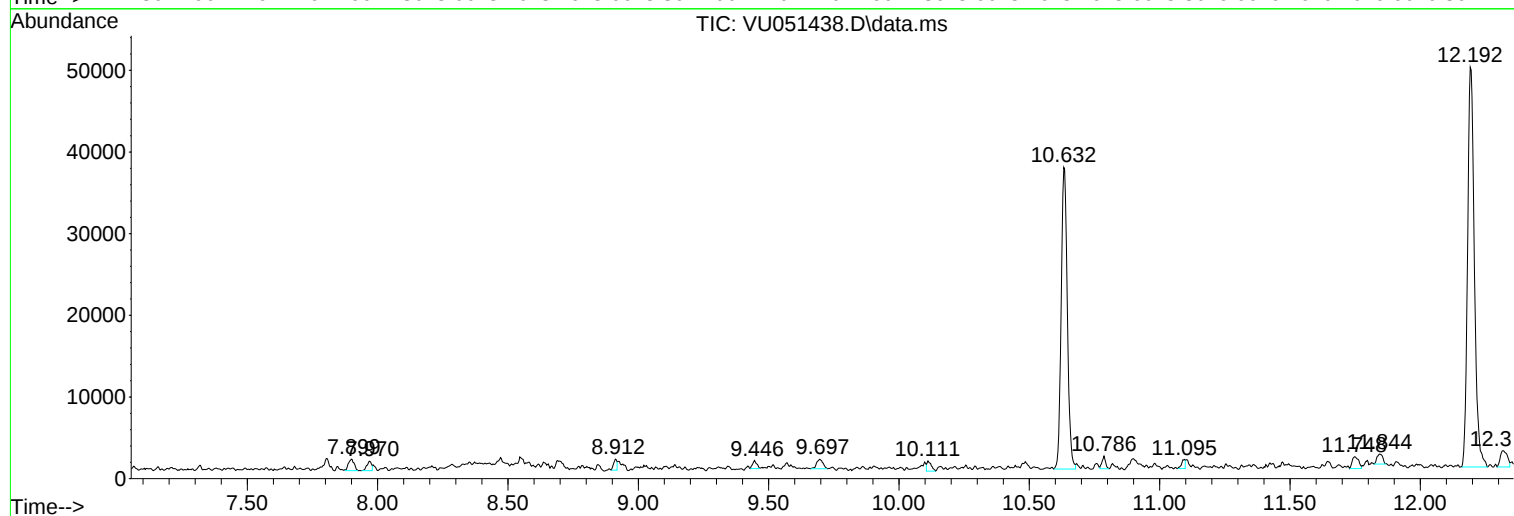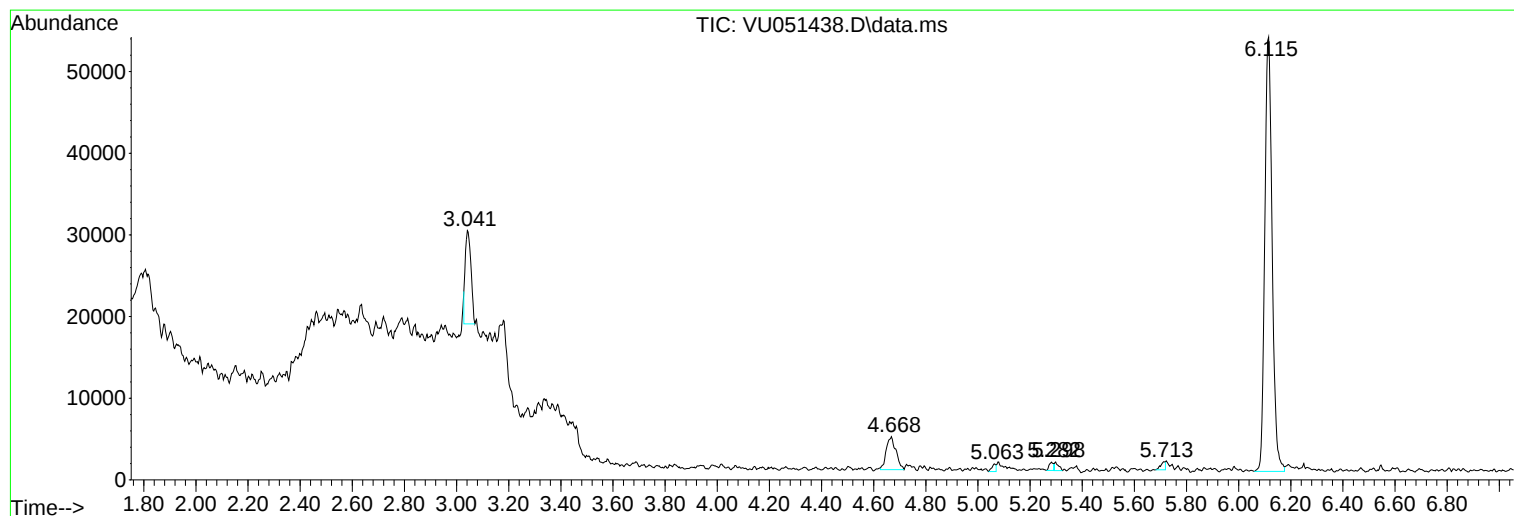

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
Data File : VU051438.D
Acq On : 18 Oct 2022 13:17
Operator : JC/MD
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101822\
Data File : VU051438.D
Acq On : 18 Oct 2022 13:17
Operator : JC/MD
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------