

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110122\
 Data File : VU051666.D
 Acq On : 01 Nov 2022 20:11
 Operator : JC/MD
 Sample : N5319-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAF2

Quant Time: Nov 02 02:06:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 02 01:48:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	186184	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	196132	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	83876	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	75043	5.352	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	107.000%	
7) Chloroethane-d5	1.909	69	68138	4.659	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.200%	
11) 1,1-Dichloroethene-d2	2.565	65	29260	5.749	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	115.000%	
20) 2-Butanone-d5	4.620	46	176941	34.842	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	69.680%	
24) Chloroform-d	5.060	84	152523	4.648	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
26) 1,2-Dichloroethane-d4	5.700	65	75097	4.237	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.800%	
32) Benzene-d6	5.726	84	289467	4.677	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
36) 1,2-Dichloropropane-d6	6.690	67	95548	4.415	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.200%	
41) Toluene-d8	7.896	98	235082	4.830	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.600%	
43) trans-1,3-Dichloroprop...	8.179	79	29948	4.526	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.629	63	139004	34.894	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	69.780%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	80470	4.057	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.200%	
66) 1,2-Dichlorobenzene-d4	12.192	152	83350	5.414	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.200%	
Target Compounds						Qvalue
13) Acetone	2.626	43	15040	5.837	ug/L	97
25) Chloroform	5.086	83	75795	2.280	ug/L	98
42) Toluene	7.970	91	20248	0.255	ug/L	94
53) m,p-Xylene	9.690	106	3801	0.128	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110122\
Data File : VU051666.D
Acq On : 01 Nov 2022 20:11
Operator : JC/MD
Sample : N5319-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAf2

Quant Time: Nov 02 02:06:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 02 01:48:00 2022
Response via : Initial Calibration

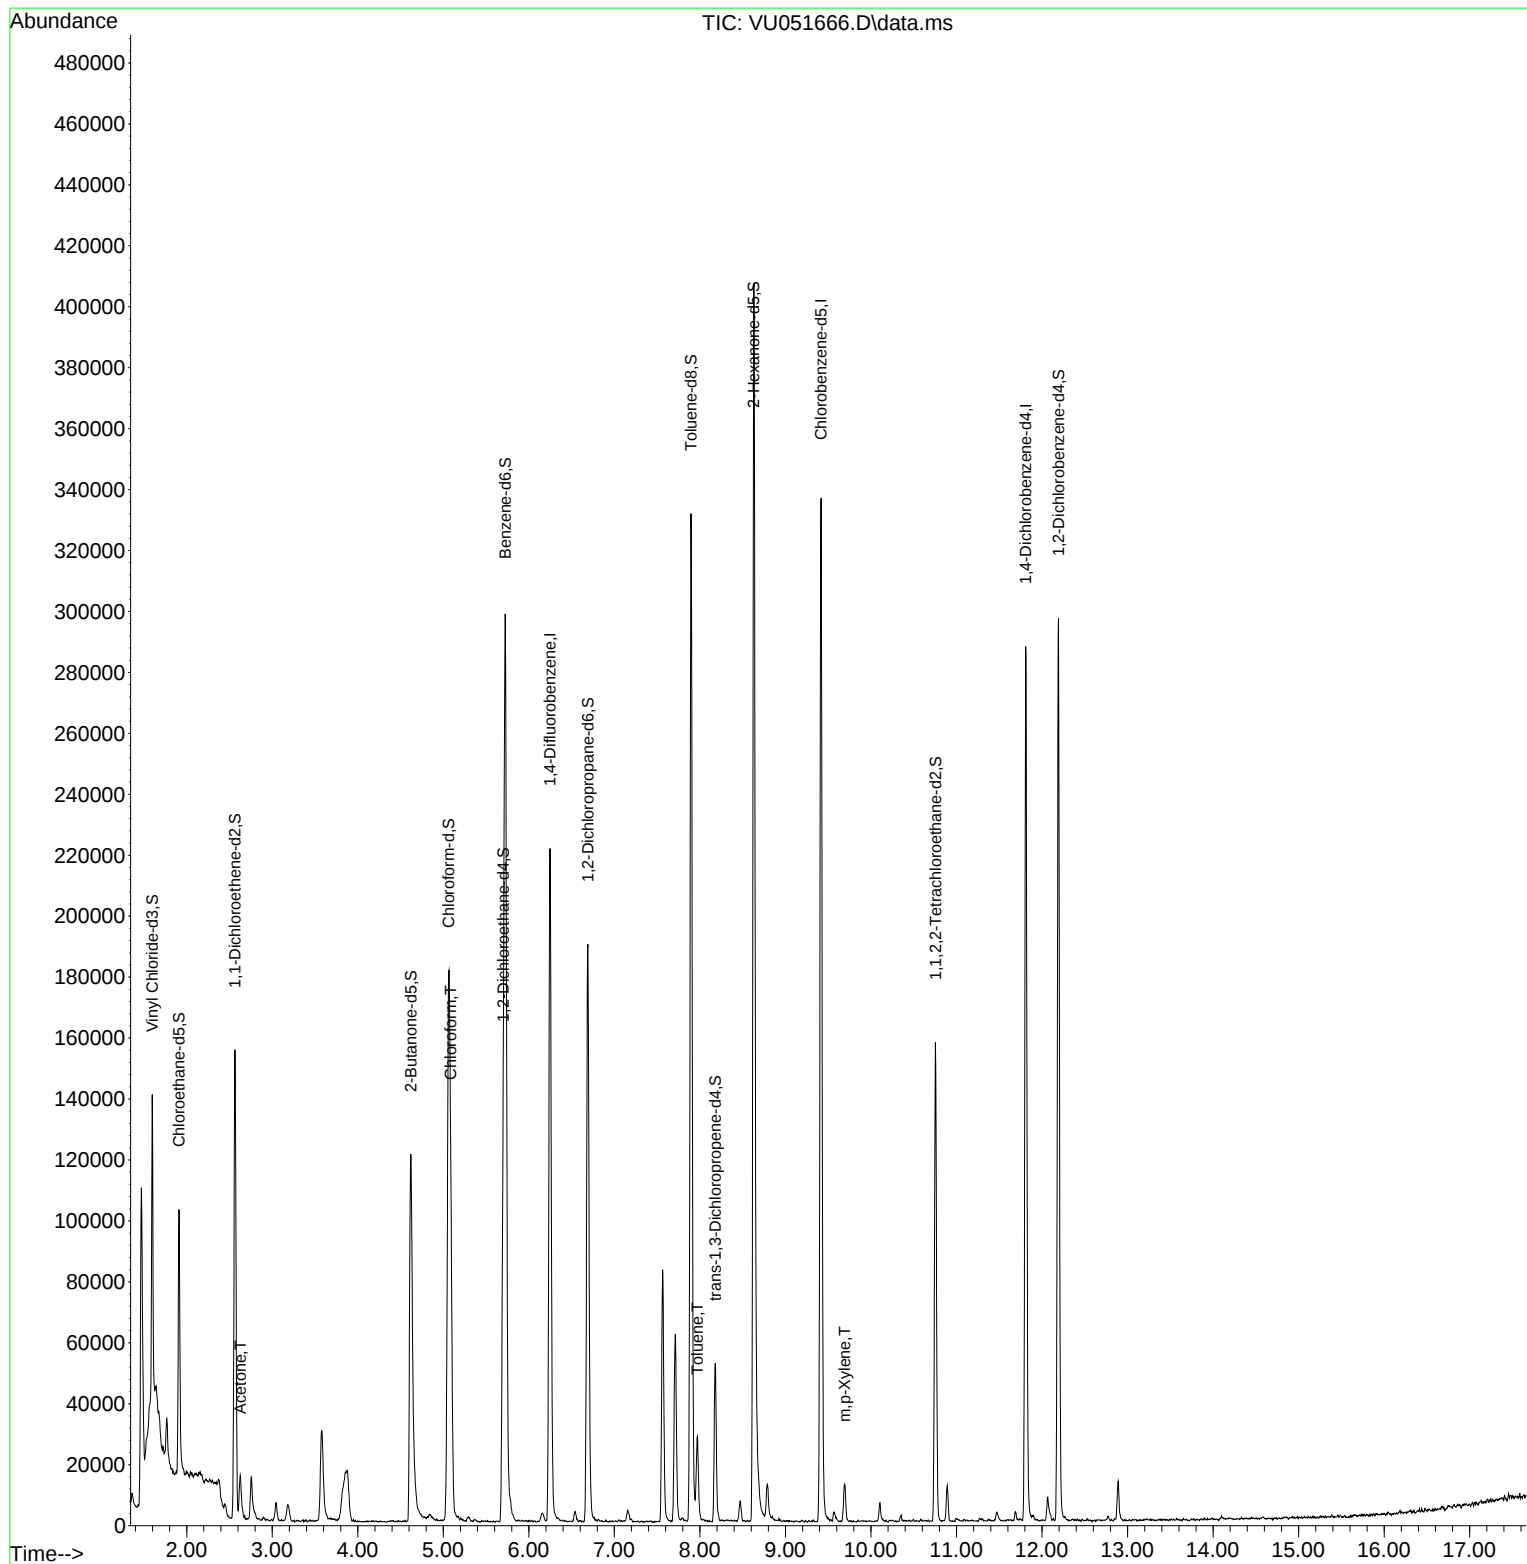

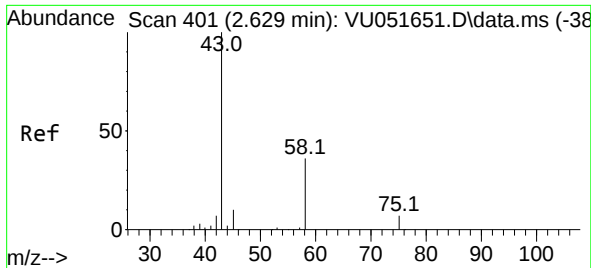

#13

Acetone

Concen: 5.837 ug/L

RT: 2.626 min Scan# 401

Delta R.T. -0.003 min

Lab File: VU051666.D

Acq: 01 Nov 2022 20:11

Instrument :

MSVOA_U

ClientSampleId :





BHAF2

Tgt Ion: 43 Resp: 15040

Ion Ratio Lower Upper

43 100

58 35.3 0.0 73.8

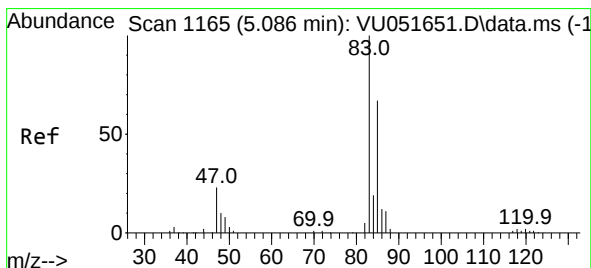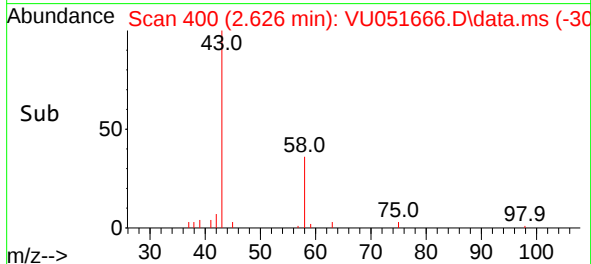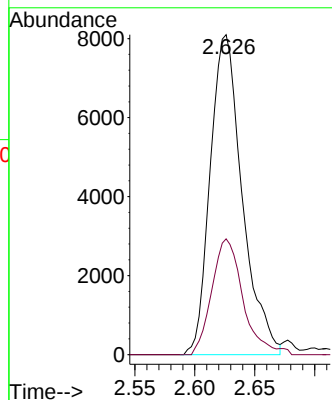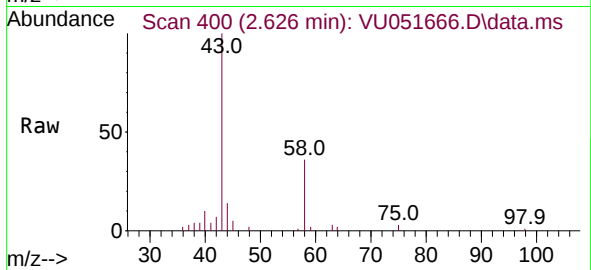

#25

Chloroform

Concen: 2.280 ug/L

RT: 5.086 min Scan# 1165

Delta R.T. -0.000 min

Lab File: VU051666.D




Acq: 01 Nov 2022 20:11


Tgt Ion: 83 Resp: 75795

Ion Ratio Lower Upper

83 100

85 66.5 45.2 84.0

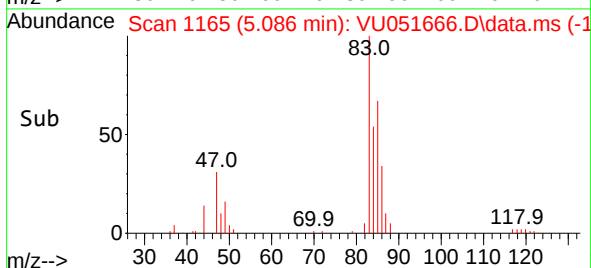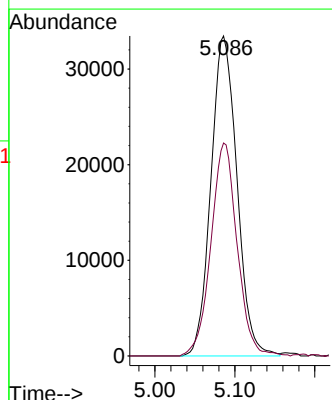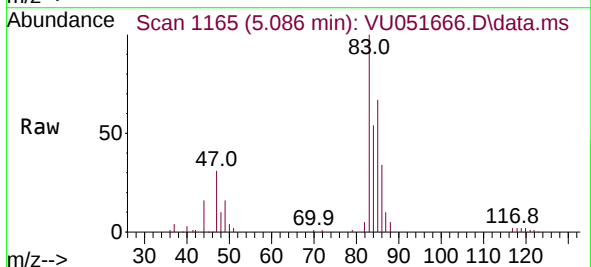

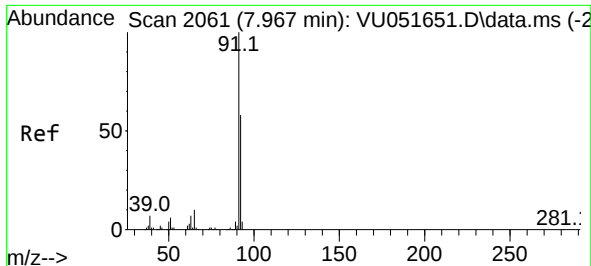

#42

Toluene

Concen: 0.255 ug/L

RT: 7.970 min Scan# 2061

Delta R.T. 0.003 min

Lab File: VU051666.D

Acq: 01 Nov 2022 20:11

Instrument :

MSVOA_U

ClientSampleId :





BHAF2

Tgt Ion: 91 Resp: 20248

Ion Ratio Lower Upper

91 100

92 53.6 40.5 75.3

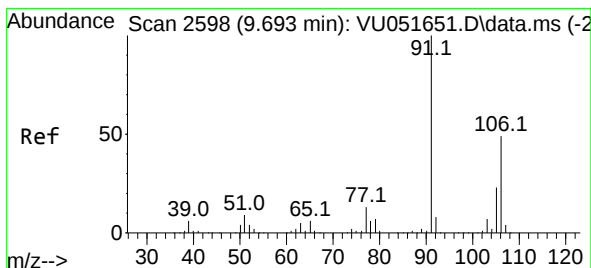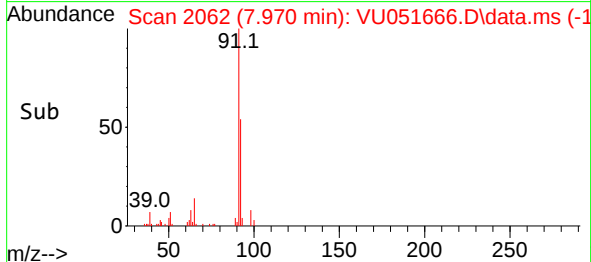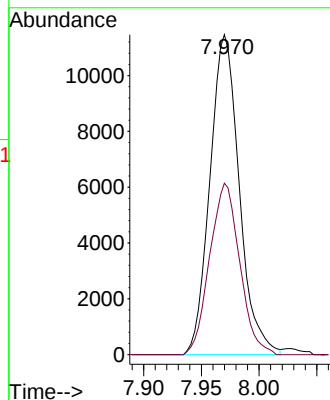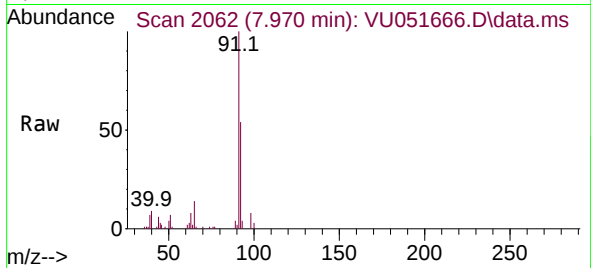

#53

m,p-Xylene

Concen: 0.128 ug/L

RT: 9.690 min Scan# 2597

Delta R.T. -0.003 min

Lab File: VU051666.D

Acq: 01 Nov 2022 20:11

Tgt Ion: 106 Resp: 3801

Ion Ratio Lower Upper

106 100

91 199.8 139.4 259.0

