

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110122\
 Data File : VU051668.D
 Acq On : 01 Nov 2022 21:56
 Operator : JC/MD
 Sample : VU1101WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK127

Quant Time: Nov 02 03:07:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 02 03:06:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	183663	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	194856	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	78406	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	75982	5.493	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	109.800%	
7) Chloroethane-d5	1.913	69	68709	4.763	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.200%	
11) 1,1-Dichloroethene-d2	2.565	65	31483	6.271	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	125.400%#	
20) 2-Butanone-d5	4.636	46	188902	37.708	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	75.420%	
24) Chloroform-d	5.064	84	151729	4.687	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	5.700	65	76617	4.382	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.600%	
32) Benzene-d6	5.726	84	294932	4.796	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	6.687	67	98936	4.601	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.000%	
41) Toluene-d8	7.896	98	232385	4.806	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.200%	
43) trans-1,3-Dichloroprop...	8.179	79	29195	4.441	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.800%	
46) 2-Hexanone-d5	8.633	63	142189	35.927	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	71.860%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	80875	4.104	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	82.000%	
66) 1,2-Dichlorobenzene-d4	12.192	152	80211	5.574	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.400%	
Target Compounds						Qvalue
16) Methylene chloride	3.044	84	7375	0.282	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110122\
Data File : VU051668.D
Acq On : 01 Nov 2022 21:56
Operator : JC/MD
Sample : VU1101WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK127

Quant Time: Nov 02 03:07:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 02 03:06:15 2022
Response via : Initial Calibration

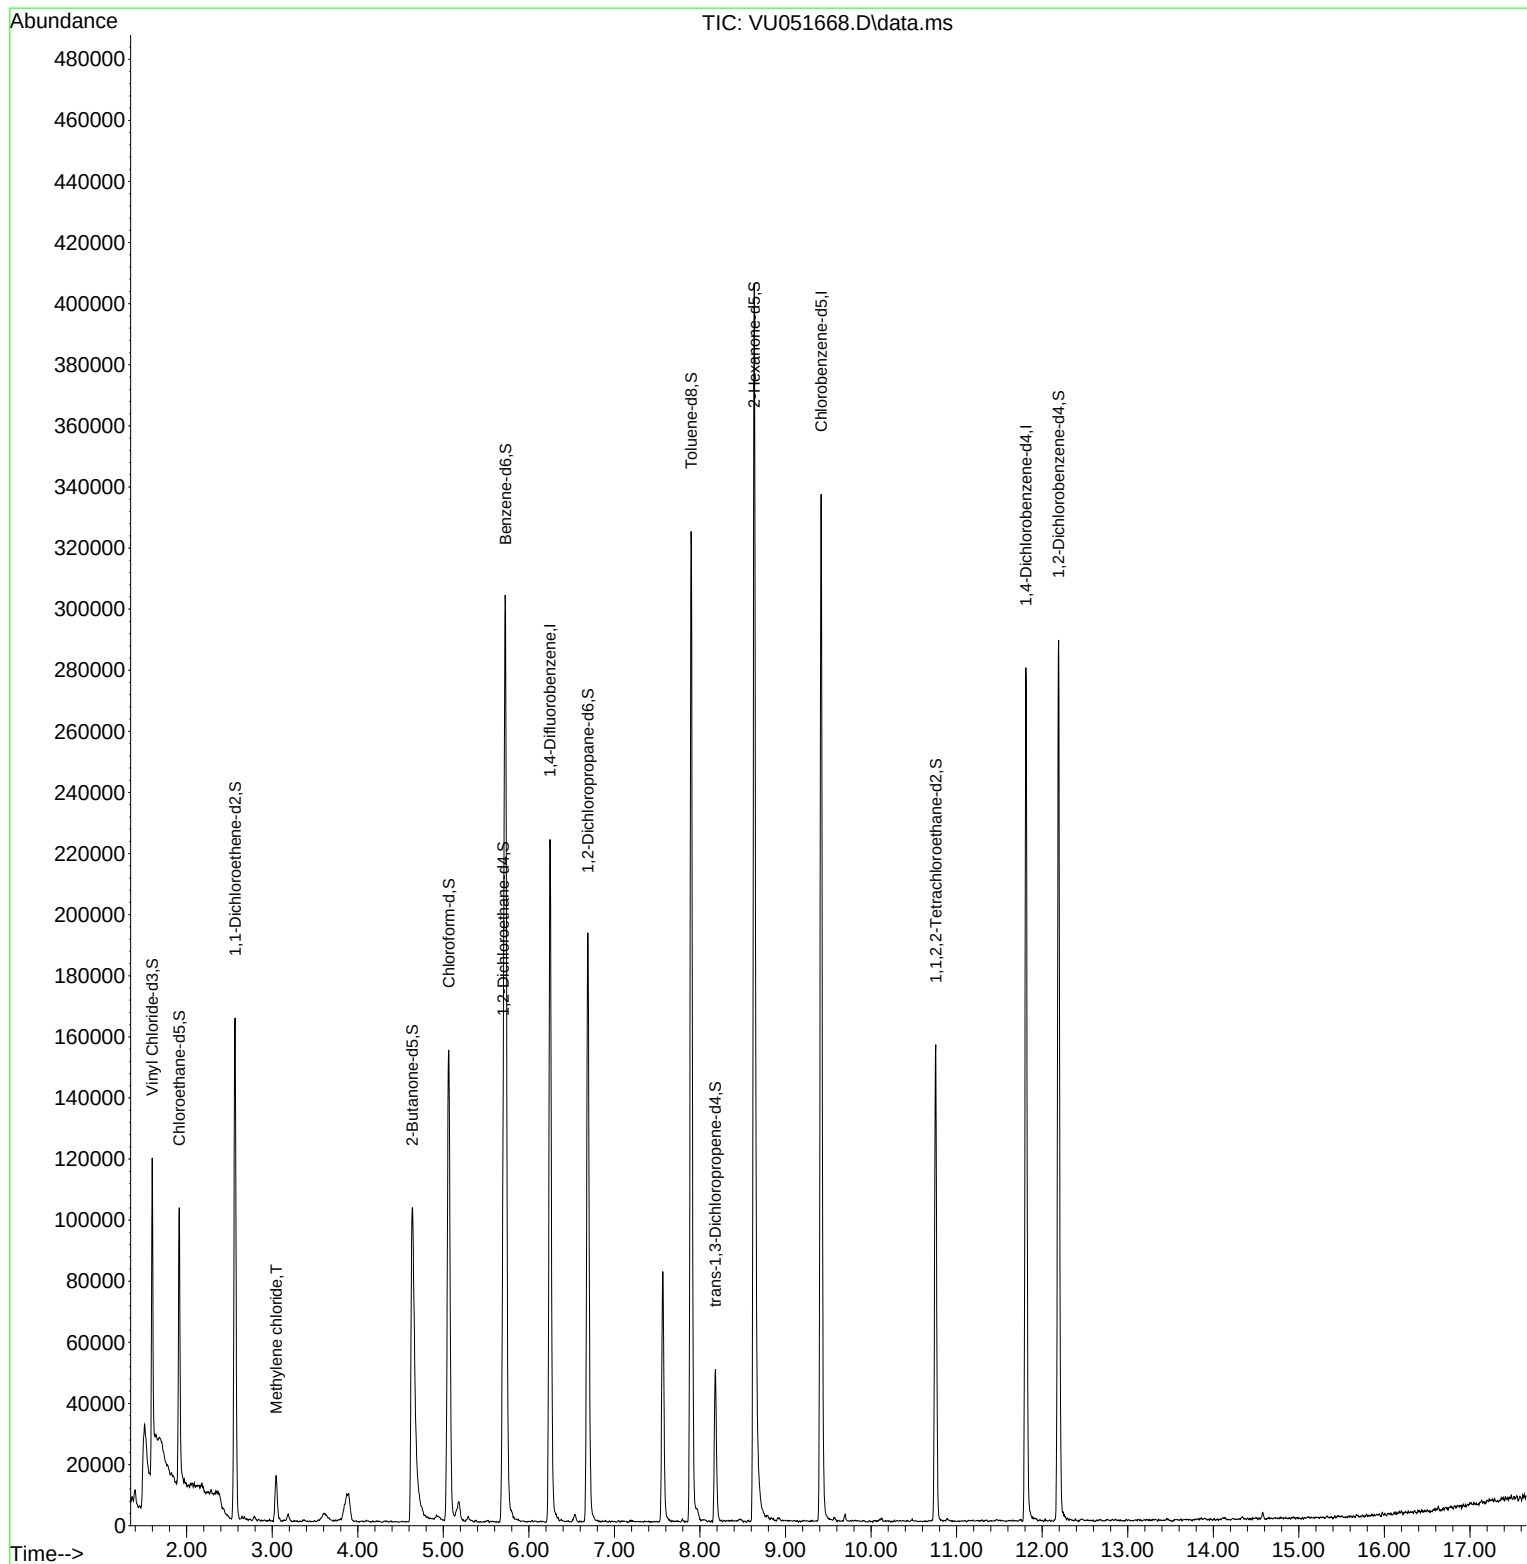

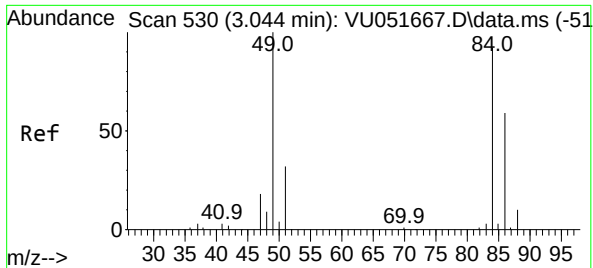

#16
Methylene chloride
Concen: 0.282 ug/L
RT: 3.044 min Scan# 51
Delta R.T. 0.000 min
Lab File: VU051668.D
Acq: 01 Nov 2022 21:56

Instrument :
MSVOA_U
ClientSampleId :
VBLK127

Tgt Ion:	84	Resp:	7375
Ion	Ratio	Lower	Upper
84	100		
86	72.2	46.3	85.9
49	119.8	76.0	141.2

