

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110725\
 Data File : VU063679.D
 Acq On : 07 Nov 2025 10:42
 Operator : MD/SY
 Sample : VU1107WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1107WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.081	1480	1490	1507	rBV	57848	117074	84.24%	24.359%
2	6.512	1618	1624	1627	rBV6	1746	1758	1.26%	0.366%
3	7.795	2016	2023	2027	rBV5	1547	2387	1.72%	0.497%
4	7.878	2042	2049	2057	rVB5	2100	2997	2.16%	0.624%
5	9.402	2513	2523	2525	rBV6	1832	2417	1.74%	0.503%
6	9.679	2598	2609	2617	rBV5	2777	4344	3.13%	0.904%
7	10.090	2727	2737	2749	rBV8	2004	3878	2.79%	0.807%
8	10.460	2845	2852	2860	rBV3	1296	1673	1.20%	0.348%
9	10.614	2889	2900	2921	rBV2	57631	105337	75.79%	21.917%
10	10.762	2937	2946	2952	rBV8	1438	1944	1.40%	0.404%
11	10.884	2979	2984	2995	rVB6	2824	4151	2.99%	0.864%
12	10.965	3001	3009	3016	rBV4	1515	2469	1.78%	0.514%
13	11.077	3035	3044	3056	rBV9	3358	5870	4.22%	1.221%
14	11.392	3135	3142	3152	rVB4	2269	3045	2.19%	0.634%
15	11.447	3152	3159	3167	rBV4	2489	3666	2.64%	0.763%
16	11.624	3205	3214	3223	rVB5	3119	5024	3.61%	1.045%
17	11.730	3237	3247	3253	rBV8	2236	3419	2.46%	0.711%
18	11.772	3253	3260	3265	rBV6	3537	4613	3.32%	0.960%
19	11.820	3271	3275	3287	rVB7	3440	5235	3.77%	1.089%
20	12.171	3373	3384	3402	rBV2	70876	138982	100.00%	28.918%
21	13.823	3888	3898	3910	rVB4	7897	14375	10.34%	2.991%
22	13.994	3945	3951	3961	rVB6	2806	3688	2.65%	0.767%
23	14.068	3965	3974	3987	rBV	12828	23925	17.21%	4.978%
24	14.306	4037	4048	4060	rVB3	9522	16719	12.03%	3.479%
25	14.560	4123	4127	4135	rVB4	1234	1622	1.17%	0.337%




Sum of corrected areas: 480612

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110725\
Data File : VU063679.D
Acq On : 07 Nov 2025 10:42
Operator : MD/SY
Sample : VU1107WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1107WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

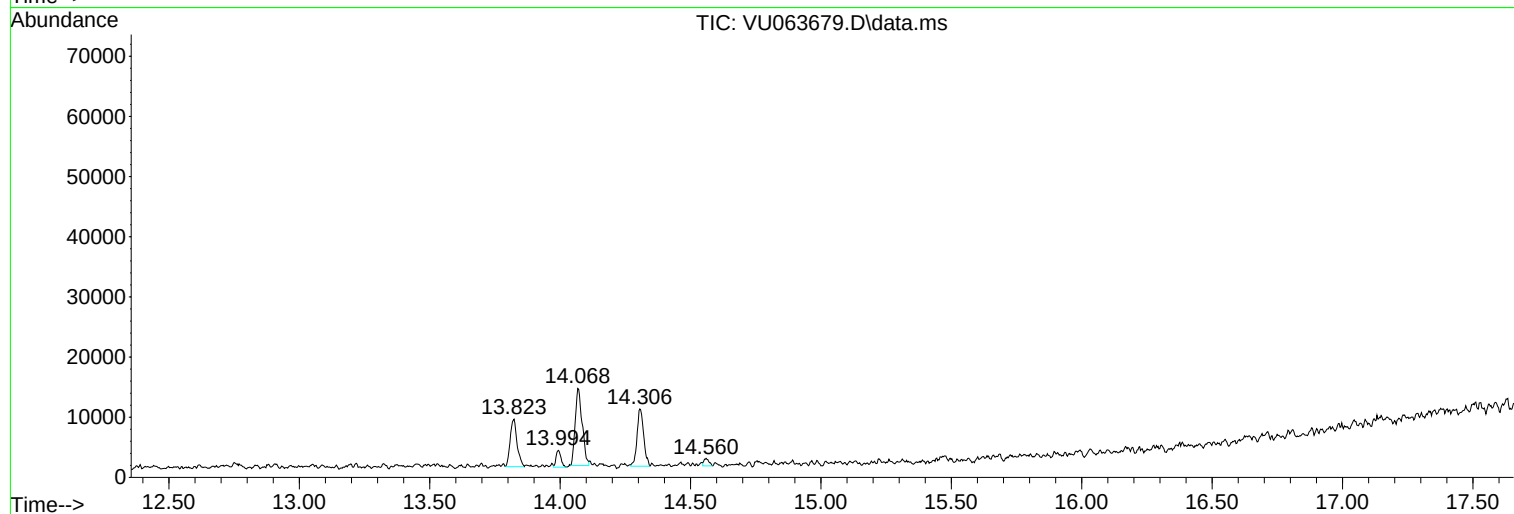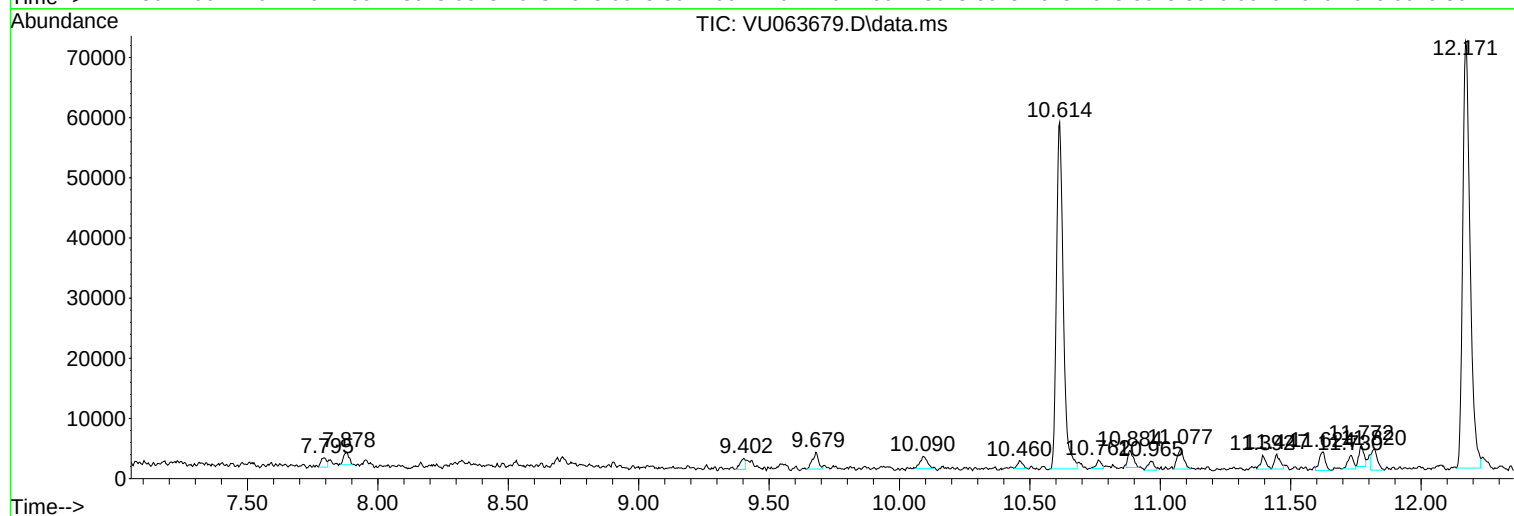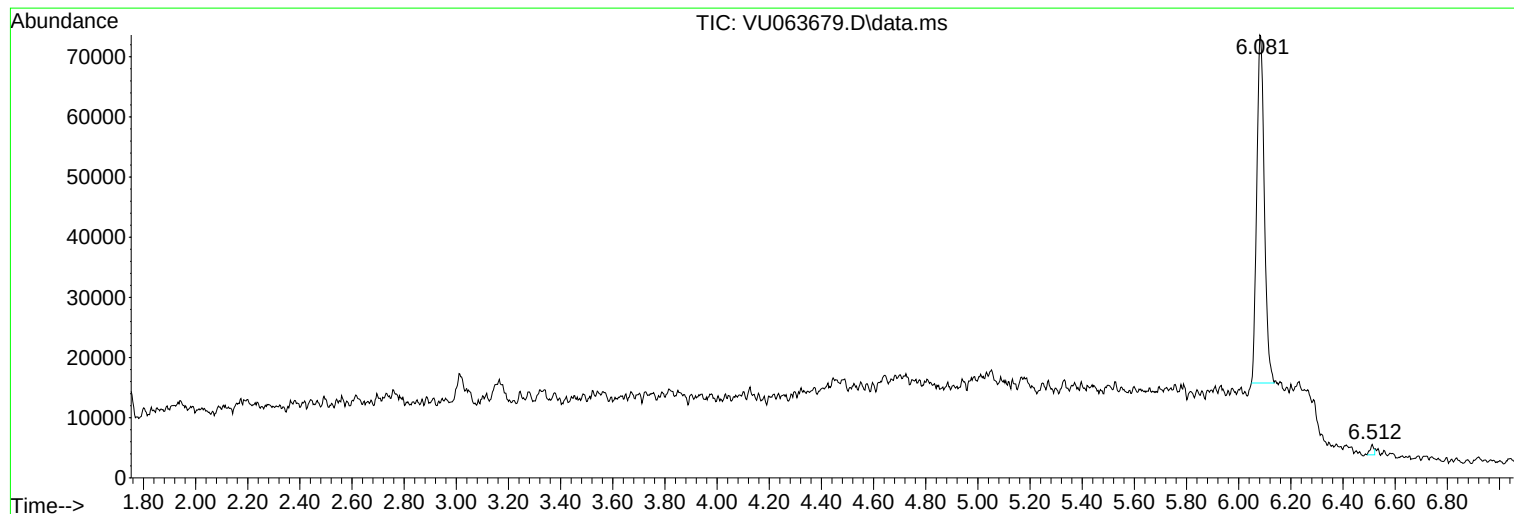

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110725\
Data File : VU063679.D
Acq On : 07 Nov 2025 10:42
Operator : MD/SY
Sample : VU1107WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1107WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110725\
Data File : VU063679.D
Acq On : 07 Nov 2025 10:42
Operator : MD/SY
Sample : VU1107WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1107WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------