
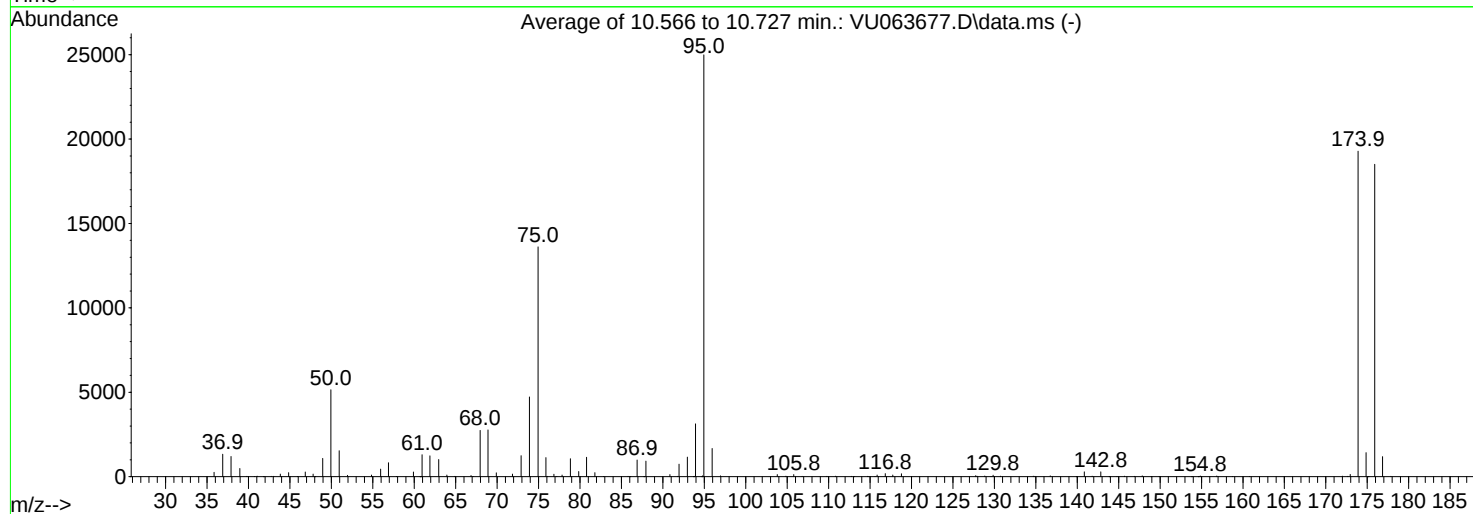


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110725\
Data File : VU063677.D
Acq On : 07 Nov 2025 08:04
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Nov 03 00:51:51 2025

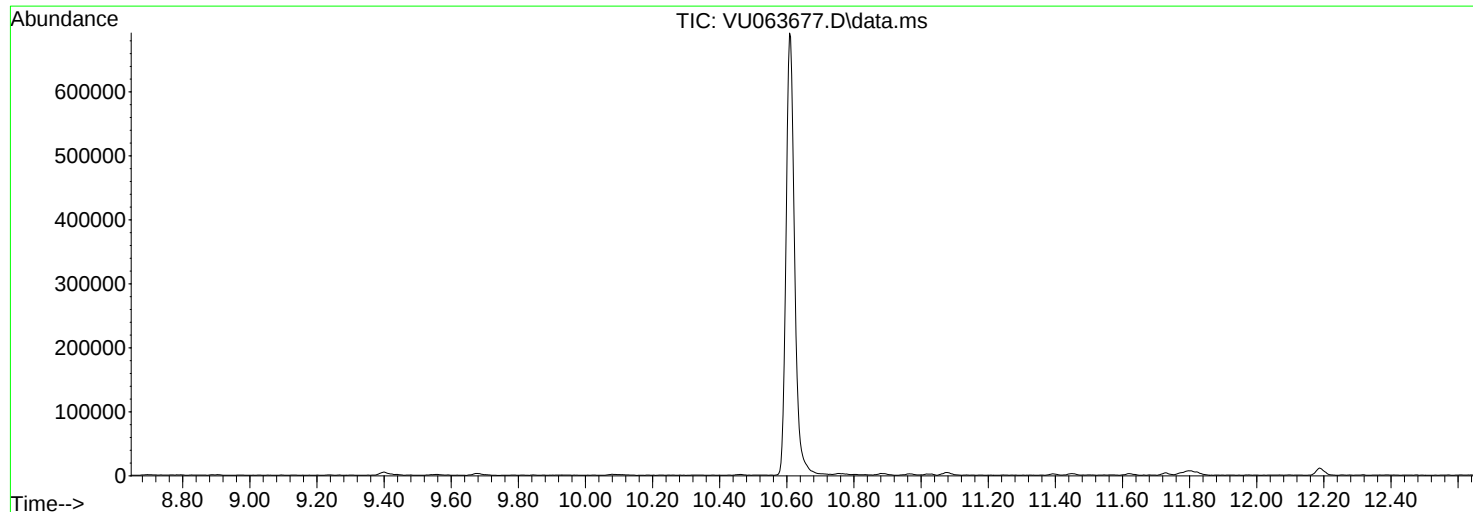

AutoFind: Averaged scan 2885 to 2935; Bkg corrected with scan 2884

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	5150	PASS
75	95	30	60	54.5	13616	PASS
95	95	100	100	100.0	24990	PASS
96	95	5	9	6.7	1670	PASS
173	174	0.00	2	0.7	136	PASS
174	95	50	100	77.2	19281	PASS
175	174	5	9	7.4	1422	PASS
176	174	95	101	96.0	18504	PASS
177	176	5	9	6.4	1186	PASS