

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123021\
 Data File : VU046647.D
 Acq On : 30 Dec 2021 14:29
 Operator : SY/MD
 Sample : VU1230WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1230WBL01

Quant Time: Dec 31 07:24:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U123021DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Dec 30 12:44:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	18399	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	5146	0.786	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	5739	0.810	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123021\
Data File : VU046647.D
Acq On : 30 Dec 2021 14:29
Operator : SY/MD
Sample : VU1230WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1230WBL01

Quant Time: Dec 31 07:24:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U123021DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Dec 30 12:44:59 2021
Response via : Initial Calibration




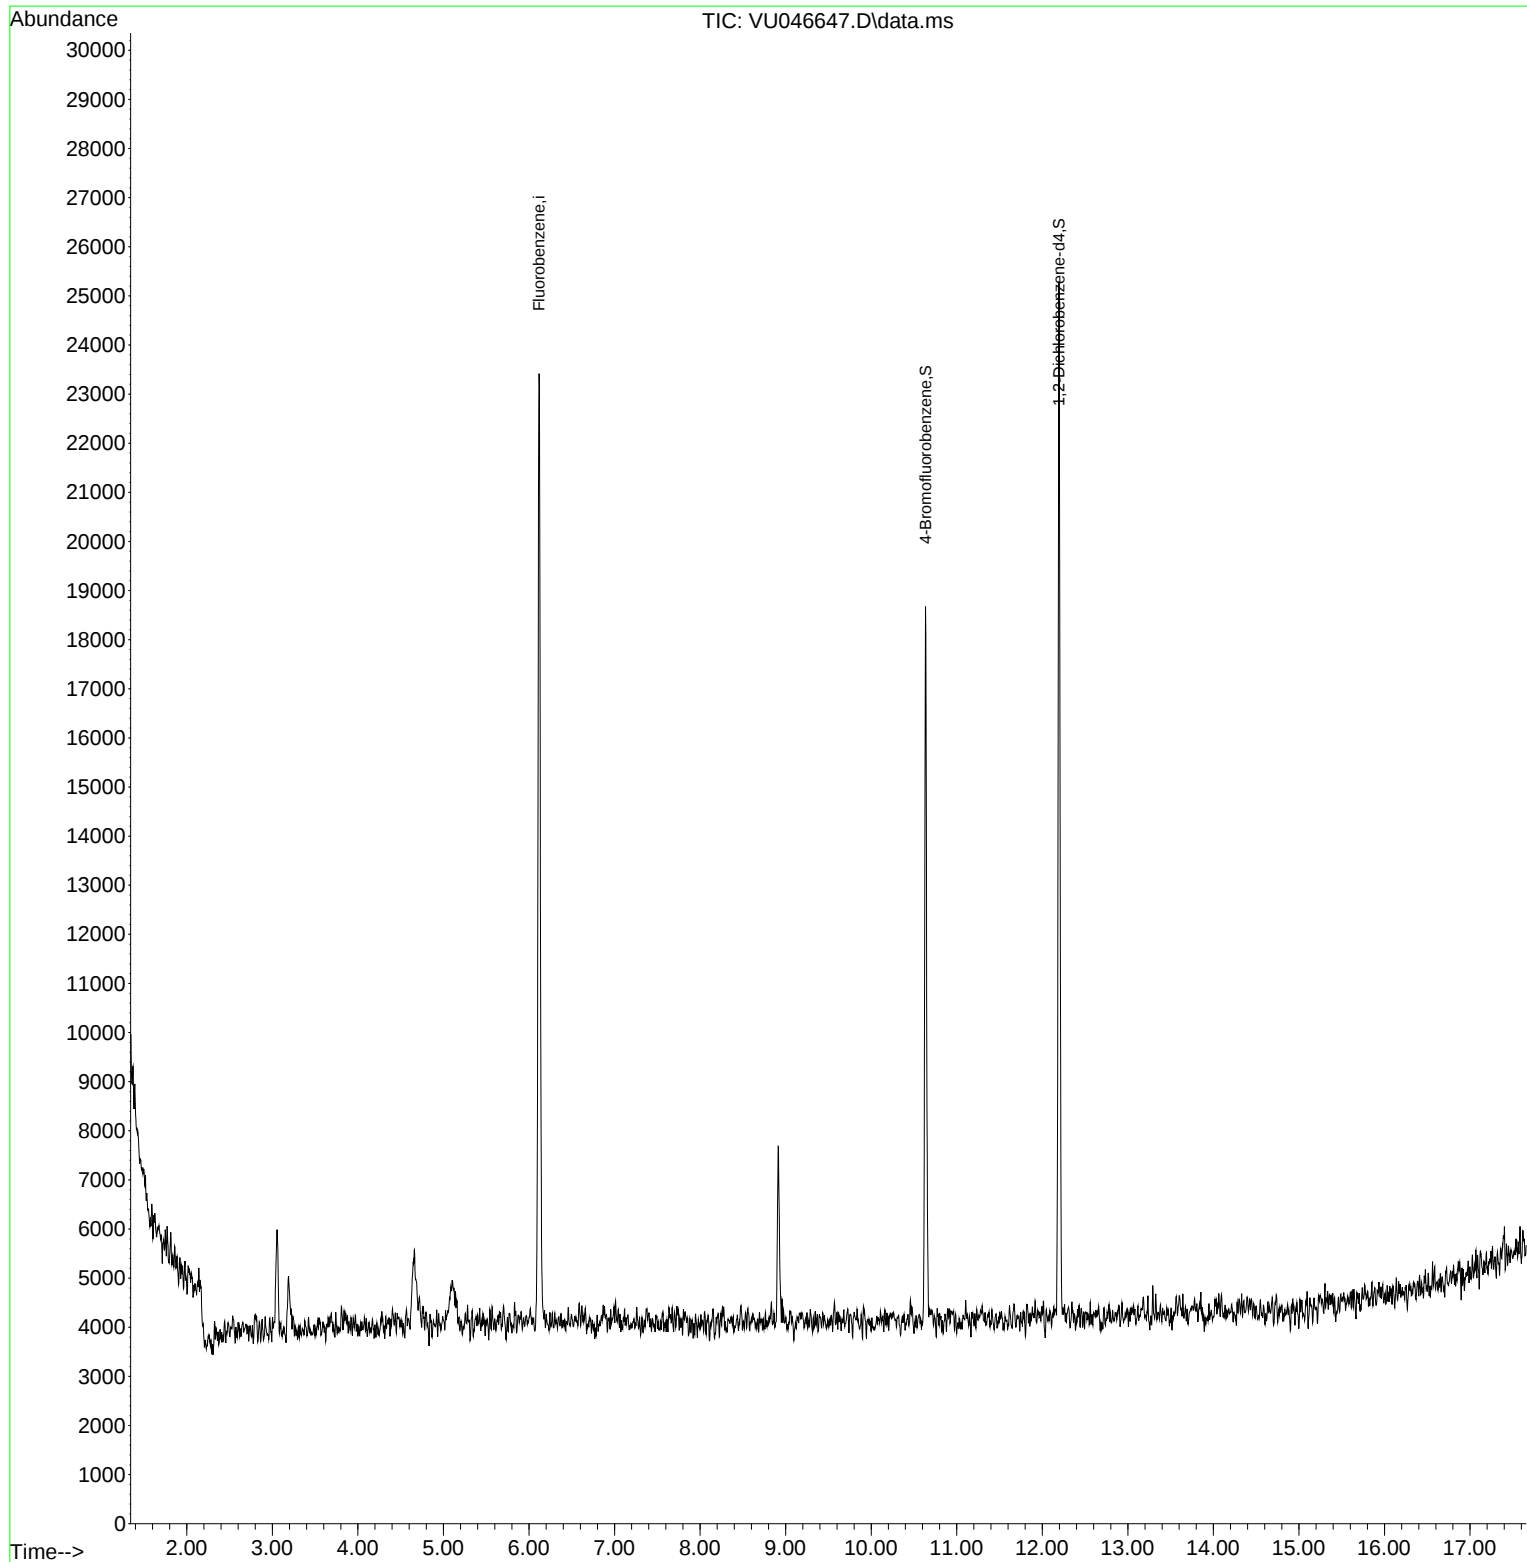


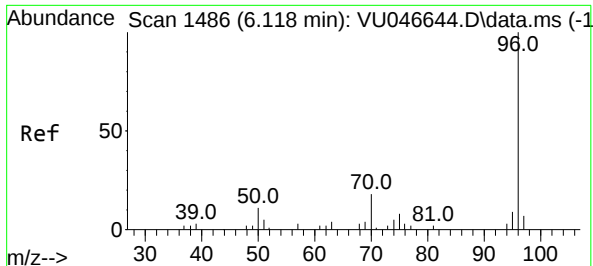

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU046647.D
Acq: 30 Dec 2021 14:29




Instrument :
MSVOA_U
ClientSampleId :
VU1230WBL01


Tgt Ion: 96	Resp: 18399
Ion Ratio	Lower Upper
96 100	
70 20.3	16.8 25.2
95 8.8	7.3 10.9
97 5.8	0.0 0.0#

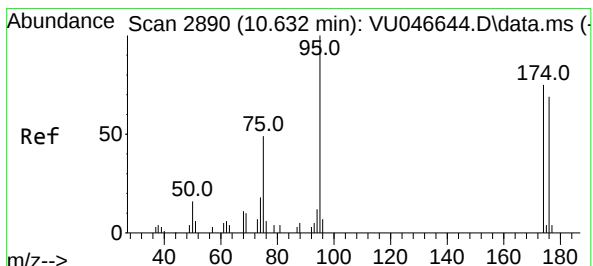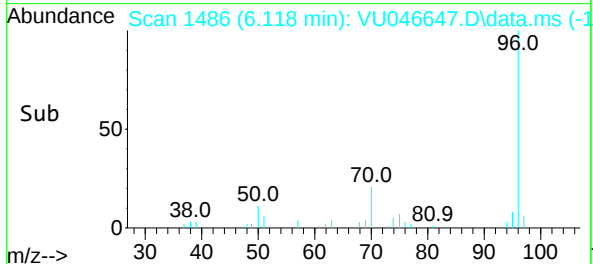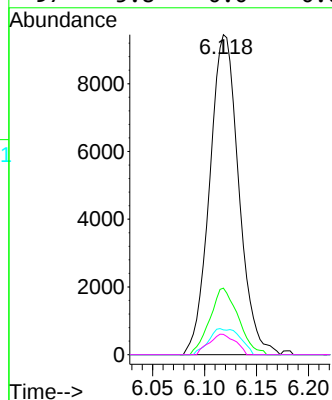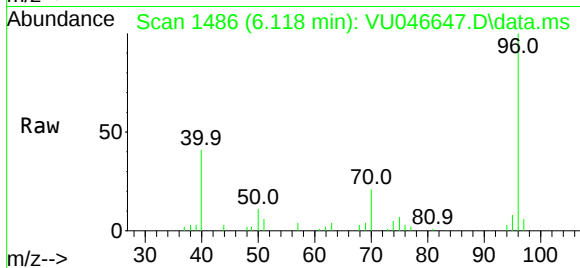

#57
4-Bromofluorobenzene
Concen: 0.786 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.004 min
Lab File: VU046647.D
Acq: 30 Dec 2021 14:29


Tgt Ion: 95	Resp: 5146
Ion Ratio	Lower Upper
95 100	
174 84.2	56.6 84.8
176 73.8	54.3 81.5

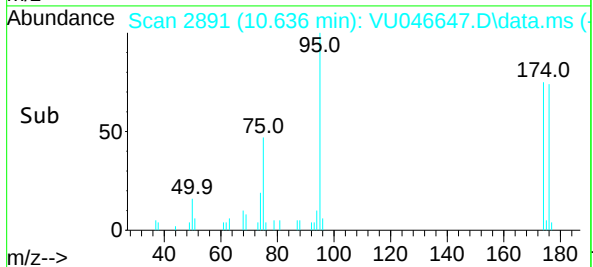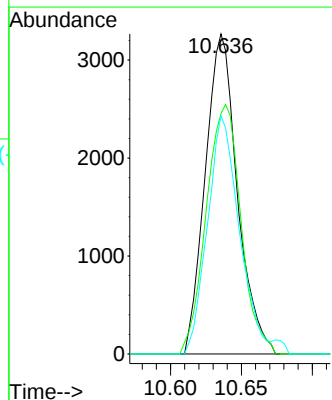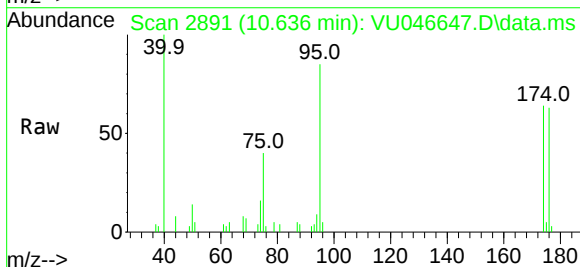

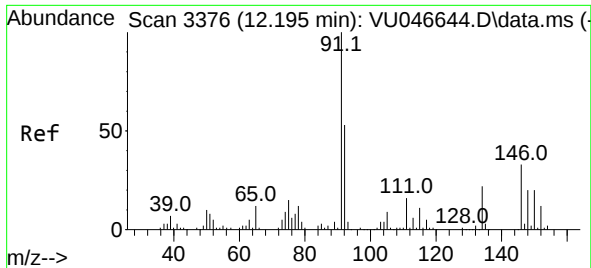

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.810 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU046647.D
 Acq: 30 Dec 2021 14:29

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1230WBL01

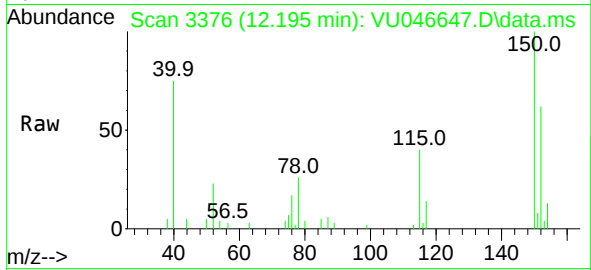

Tgt Ion:	152	Resp:	5739
Ion Ratio	Lower	Upper	
152	100		
115	63.9	0.0	251.0
150	161.8	0.0	613.8

