

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123021\
 Data File : VU046650.D
 Acq On : 30 Dec 2021 15:48
 Operator : SY/MD
 Sample : M5221-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-122221

Quant Time: Dec 31 07:25:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U123021DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Dec 30 12:44:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	18273	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.635	95	5089	0.783	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	6011	0.854	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123021\
Data File : VU046650.D
Acq On : 30 Dec 2021 15:48
Operator : SY/MD
Sample : M5221-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-01-122221

Quant Time: Dec 31 07:25:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U123021DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Dec 30 12:44:59 2021
Response via : Initial Calibration




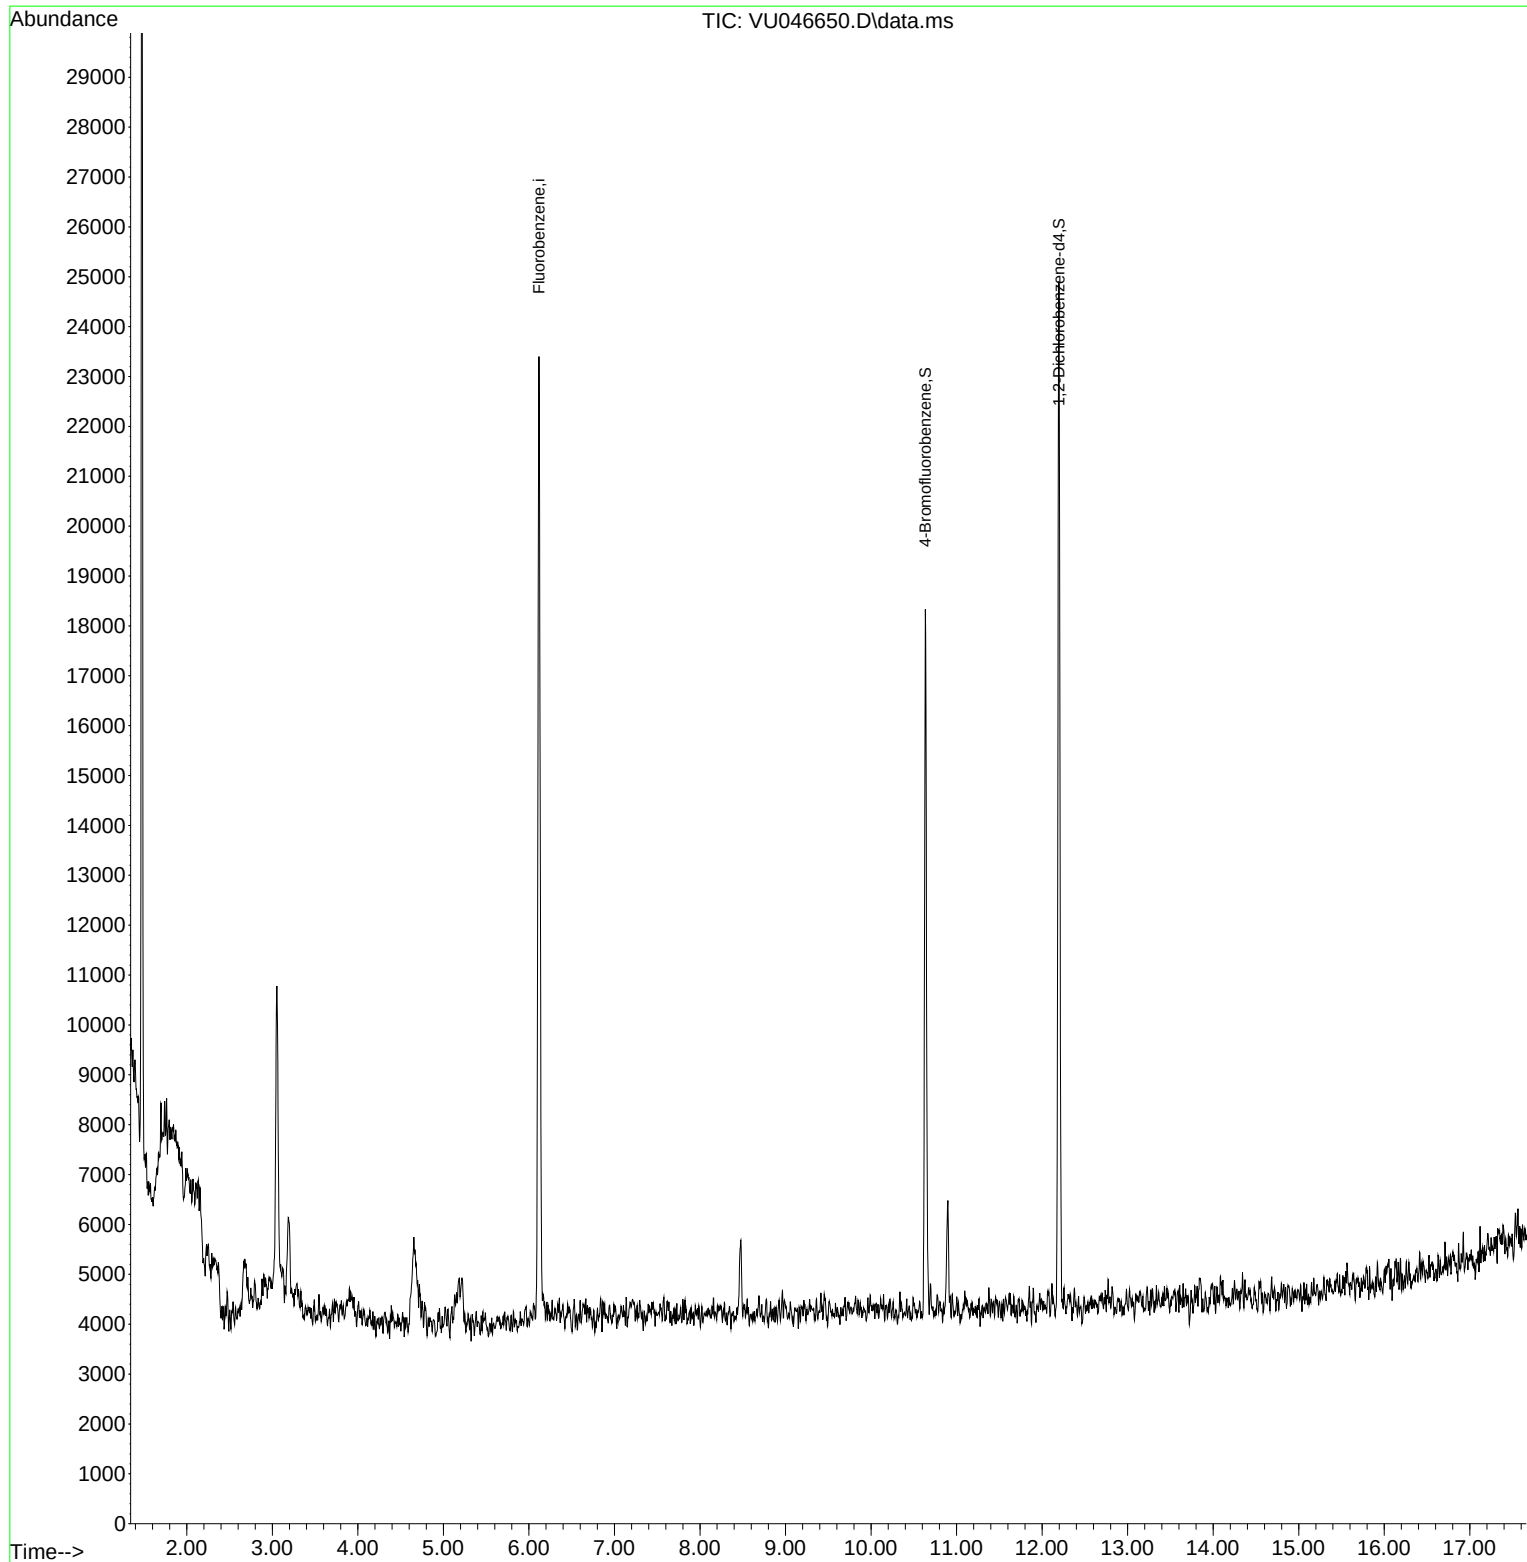


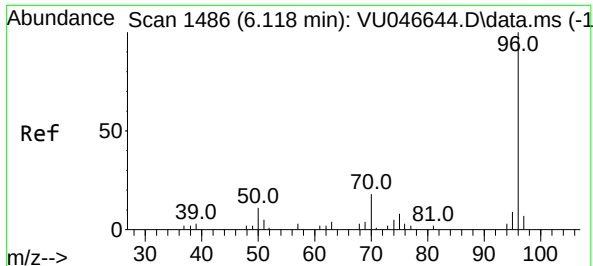

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. -0.000 min
Lab File: VU046650.D
Acq: 30 Dec 2021 15:48




Instrument :
MSVOA_U
ClientSampleId :
TB-01-122221


Tgt Ion: 96	Resp: 18273
Ion Ratio	Lower Upper
96 100	
70 20.0	16.8 25.2
95 8.7	7.3 10.9
97 6.7	0.0 0.0#

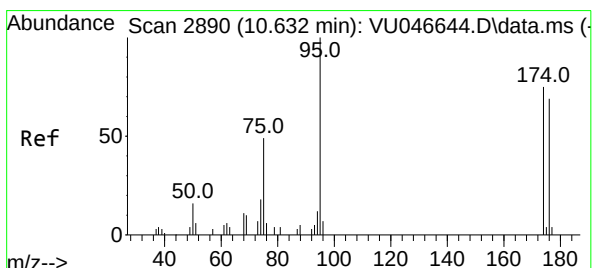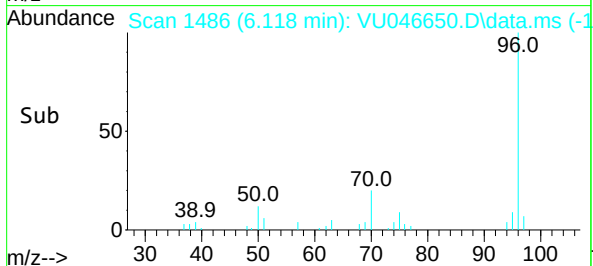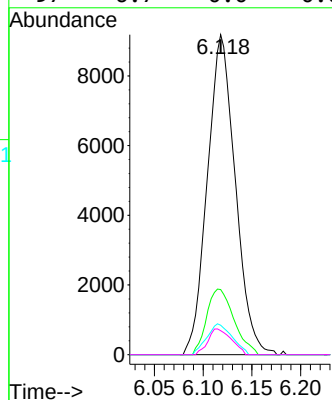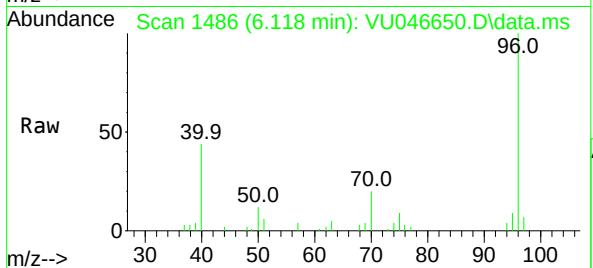

#57
4-Bromofluorobenzene
Concen: 0.783 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU046650.D
Acq: 30 Dec 2021 15:48


Tgt Ion: 95	Resp: 5089
Ion Ratio	Lower Upper
95 100	
174 81.6	56.6 84.8
176 74.4	54.3 81.5

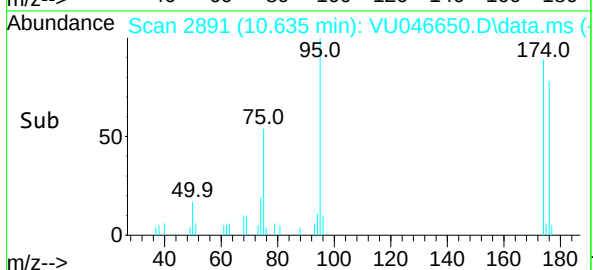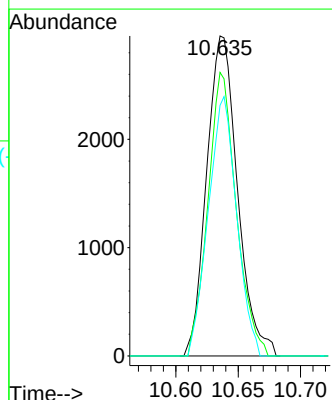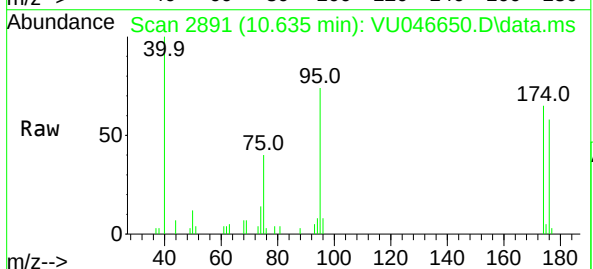

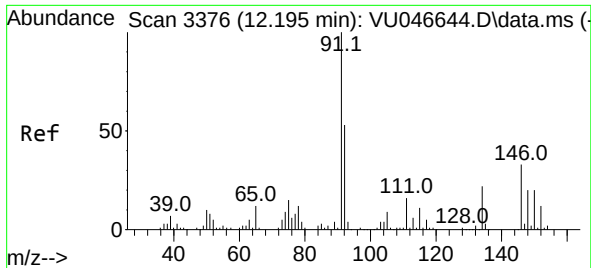

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.854 ug/l
 RT: 12.198 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU046650.D
 Acq: 30 Dec 2021 15:48

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-01-122221

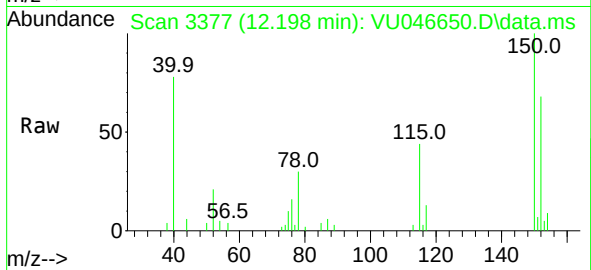

Tgt Ion:152	Resp:	6011
Ion	Ratio	Lower Upper
152	100	
115	63.5	0.0 251.0
150	150.7	0.0 613.8

