
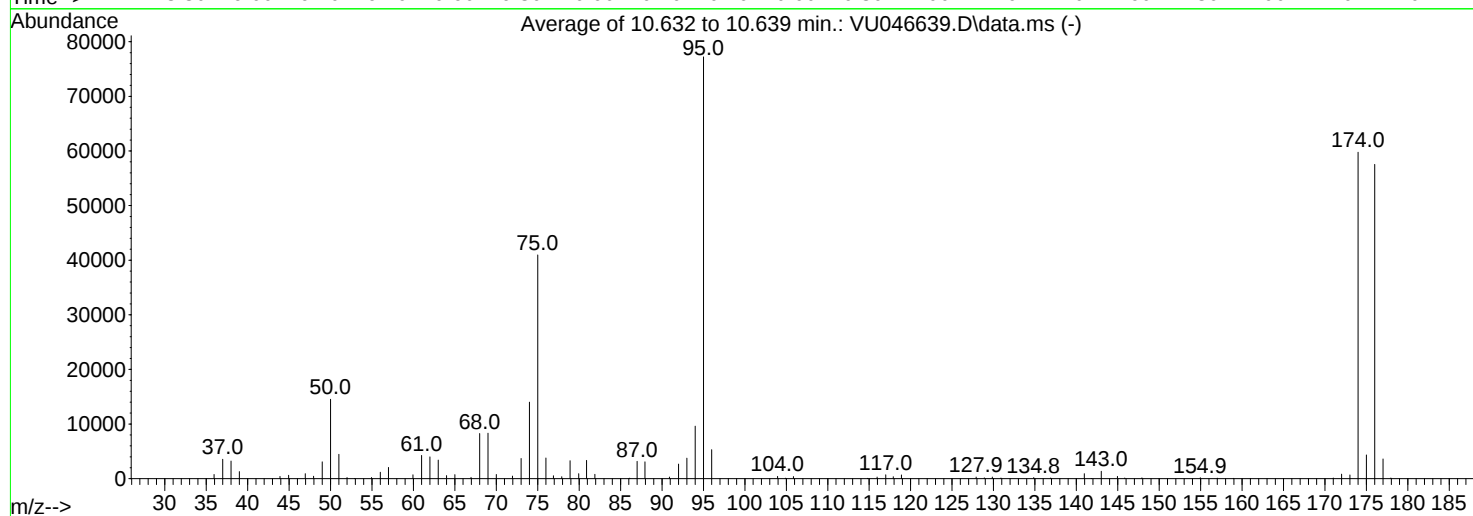


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123021\
 Data File : VU046639.D
 Acq On : 30 Dec 2021 08:03
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U123021DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Dec 30 12:44:59 2021

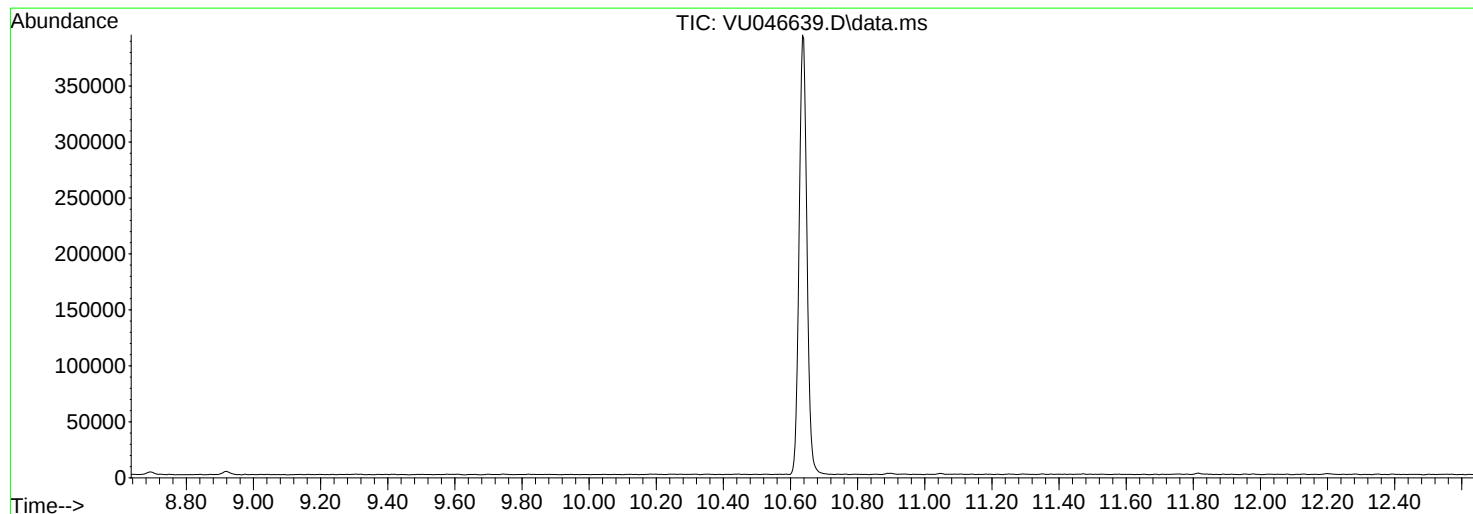

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	14537	PASS
75	95	30	60	53.0	40957	PASS
95	95	100	100	100.0	77235	PASS
96	95	5	9	6.9	5319	PASS
173	174	0.00	2	1.2	690	PASS
174	95	50	100	77.4	59765	PASS
175	174	5	9	7.2	4328	PASS
176	174	95	101	96.3	57555	PASS
177	176	5	9	6.3	3614	PASS