


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011922\
 Data File : VU046791.D
 Acq On : 19 Jan 2022 09:08
 Operator : SY/MD
 Sample : BFB099
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB099

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jan 20 02:00:32 2022

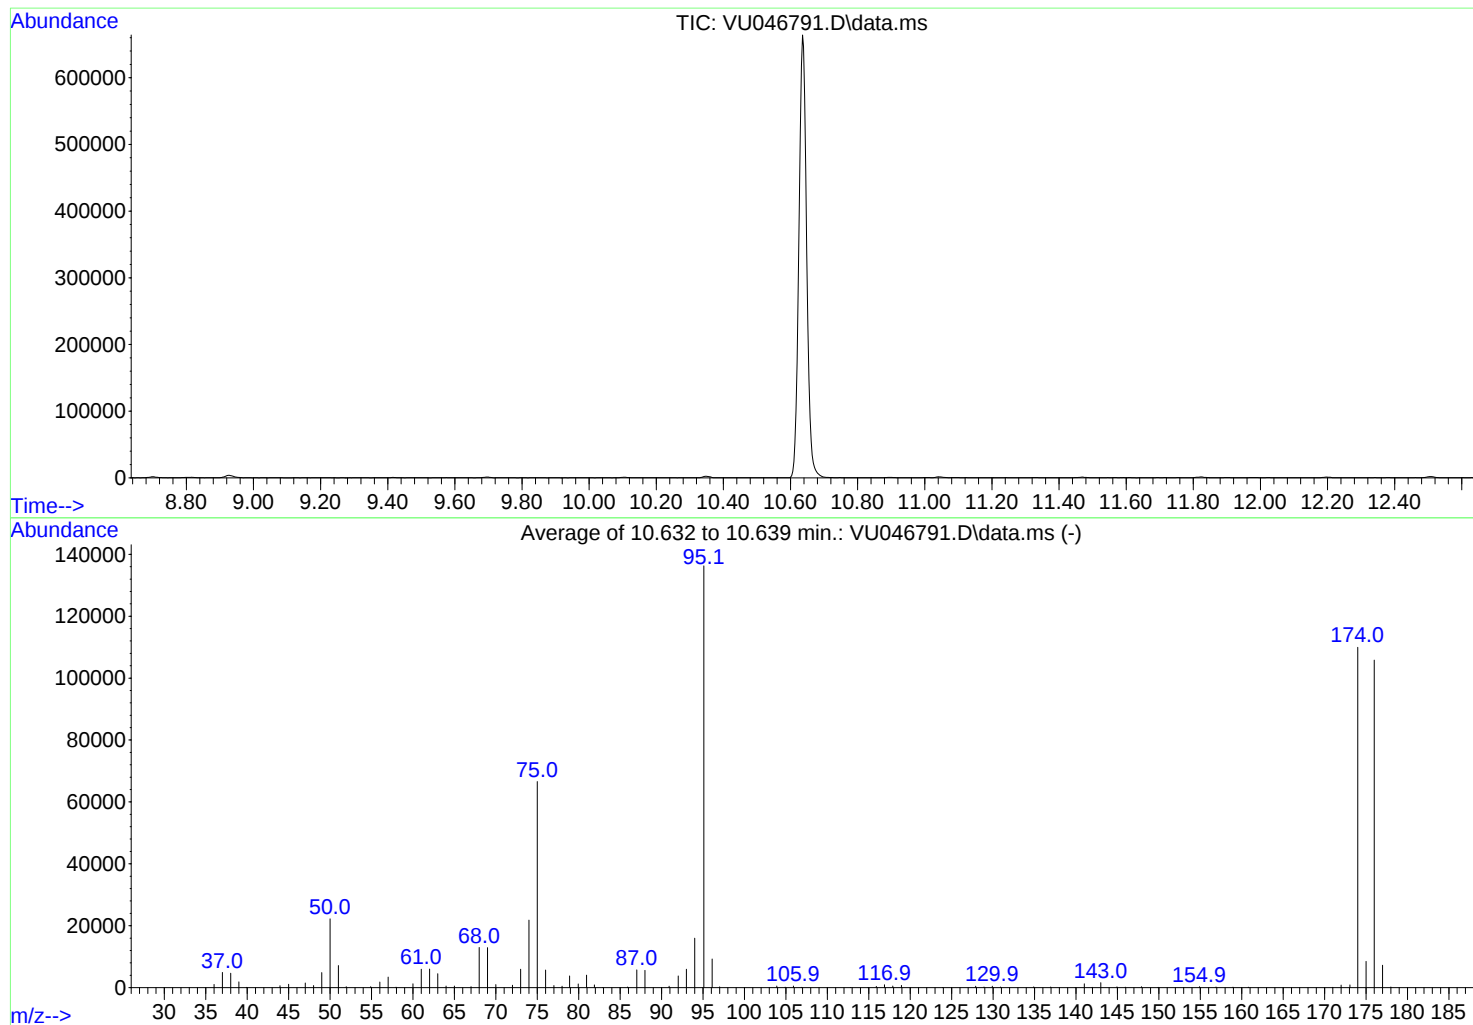

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	22240	PASS
75	95	30	80	48.8	66571	PASS
95	95	100	100	100.0	136277	PASS
96	95	5	9	6.8	9237	PASS
173	174	0.00	2	0.8	877	PASS
174	95	50	120	80.7	109973	PASS
175	174	5	9	7.7	8508	PASS
176	174	95	101	96.2	105845	PASS
177	176	5	9	6.8	7223	PASS

m/z	Abundance
43.90	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
36.00	1052.0
37.00	4797.0
38.00	4598.0
39.00	1761.0
39.90	126.0
44.00	733.0
45.00	1071.0
47.00	1552.0
48.00	704.0
49.00	4800.0
50.00	21704.0
51.00	7173.0
51.90	285.0
54.90	326.0
56.00	1733.0
57.00	3345.0
58.00	192.0
60.00	1259.0
61.00	5800.0
62.00	5869.0
63.00	4434.0
64.00	601.0
65.00	563.0
67.00	307.0
68.00	12678.0
69.00	12705.0
70.00	1026.0
72.00	808.0
73.00	5643.0
74.00	21208.0
75.00	64928.0
76.00	5710.0
77.00	710.0
78.00	541.0
78.90	3623.0
79.90	1166.0
81.00	3850.0
81.90	839.0
85.90	146.0
87.00	5664.0
88.00	5390.0
90.90	459.0
92.00	3716.0
93.00	5732.0
94.00	15433.0
95.10	131072.0
96.10	8938.0
97.00	244.0
103.90	544.0
104.90	158.0
105.90	488.0
106.80	113.0
112.80	110.0
114.90	120.0
115.90	413.0
116.90	887.0
117.90	448.0
118.90	703.0
127.90	405.0
128.90	236.0
129.90	458.0
130.90	206.0
134.90	276.0
136.90	245.0
141.00	1055.0
141.90	147.0
143.00	1572.0
144.90	299.0
145.90	179.0
147.90	301.0
149.90	123.0
154.90	315.0
156.90	180.0
159.00	129.0
160.80	140.0
171.00	109.0
172.00	894.0
173.00	861.0
174.00	103896.0
175.00	8255.0
176.00	99112.0
177.00	7019.0
178.00	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
36.00	1063.0
37.00	5052.0
38.00	4791.0
39.00	1914.0
39.90	108.0
44.00	797.0
45.00	1102.0
47.00	1531.0
48.00	721.0
49.00	5011.0
50.00	22928.0
51.00	7467.0
51.90	312.0
54.90	313.0
56.00	1868.0
57.00	3524.0
58.00	169.0
60.00	1355.0
61.00	6135.0
62.00	6220.0
63.00	4669.0
64.00	529.0
65.00	547.0
67.00	340.0
68.00	13348.0
69.00	13338.0
70.00	1032.0
72.00	827.0
73.00	6186.0
74.00	22584.0
75.00	68672.0
76.00	5910.0
77.00	708.0
78.00	496.0
78.90	3873.0
80.00	1243.0
81.00	4173.0
81.90	916.0
85.90	205.0
87.00	5890.0
88.00	5733.0
90.90	488.0
92.00	3896.0
93.00	6159.0
94.00	16488.0
95.10	140992.0
96.10	9547.0
97.00	260.0
103.90	526.0
104.90	167.0
105.90	578.0
106.90	116.0
112.80	101.0
114.90	114.0
115.90	432.0
116.90	966.0
117.90	514.0
118.90	733.0
127.90	472.0
128.90	217.0
129.90	504.0
130.90	218.0
134.90	288.0
136.90	226.0
139.90	115.0
141.00	1312.0
142.00	128.0
143.00	1664.0
145.00	280.0
146.00	179.0
147.90	323.0
149.90	138.0
153.00	109.0
154.90	314.0
156.90	209.0
158.90	168.0
160.80	183.0
171.00	112.0
172.00	828.0
173.00	921.0
174.00	113656.0
175.00	8858.0
176.00	109144.0
177.00	7475.0
178.00	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
36.00	955.0
37.00	4836.0
38.00	4557.0
39.00	1890.0
39.90	100.0
44.00	770.0
45.00	1047.0
47.00	1390.0
48.00	675.0
49.00	4844.0
50.00	22088.0
51.00	6856.0
52.00	288.0
54.90	301.0
56.00	1850.0
57.00	3427.0
57.90	125.0
60.00	1189.0
61.00	5967.0
62.00	5965.0
63.00	4431.0
64.00	506.0
65.00	490.0
67.00	330.0
68.00	12834.0
69.00	12713.0
70.00	913.0
72.00	740.0
73.00	6062.0
74.00	21728.0
75.00	66112.0
76.00	5528.0
77.00	669.0
78.00	435.0
78.90	3816.0
80.00	1196.0
80.90	4097.0
81.90	901.0
82.90	114.0
85.90	215.0
87.00	5721.0
88.00	5565.0
90.90	475.0
92.00	3707.0
93.00	5957.0
94.00	16031.0
95.10	136768.0
96.10	9227.0
97.00	237.0
103.90	497.0
104.90	150.0
105.90	560.0
106.90	103.0
115.90	438.0
116.90	976.0
117.90	534.0
119.00	753.0
123.90	108.0
127.90	496.0
128.90	187.0
129.90	481.0
130.90	213.0
134.90	246.0
137.00	223.0
139.90	123.0
141.00	1406.0
142.00	112.0
143.00	1601.0
145.00	251.0
146.00	192.0
147.90	315.0
149.90	121.0
154.90	278.0
156.90	212.0
158.90	183.0
160.80	184.0
171.00	105.0
172.00	706.0
173.10	848.0
174.00	112368.0
175.00	8411.0
176.00	109280.0
177.00	7175.0
178.00	229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099