


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046844.D
Acq On : 26 Jan 2022 14:36
Operator : SY/MD
Sample : N1260-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX3

Manual IntegrationsAPPROVED

Quant Time: Jan 26 15:23:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 24 00:23:26 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2022
Supervised By :Mahesh Dadoda 01/27/2022

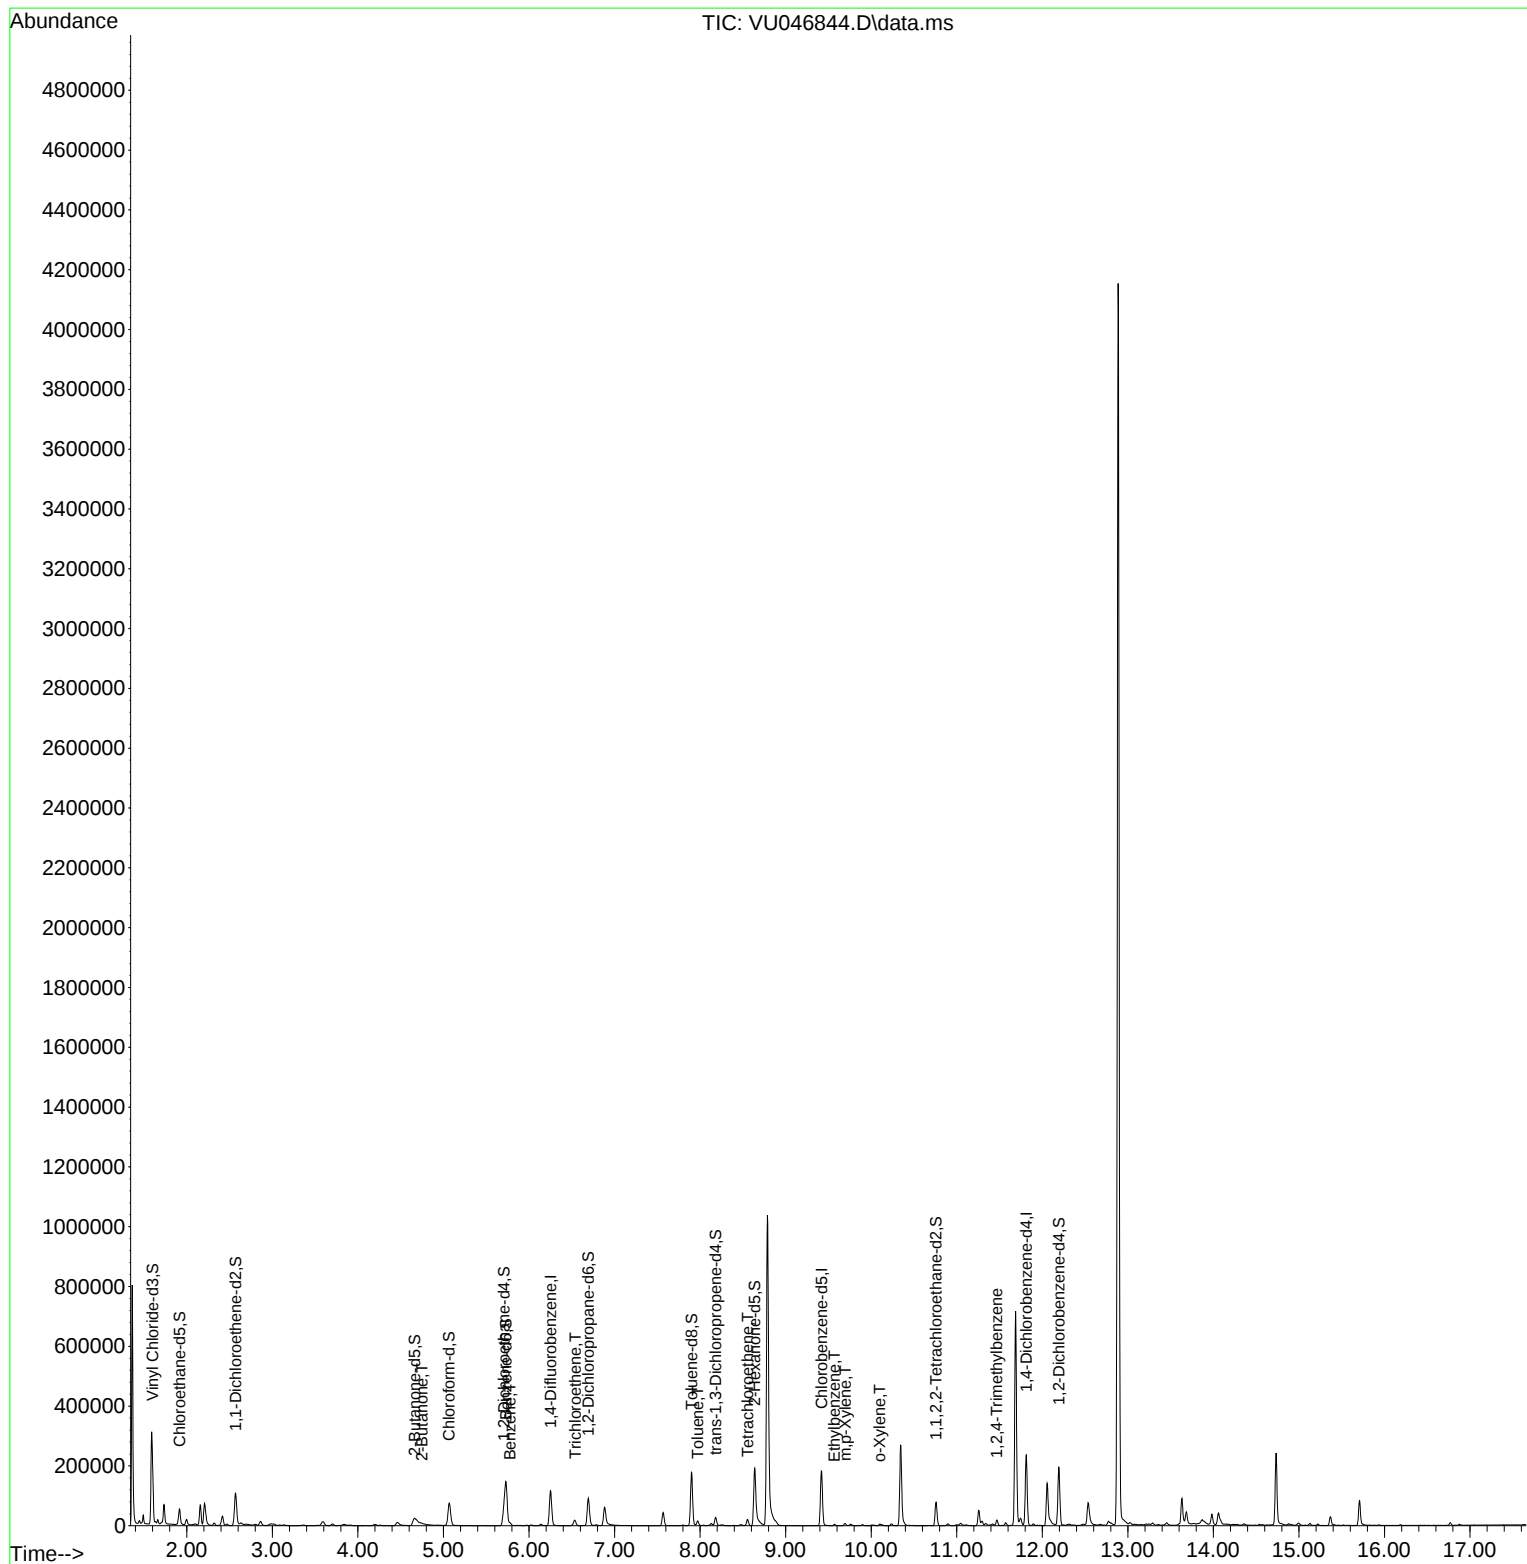




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046844.D
 Acq On : 26 Jan 2022 14:36
 Operator : SY/MD
 Sample : N1260-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX3

Manual IntegrationsAPPROVED

Quant Time: Jan 26 15:23:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 24 00:23:26 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2022
 Supervised By :Mahesh Dadoda 01/27/2022

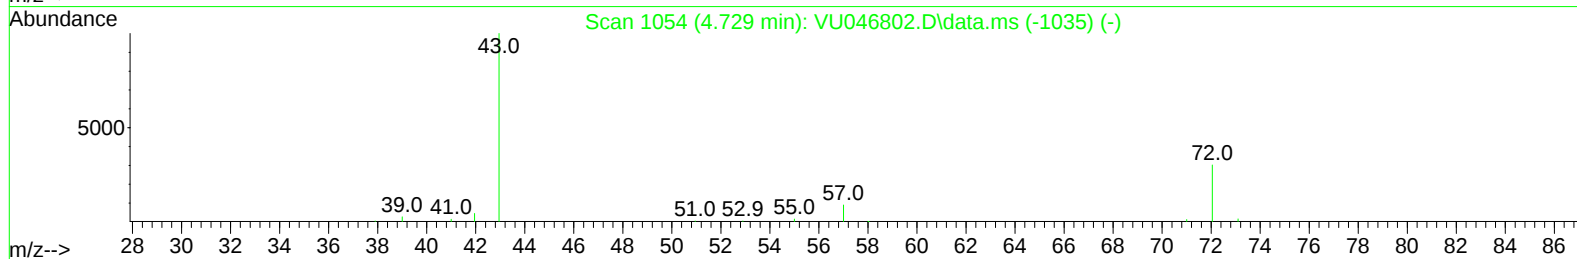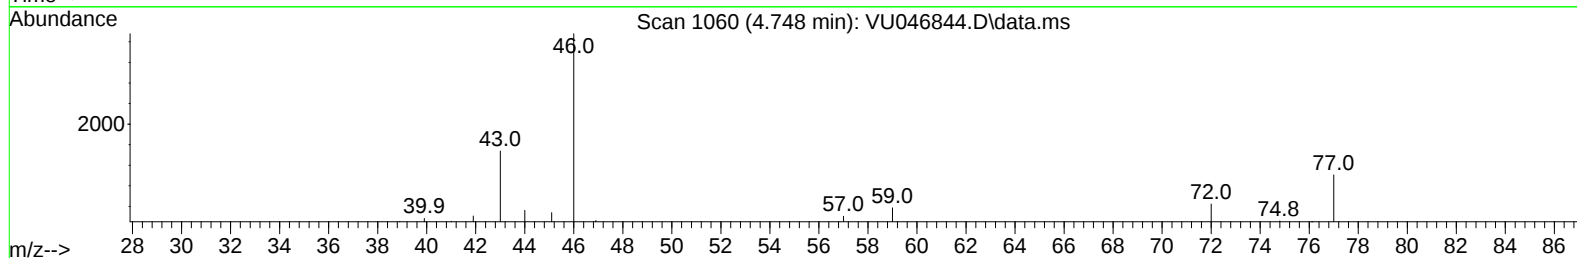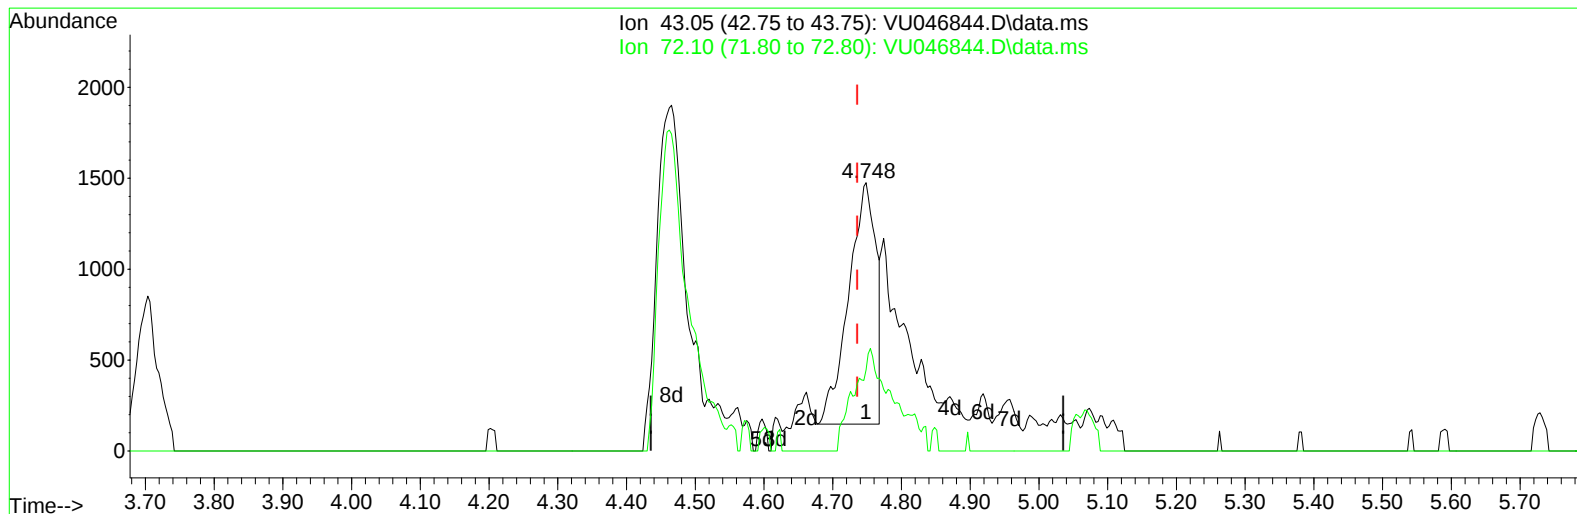

TIC: VU046844.D\data.ms

(21) 2-Butanone (T)

4.748min (+ 0.013) 1.72 ug/L

response 3657

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.20	53.51#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046844.D
 Acq On : 26 Jan 2022 14:36
 Operator : SY/MD
 Sample : N1260-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX3

Manual IntegrationsAPPROVED

Quant Time: Jan 26 15:23:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 24 00:23:26 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2022
 Supervised By :Mahesh Dadoda 01/27/2022

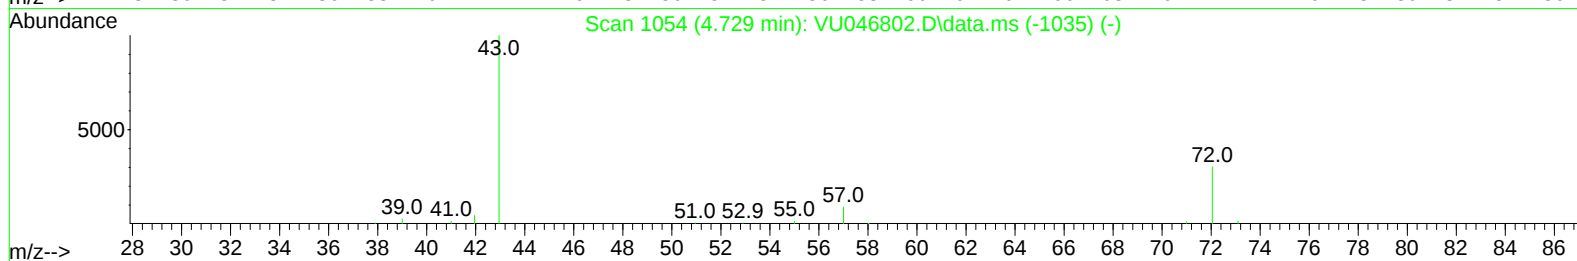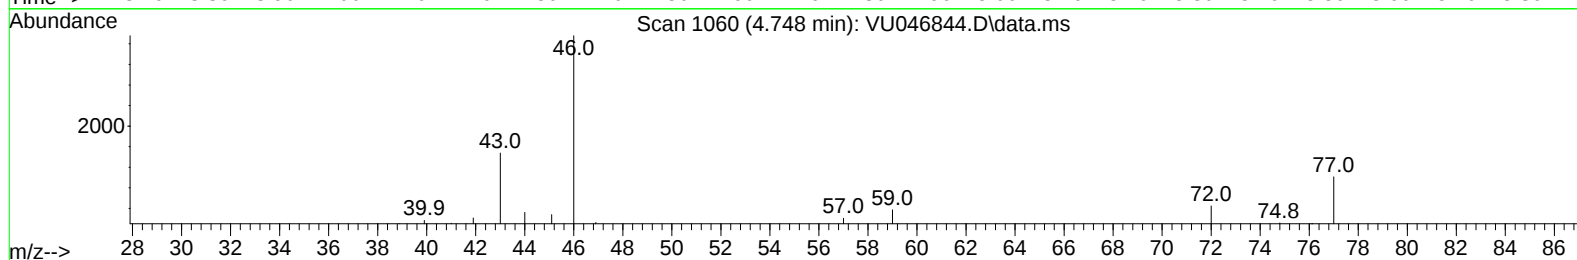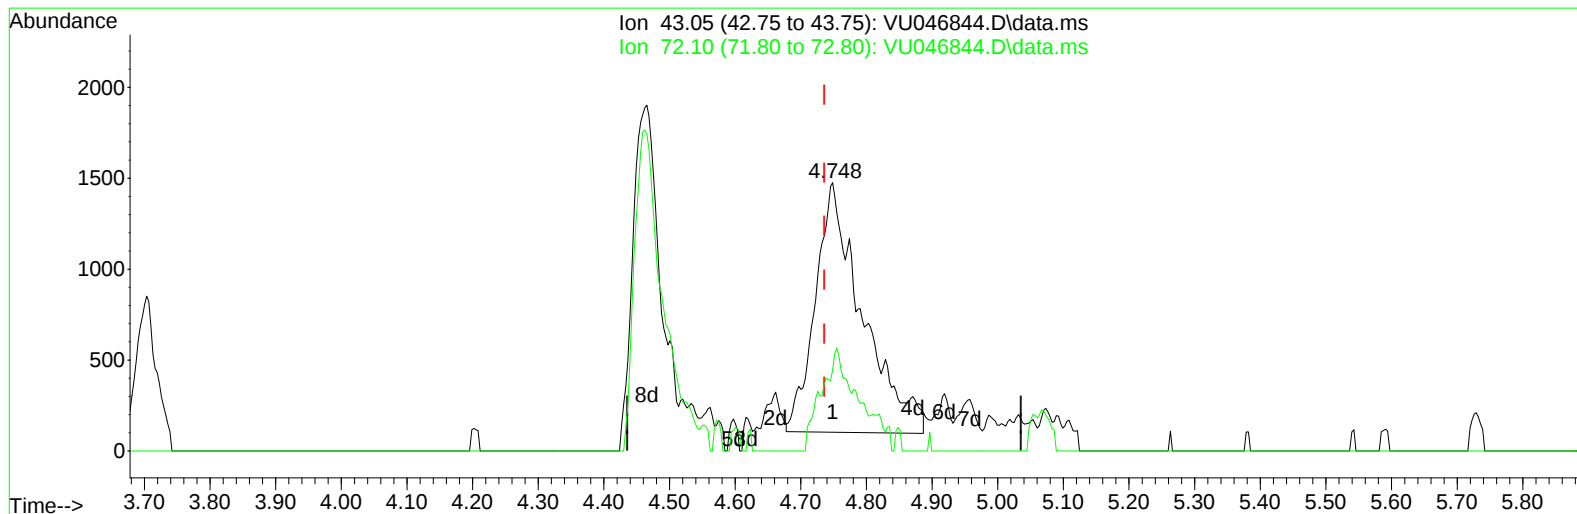

TIC: VU046844.D\data.ms

(21) 2-Butanone (T)

4.748min (+ 0.013) 3.21 ug/L m

response 6830

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.20	28.65
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046844.D
 Acq On : 26 Jan 2022 14:36
 Operator : SY/MD
 Sample : N1260-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXX3

Manual IntegrationsAPPROVED

Quant Time: Jan 26 15:23:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 24 00:23:26 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2022
 Supervised By :Mahesh Dadoda 01/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	96794	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	105395	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	62724	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	36026	4.392	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.800%	
7) Chloroethane-d5	1.916	69	32257	4.992	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.800%	
11) 1,1-Dichloroethene-d2	2.572	65	15182	4.653	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.000%	
20) 2-Butanone-d5	4.665	46	75677	31.145	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	62.300%	
24) Chloroform-d	5.067	84	72434	5.031	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.707	65	39282	5.010	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.732	84	140677	4.541	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	6.694	67	44688	4.805	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.899	98	120056	4.234	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	8.182	79	16729	4.096	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.639	63	84288	34.852	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	69.700%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	39482	4.228	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.600%	
66) 1,2-Dichlorobenzene-d4	12.195	152	50220	4.269	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	85.400%	
Target Compounds					Qvalue	
21) 2-Butanone	4.748	43	6830m	3.214	ug/L	
33) Benzene	5.777	78	7661	0.309	ug/L	100
34) Trichloroethene	6.543	95	2337	0.363	ug/L	# 69
42) Toluene	7.970	91	11109	0.375	ug/L	100
47) Tetrachloroethene	8.555	164	3932	0.750	ug/L	94
52) Ethylbenzene	9.568	91	3370	0.120	ug/L	95
53) m,p-Xylene	9.697	106	2371	0.211	ug/L	95
54) o-Xylene	10.099	106	1283	0.118	ug/L	81
63) 1,2,4-Trimethylbenzene	11.468	105	6977	0.283	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed