

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046840.D
 Acq On : 26 Jan 2022 12:57
 Operator : SY/MD
 Sample : N1260-01 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXX3

Quant Time: Jan 26 14:51:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 24 00:23:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	99022	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	110727	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	49592	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	38614	4.602	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.000%
7) Chloroethane-d5	1.919	69	33567	5.077	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.600%
11) 1,1-Dichloroethene-d2	2.575	65	16865	5.053	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.000%
20) 2-Butanone-d5	4.652	46	109302	43.971	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.940%
24) Chloroform-d	5.070	84	75416	5.120	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	5.706	65	43428	5.414	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
32) Benzene-d6	5.732	84	146049	4.488	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
36) 1,2-Dichloropropane-d6	6.693	67	46422	4.751	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.899	98	118582	3.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.182	79	16683	3.888	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.800%
46) 2-Hexanone-d5	8.639	63	101066	39.777	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.560%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	42897	4.373	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	44786	4.816	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						
					Qvalue	
38) Bromodichloromethane	7.108	83	438	0.048	ug/L	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046840.D
Acq On : 26 Jan 2022 12:57
Operator : SY/MD
Sample : N1260-01 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX3


Quant Time: Jan 26 14:51:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 24 00:23:26 2022
Response via : Initial Calibration

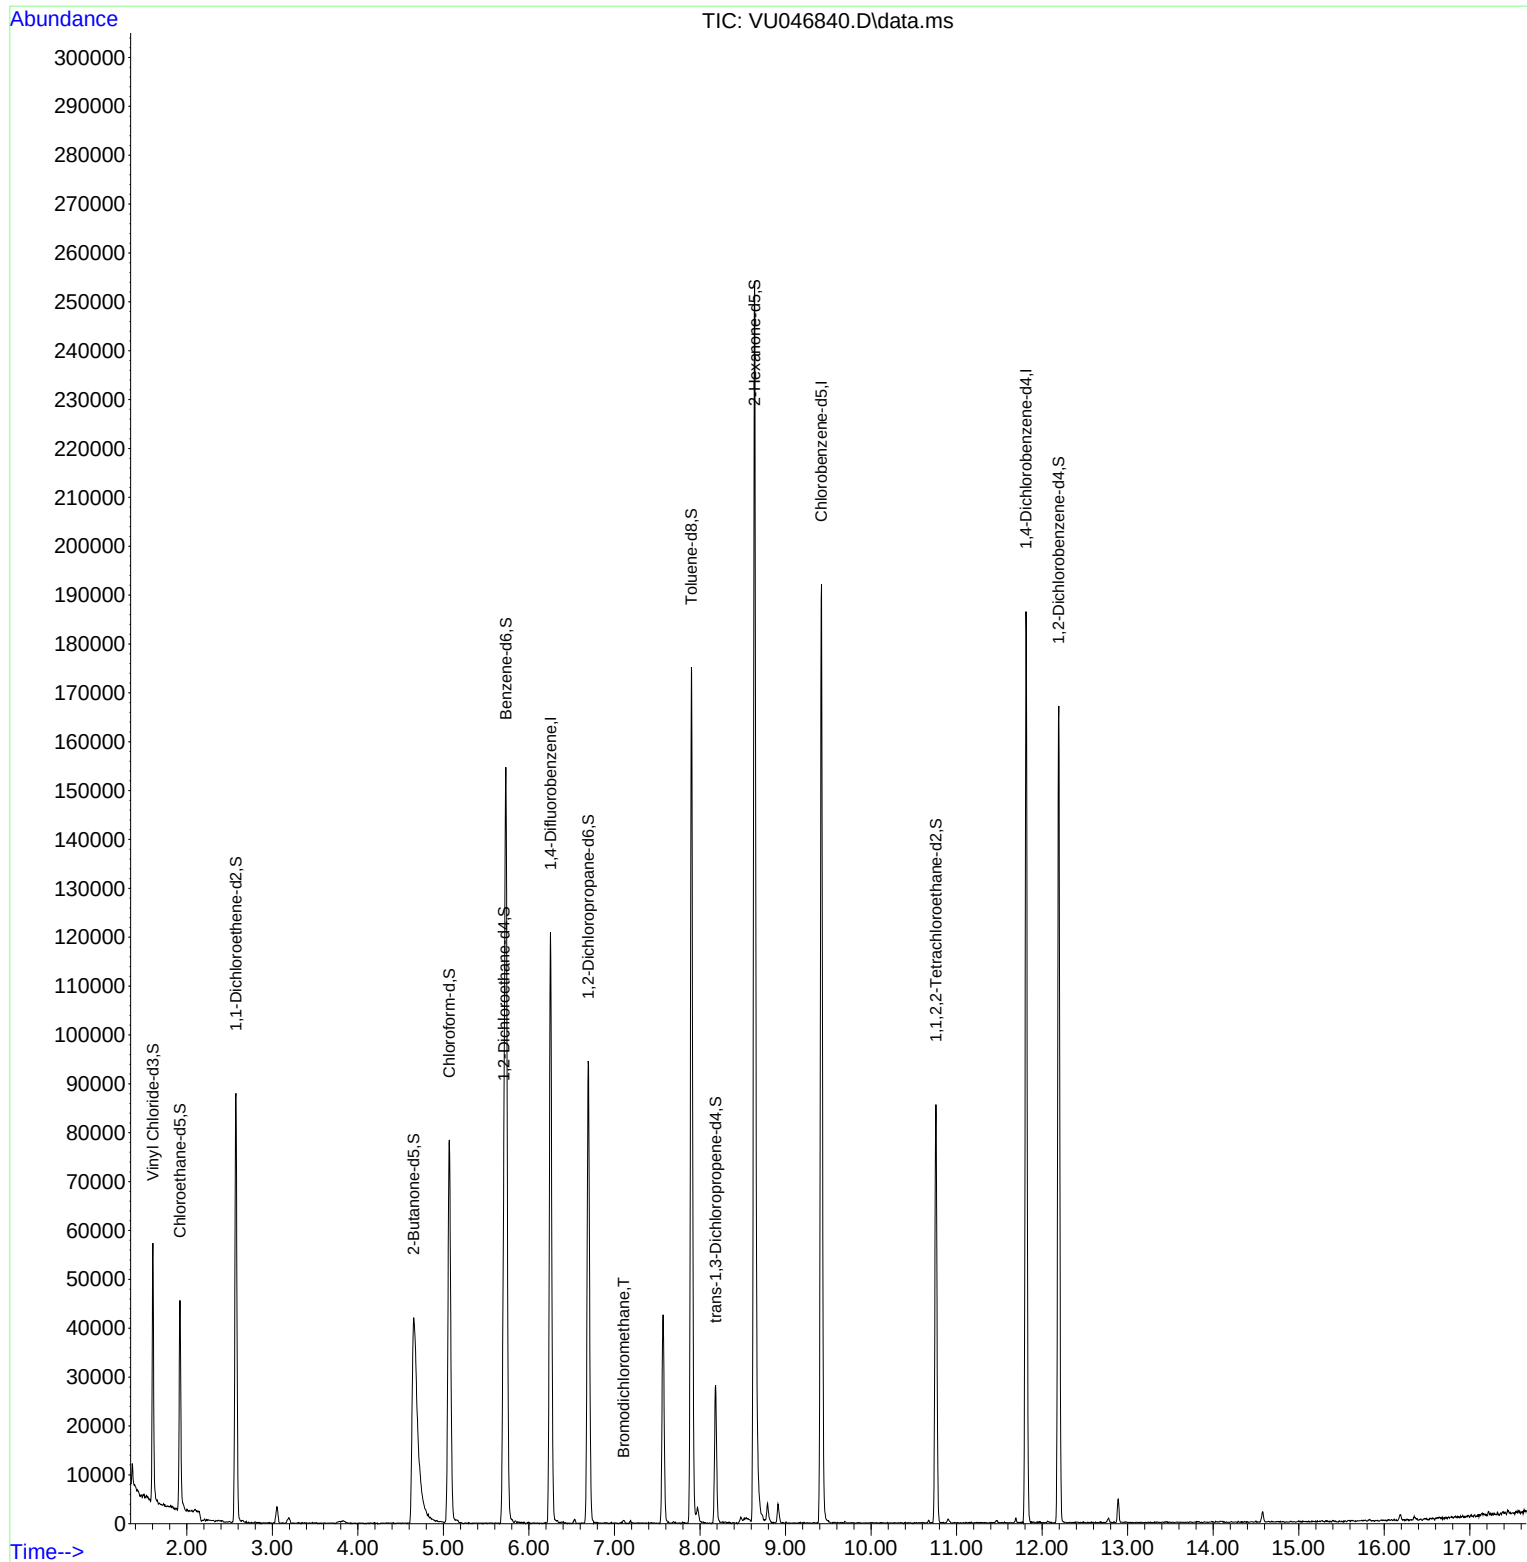

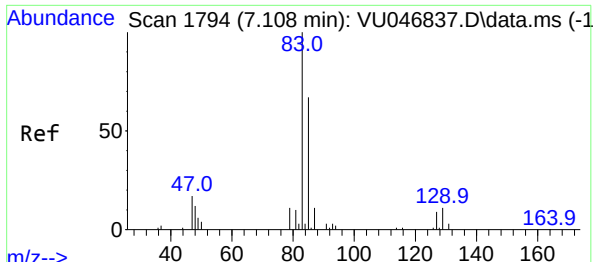

#38
 Bromodichloromethane
 Concen: 0.048 ug/L
 RT: 7.108 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VU046840.D
 Acq: 26 Jan 2022 12:57

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX3

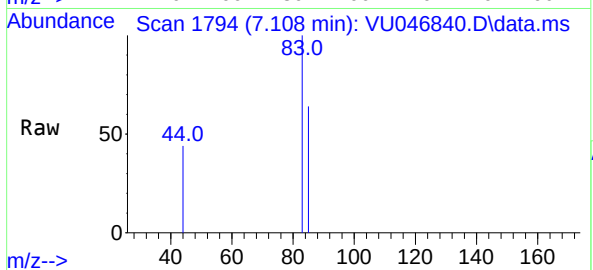

Tgt Ion: 83 Resp: 438
 Ion Ratio Lower Upper
 83 100
 85 64.1 44.0 81.8
 127 0.0 6.3 9.5#

