

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046856.D
 Acq On : 26 Jan 2022 19:54
 Operator : SY/MD
 Sample : N1277-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COVF0

Quant Time: Jan 27 00:16:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 00:12:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	98114	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	105819	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	47234	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	36296	4.366	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%
7) Chloroethane-d5	1.919	69	31207	4.764	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.575	65	15286	4.622	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.400%
20) 2-Butanone-d5	4.645	46	110338	44.799	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.600%
24) Chloroform-d	5.070	84	71626	4.908	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.706	65	39917	5.022	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.732	84	139119	4.473	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	6.693	67	44028	4.715	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.899	98	110719	3.889	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	8.182	79	16338	3.984	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.636	63	94445	38.895	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.800%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	39876	4.253	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.000%
66) 1,2-Dichlorobenzene-d4	12.195	152	42873	4.840	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds					Qvalue	
33) Benzene	5.784	78	2225	0.089	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046856.D
Acq On : 26 Jan 2022 19:54
Operator : SY/MD
Sample : N1277-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VF0

Quant Time: Jan 27 00:16:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 00:12:19 2022
Response via : Initial Calibration

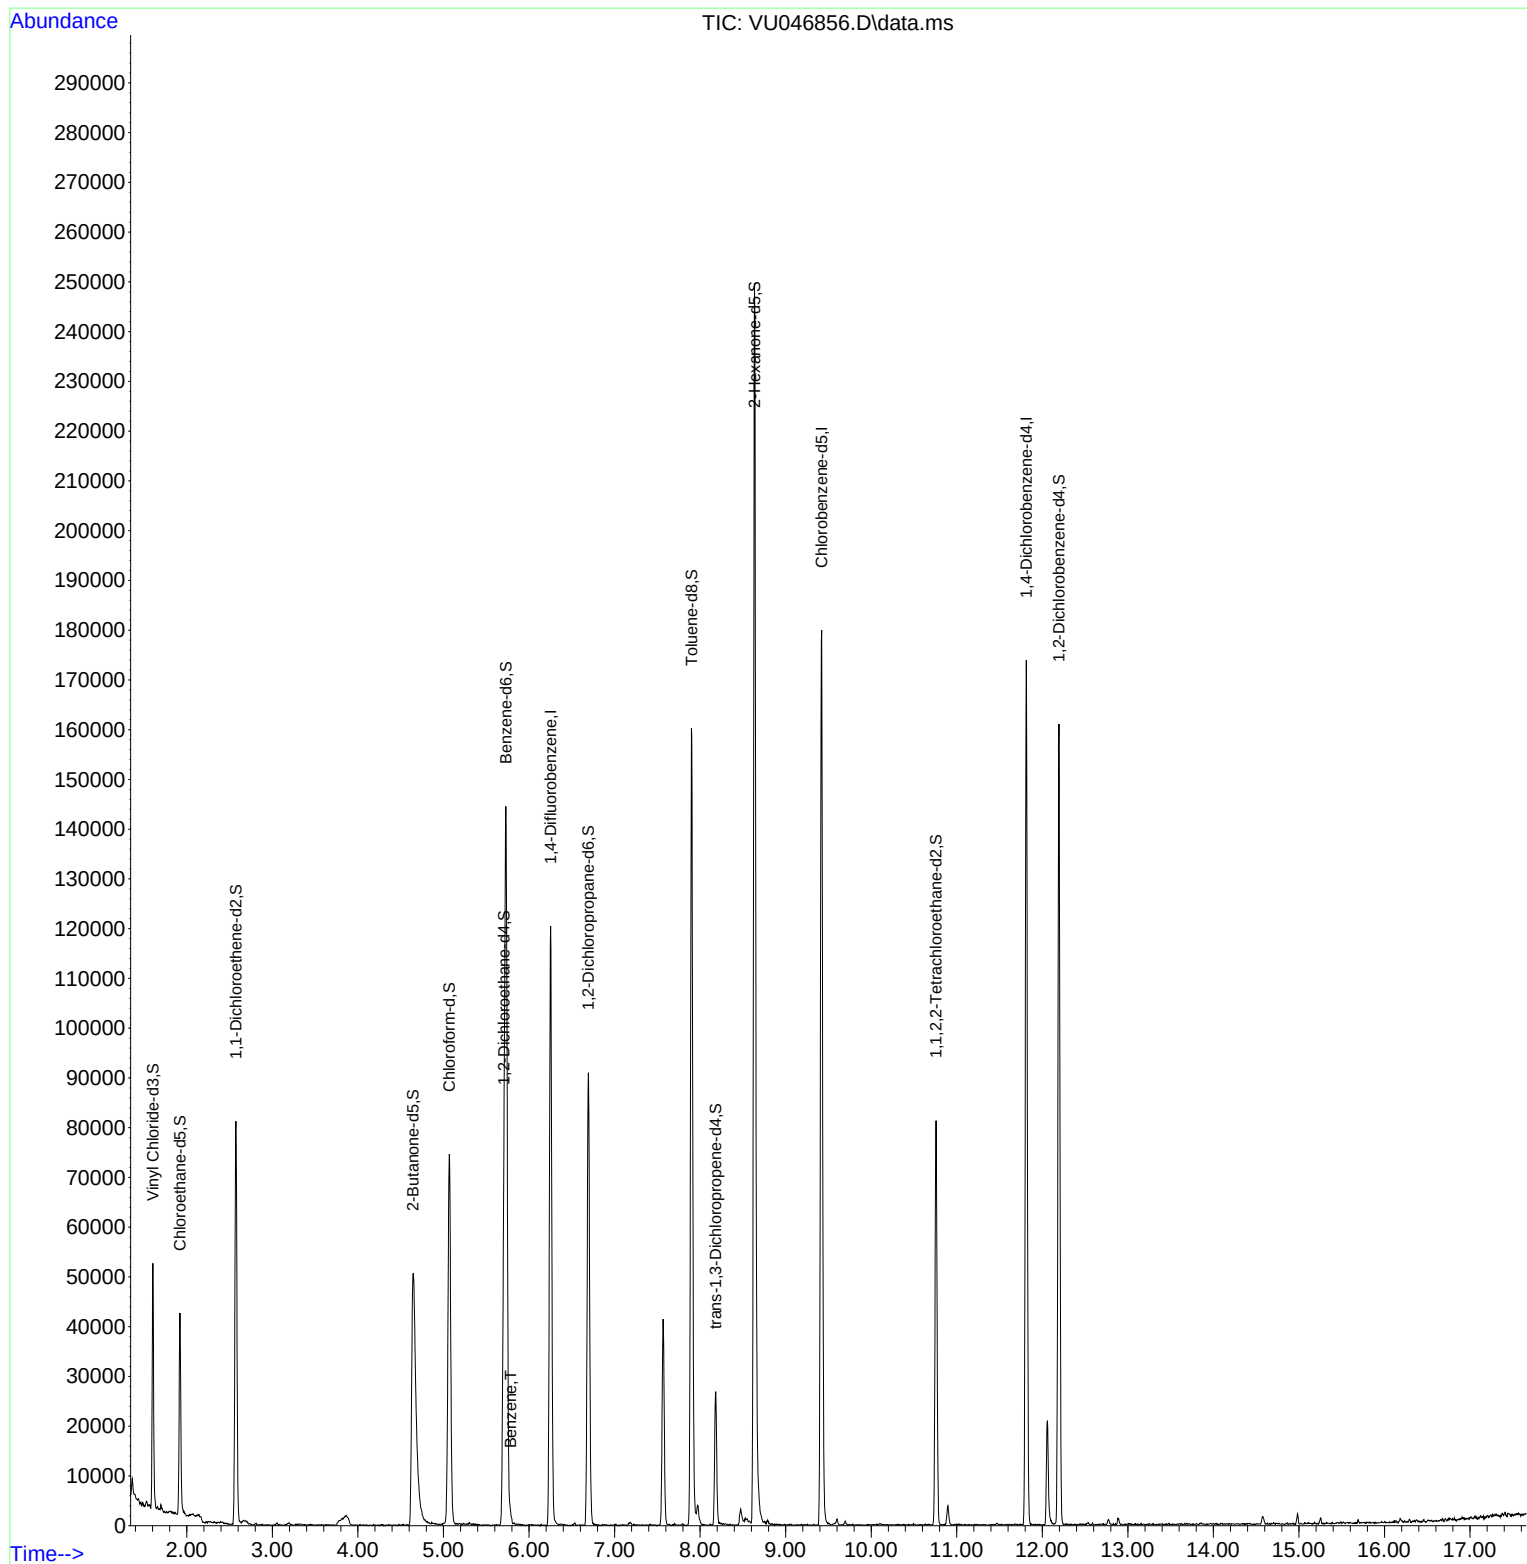

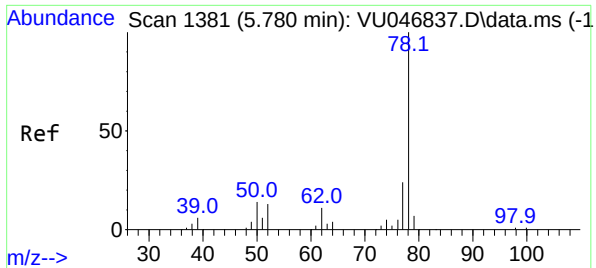

Benzene

Concen: 0.089 ug/L

RT: 5.784 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU046856.D

Acq: 26 Jan 2022 19:54

Instrument :

MSVOA_U

ClientSampleId :

C0VF0

Tgt Ion: 78 Resp: 2225

